

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
 Data File : BM010450.D
 Acq On : 09 Jun 2017 13:04
 Operator : SJ/MA
 Sample : I3521-12
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5B94

Manual Integrations
 APPROVED

mohammad
 6/12/2017 11:17:55 AM

Quant Time: Jun 10 02:05:42 2017
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 10 01:45:58 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	275948	20.00	ng/ul	0.00
18) Naphthalene-d8	10.71	136	1023877	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.54	164	693537	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.29	188	1574200	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	1686229	20.00	ng/ul	0.00
83) Perylene-d12	23.80	264	1644492	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.38	96	20154	3.00	ng/uL	0.00
5) Phenol-d5	7.09	99	325720	15.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.25	67	183267	15.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.45	132	286347	17.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.63	113	279167	16.55	ng/ul	0.00
19) Nitrobenzene-d5	9.09	128	136684	18.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.80	143	166663	19.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.33	165	336915	18.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.87	131	326631	18.97	ng/ul	0.00
43) Dimethylphthalate-d6	13.96	166	1120233	19.44	ng/ul	0.00
46) Acenaphthylene-d8	14.24	160	1244427	18.51	ng/ul	0.00
51) 4-Nitrophenol-d4	14.78	143	86796	10.07	ng/ul	0.00
57) Fluorene-d10	15.53	176	958898	18.93	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.66	200	143085	12.83	ng/ul	0.00
70) Anthracene-d10	17.39	188	1492791	19.49	ng/ul	0.00
76) Pyrene-d10	19.67	212	1717464	24.63	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.64	264	1565770	20.45	ng/ul	0.00

Target Compounds

					Qvalue	
44) Dimethylphthalate	14.00	163	1162832	20.520	ng/ul	99
74) Fluoranthene	19.34	202	865881	8.379	ng/ul#	95
77) Pyrene	19.70	202	834258	9.601	ng/ul#	94
80) Benzo(a)anthracene	21.44	228	705252	7.417	ng/ul	97
82) Chrysene	21.49	228	681044	7.923	ng/ul	96
85) Benzo(b)fluoranthene	23.08	252	989684	10.343	ng/ul	99
86) Benzo(k)fluoranthene	23.12	252	261038m	2.856	ng/ul	
88) Benzo(a)pyrene	23.69	252	412893	4.353	ng/ul	94
89) Indeno(1,2,3-cd)pyrene	26.18	276	310717	2.593	ng/ul#	94
91) Benzo(g,h,i)perylene	26.93	276	230515	2.335	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
Data File : BM010450.D
Acq On : 09 Jun 2017 13:04
Operator : SJ/MA
Sample : I3521-12
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
F5B94

Manual Integrations
APPROVED

mohammad
6/12/2017 11:17:55 AM

Quant Time: Jun 10 02:05:42 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 10 01:45:58 2017
Response via : Initial Calibration

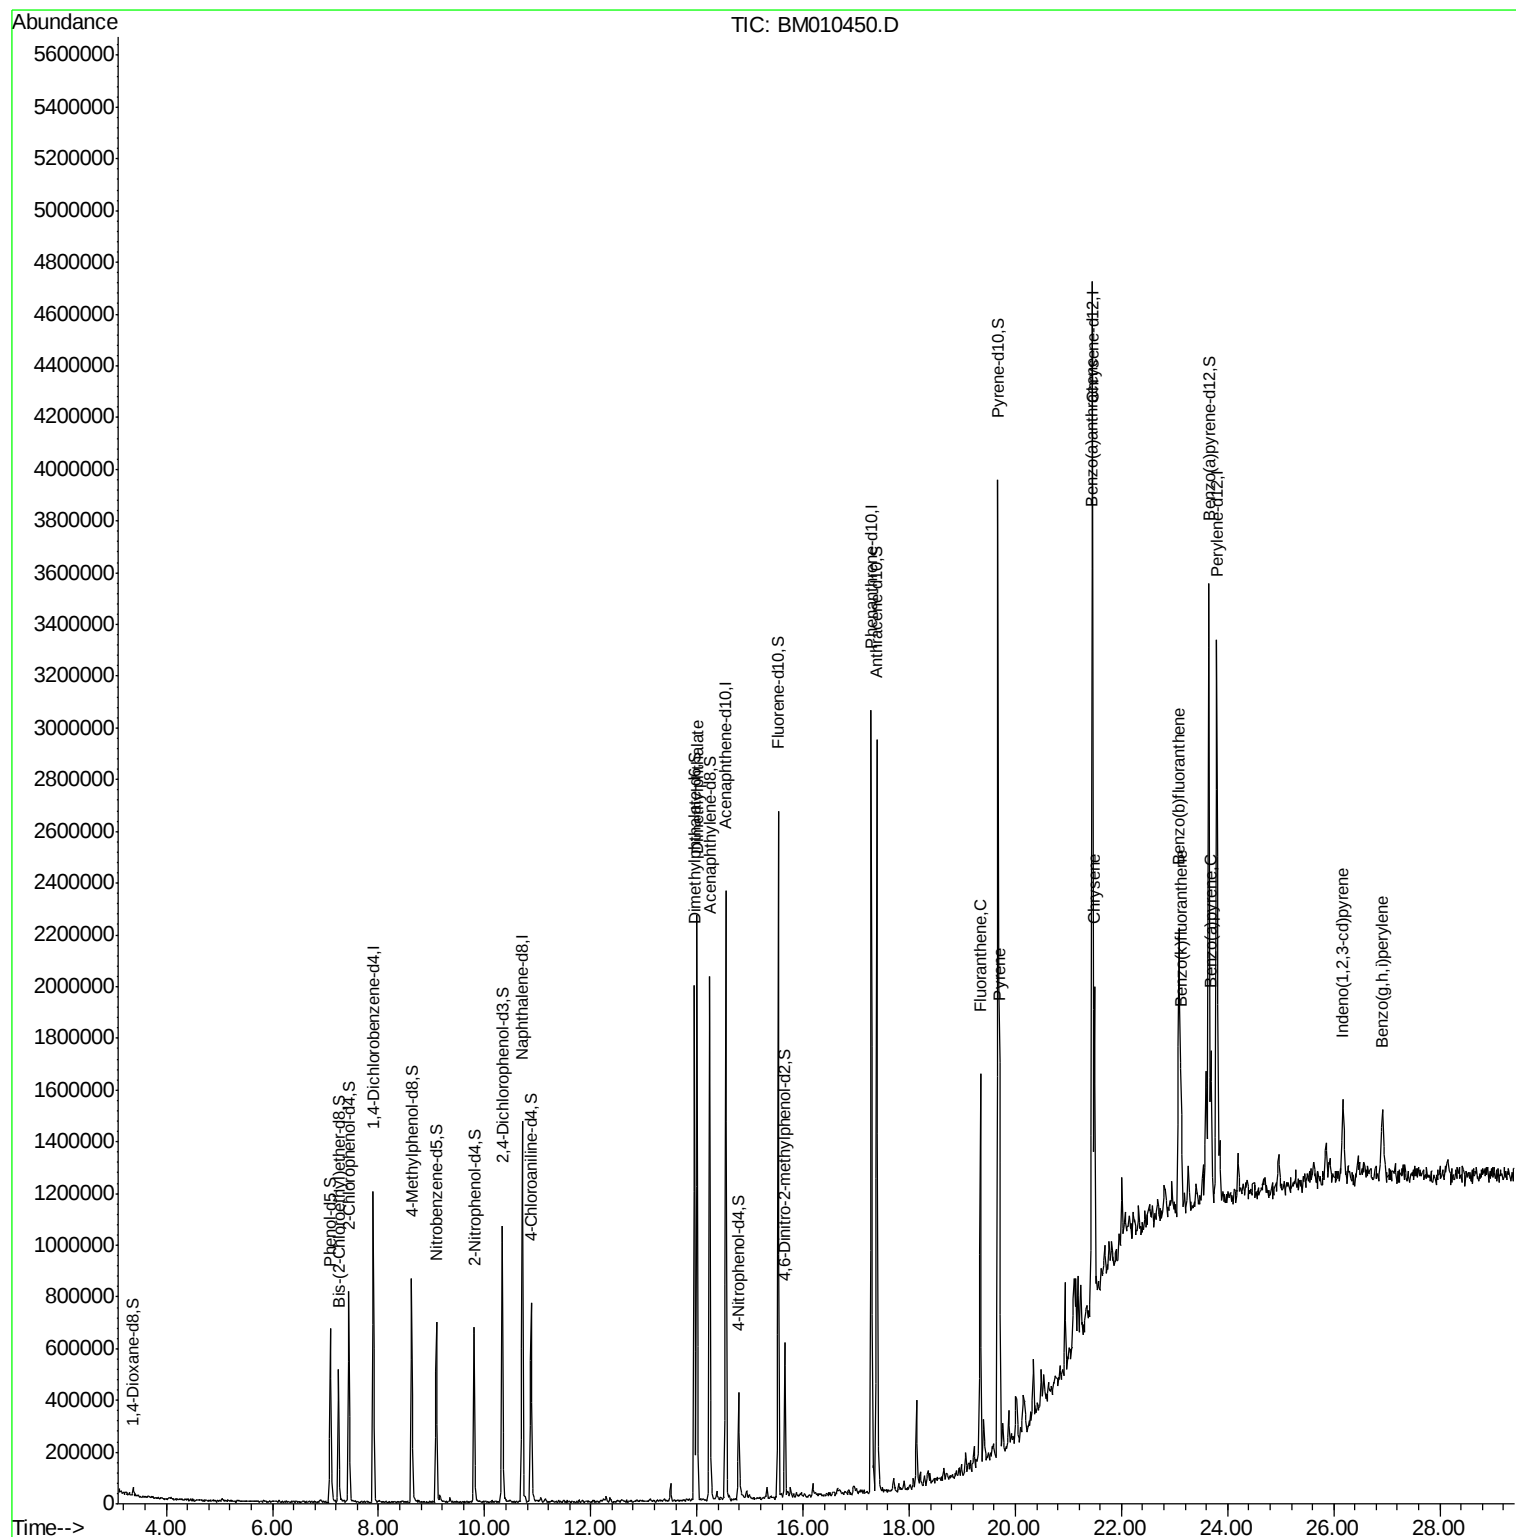

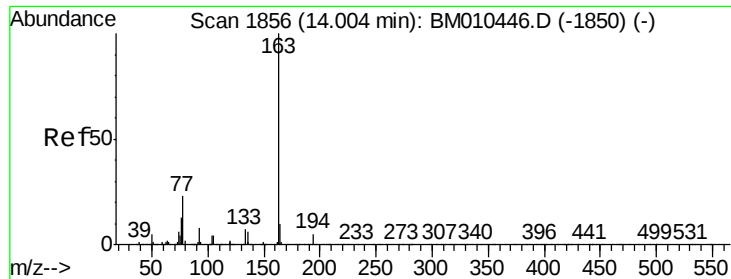





#44
Dimethylphthalate
Concen: 20.520 ng/ul
RT: 14.00 min Scan# 1856
Delta R.T. 0.00 min
Lab File: BM010450.D
Acq: 09 Jun 2017 13:04

Instrument :
BNA_M
ClientSampleId :
F5B94

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.5	3.5	5.3
164	10.9	8.2	12.4




Manual Integrations
APPROVED


mohammad
6/12/2017 11:17:55 AM

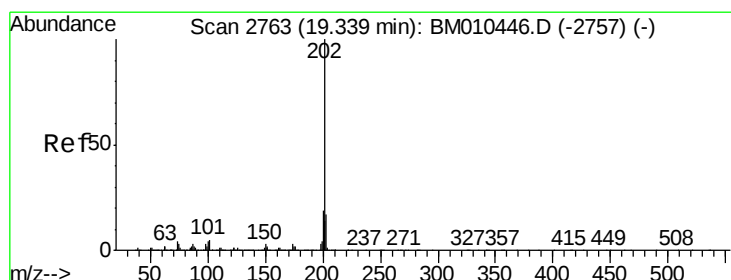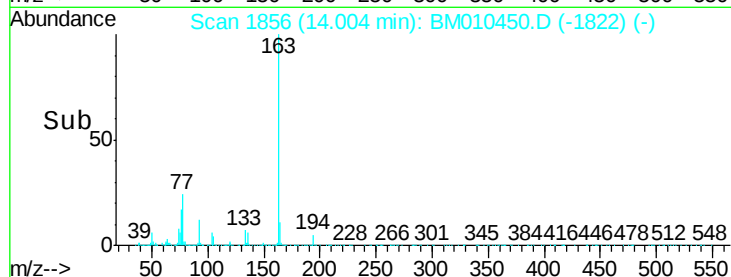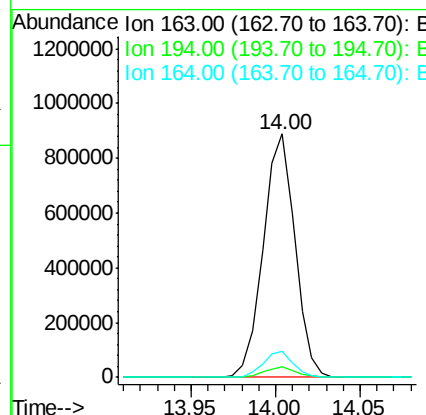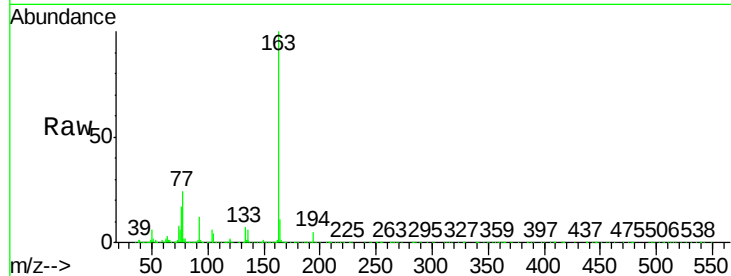

#74
Fluoranthene
Concen: 8.379 ng/ul
RT: 19.34 min Scan# 2763
Delta R.T. 0.00 min
Lab File: BM010450.D
Acq: 09 Jun 2017 13:04

Tgt Ion	Ratio	Lower	Upper
202	100		
101	3.9	4.6	7.0#
100	3.1	3.4	5.2#

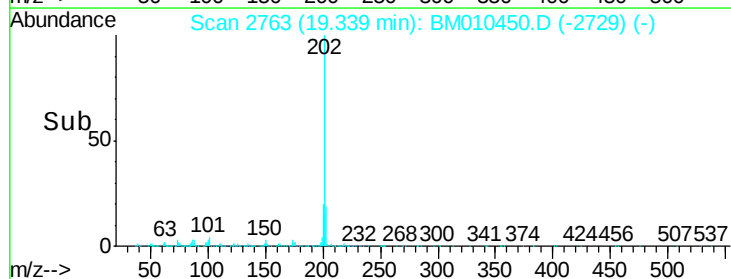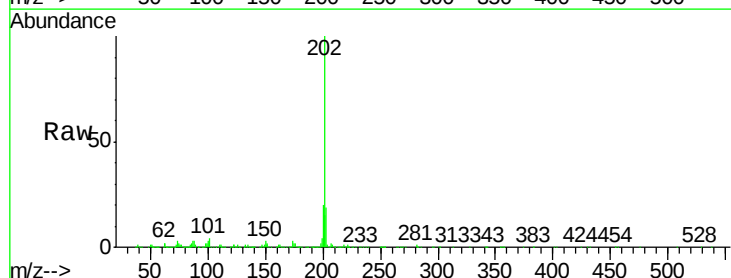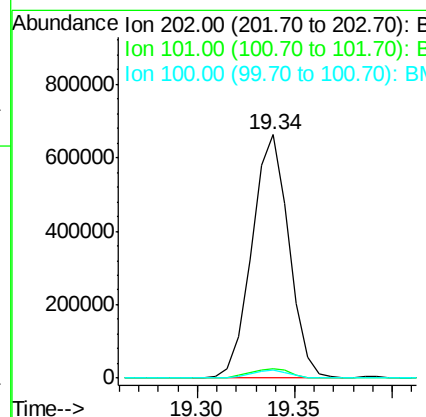

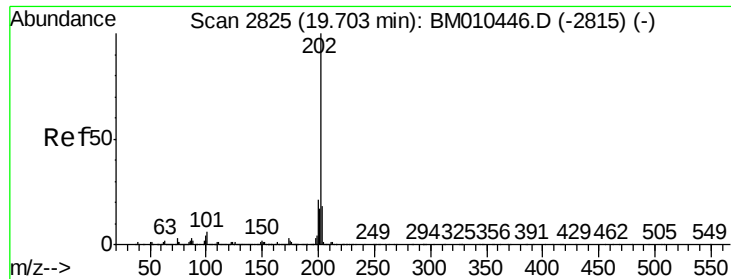

#77

Pyrene

Concen: 9.601 ng/ul

RT: 19.70 min Scan# 2825

Delta R.T. 0.00 min

Lab File: BM010450.D

Acq: 09 Jun 2017 13:04

Instrument :

BNA_M





ClientSampleId :

F5B94

Tgt Ion:	202	Resp:	834258
Ion Ratio	Lower	Upper	
202	100		
101	4.5	5.1	7.7#
100	3.7	4.9	7.3#

Manual Integrations
APPROVED

mohammad
6/12/2017 11:17:55 AM

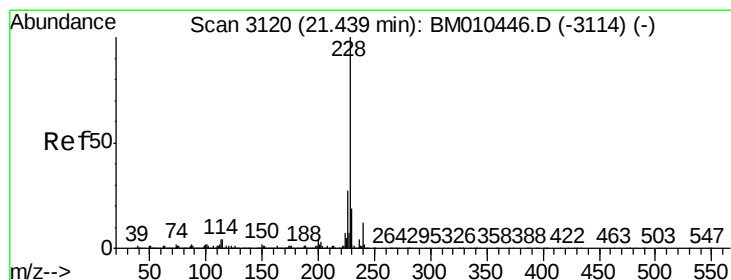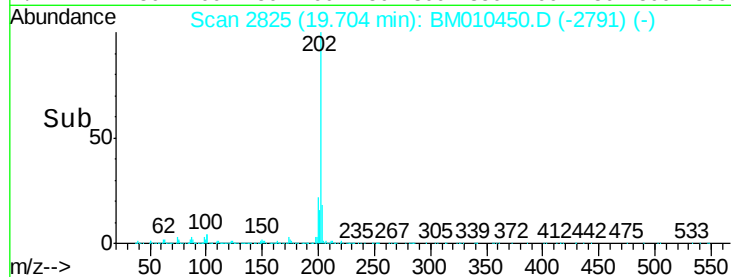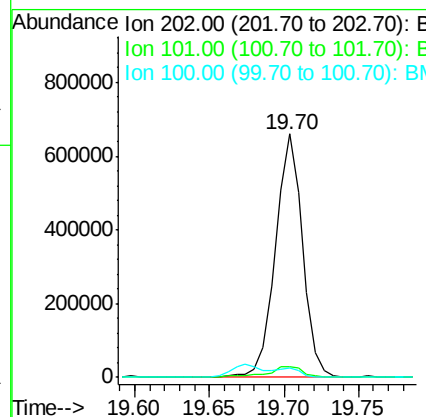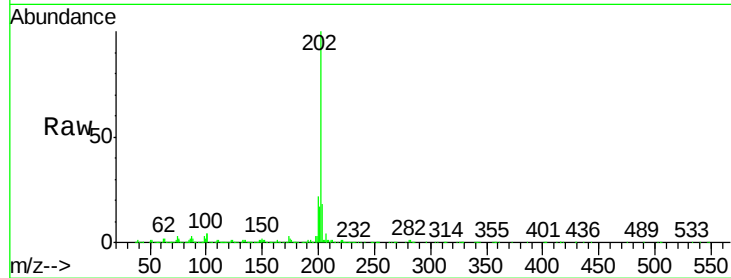

#80

Benzo(a)anthracene

Concen: 7.417 ng/ul




RT: 21.44 min Scan# 3120


Delta R.T. 0.00 min

Lab File: BM010450.D

Acq: 09 Jun 2017 13:04

Tgt Ion:	228	Resp:	705252
Ion Ratio	Lower	Upper	
228	100		
229	20.2	15.4	23.0
226	28.1	21.4	32.0

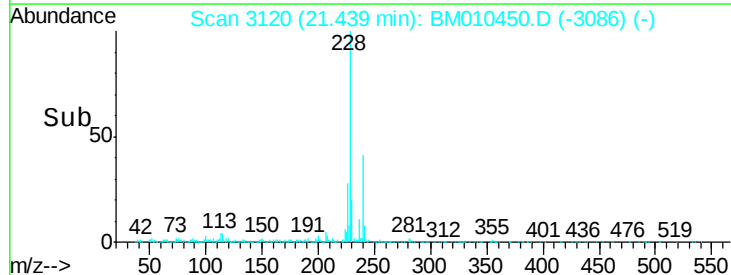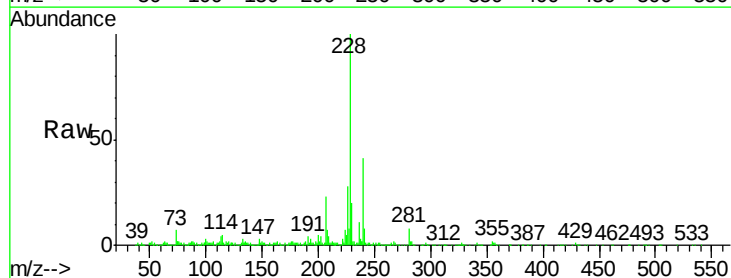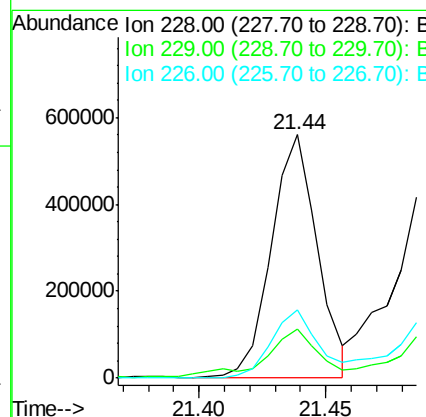

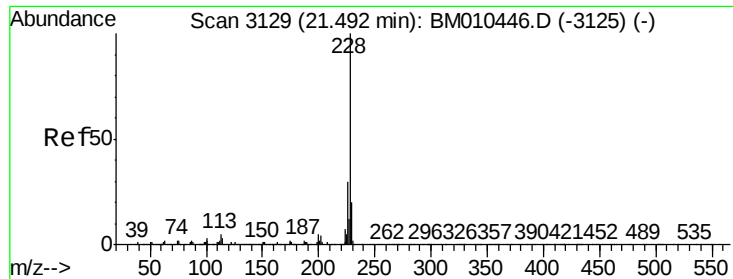

#82

Chrysene

Concen: 7.923 ng/ul

RT: 21.49 min Scan# 3129

Delta R.T. 0.00 min

Lab File: BM010450.D

Acq: 09 Jun 2017 13:04

Instrument :

BNA_M





ClientSampleId :

F5B94

Tgt Ion:	228	Resp:	681044
Ion Ratio	Lower	Upper	
228	100		
226	30.3	23.4	35.2
229	22.3	15.5	23.3

Manual Integrations
APPROVED

mohammad
6/12/2017 11:17:55 AM

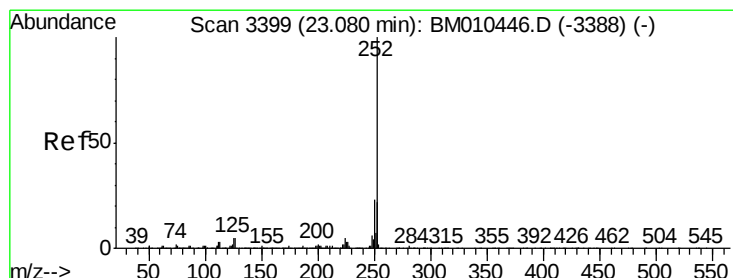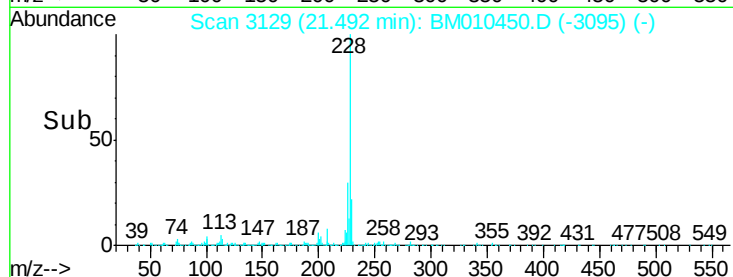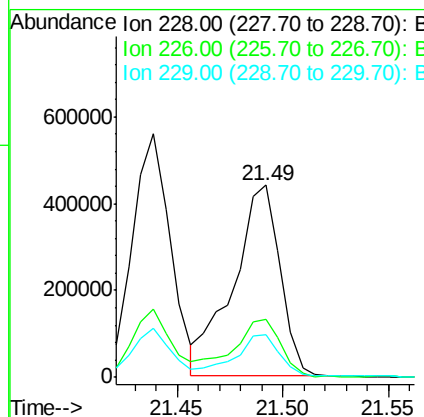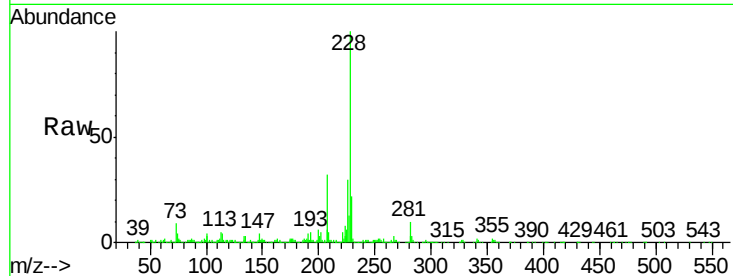

#85

Benzo(b)fluoranthene

Concen: 10.343 ng/ul




RT: 23.08 min Scan# 3399


Delta R.T. 0.00 min

Lab File: BM010450.D

Acq: 09 Jun 2017 13:04

Tgt Ion:	252	Resp:	989684
Ion Ratio	Lower	Upper	
252	100		
253	22.2	17.9	26.9
125	5.3	3.6	5.4

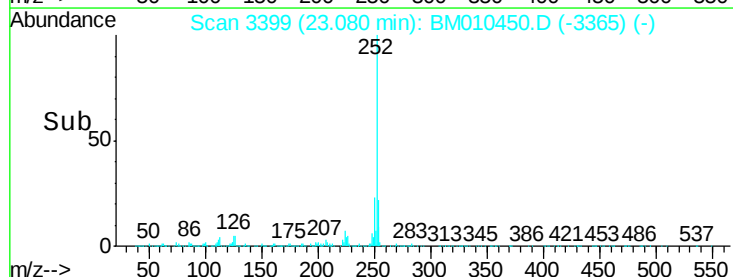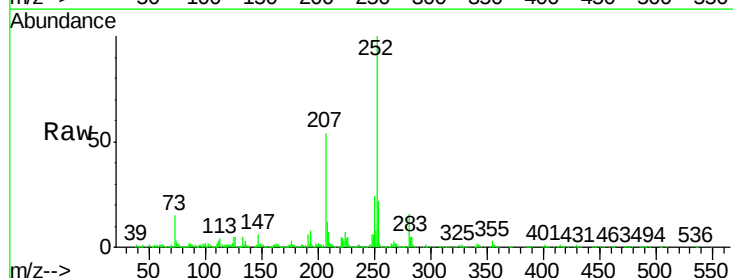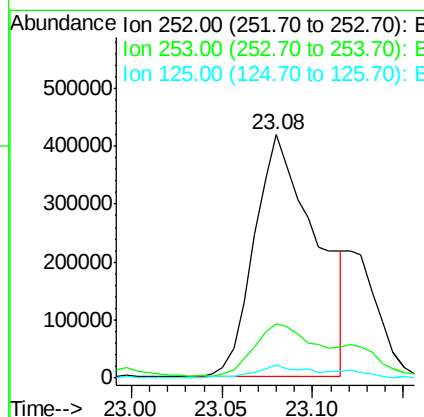

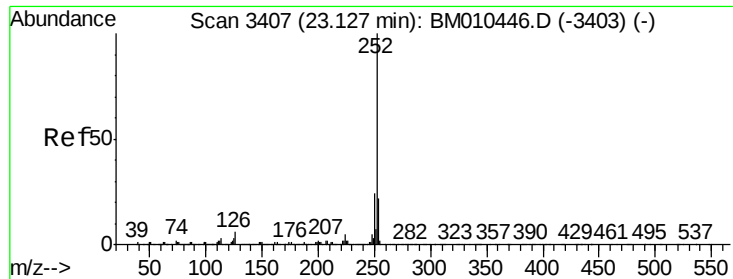





#86
Benzo(k)fluoranthene
Concen: 2.856 ng/u1 m
RT: 23.12 min Scan# 3406
Delta R.T. -0.01 min
Lab File: BM010450.D
Acq: 09 Jun 2017 13:04

Instrument :
BNA_M
ClientSampleId :
F5B94

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	261038		
253	25.9	17.1	25.7#	
125	6.3	3.4	5.2#	




Manual Integrations
APPROVED


mohammad
6/12/2017 11:17:55 AM

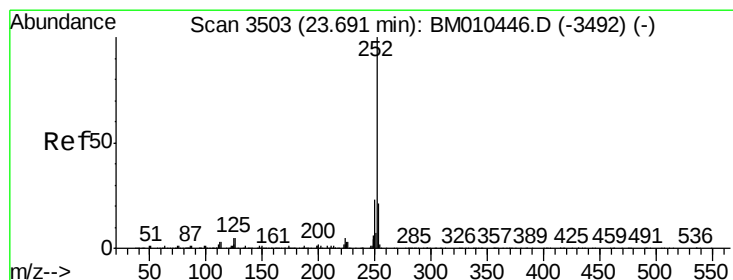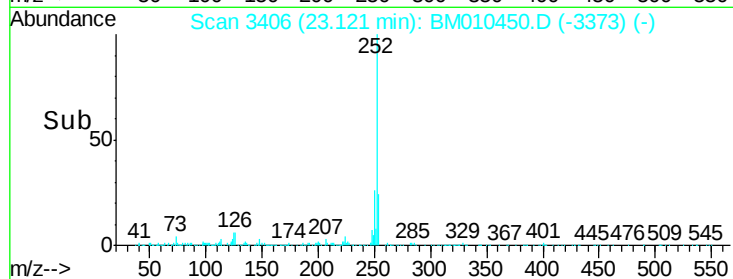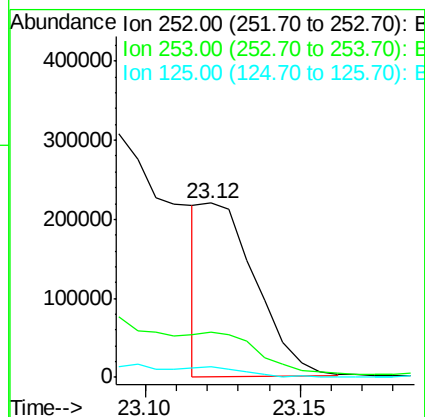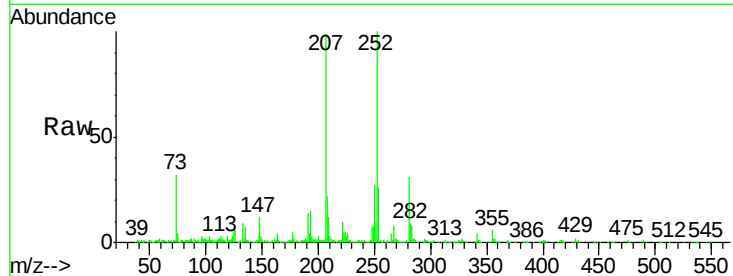

#88
Benzo(a)pyrene
Concen: 4.353 ng/u1
RT: 23.69 min Scan# 3503
Delta R.T. 0.00 min
Lab File: BM010450.D
Acq: 09 Jun 2017 13:04

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	412893		
253	26.5	18.2	27.2	
125	5.0	4.0	6.0	

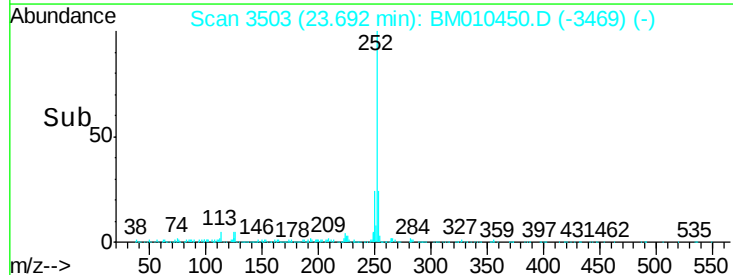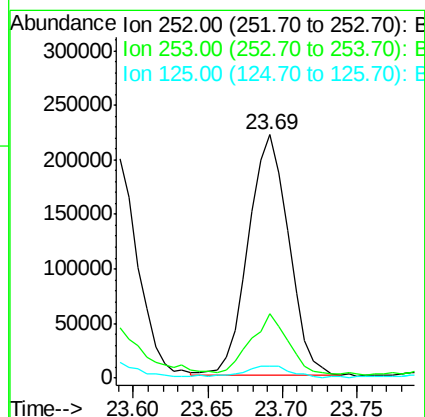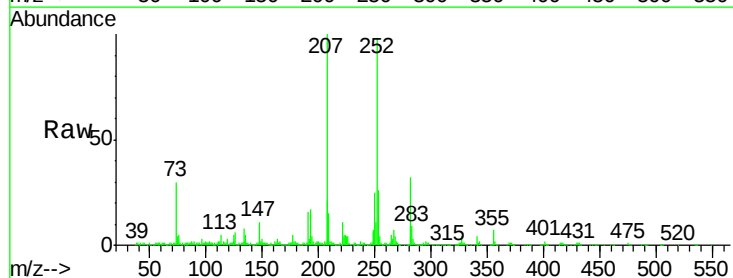

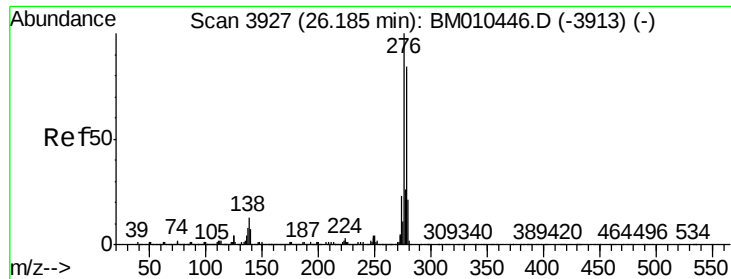

#89





Indeno(1,2,3-cd)pyrene
Concen: 2.593 ng/ul
RT: 26.18 min Scan# 3926
Delta R.T. -0.01 min
Lab File: BM010450.D
Acq: 09 Jun 2017 13:04

Instrument :
BNA_M
ClientSampled :
F5B94

Tgt Ion	Ratio	Resp	Lower	Upper
276	100	310717		
138	9.2	9.3	13.9	
277	21.8	19.9	29.9	

Manual Integrations
APPROVED

mohammad
6/12/2017 11:17:55 AM

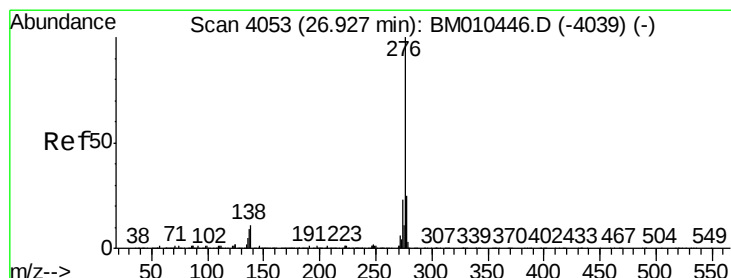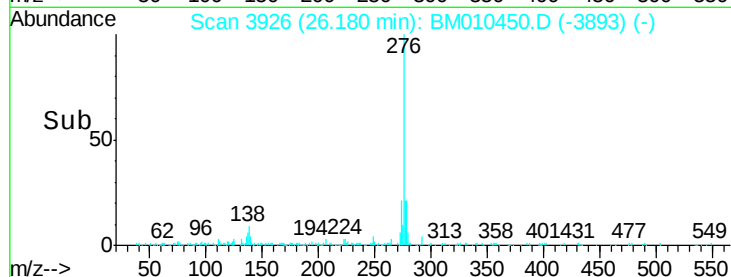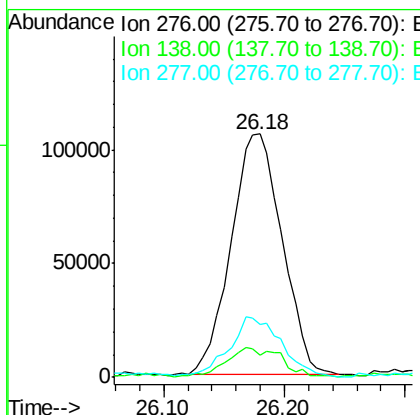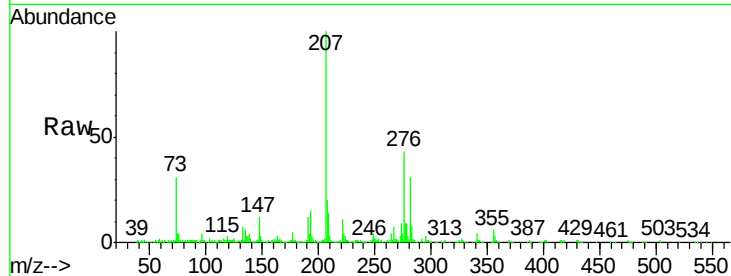

#91

Benzo(g,h,i)perylene
Concen: 2.335 ng/ul
RT: 26.93 min Scan# 4053
Delta R.T. 0.00 min
Lab File: BM010450.D
Acq: 09 Jun 2017 13:04

Tgt Ion	Ratio	Resp	Lower	Upper
276	100	230515		
138	12.0	8.5	12.7	
277	24.1	18.6	28.0	

