

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
 Data File : BM010447.D
 Acq On : 09 Jun 2017 11:16
 Operator : SJ/MA
 Sample : PB99575BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	44	49	55	rBV3	51120	89146	1.21%	0.125%
2	7.093	674	681	694	rBV	974497	1556901	21.18%	2.178%
3	7.246	701	707	717	rBV	666132	1036992	14.11%	1.451%
4	7.446	735	741	752	rBV	1158663	1801266	24.50%	2.520%
5	7.904	811	819	830	rBV	1061324	1687733	22.96%	2.361%
6	8.628	936	942	955	rBV	1279454	2053742	27.94%	2.873%
7	9.092	1013	1021	1031	rBV	1019018	1656869	22.54%	2.318%
8	9.804	1134	1142	1152	rBV	975465	1590985	21.64%	2.226%
9	10.334	1224	1232	1243	rBV	1507835	2540060	34.55%	3.554%
10	10.710	1289	1296	1304	rBV	1398988	2197974	29.90%	3.075%
11	10.875	1316	1324	1333	rBV	1302683	2190012	29.79%	3.064%
12	13.957	1841	1848	1859	rBV	3235024	4277601	58.19%	5.985%
13	14.239	1889	1896	1906	rBV	3039986	4344184	59.10%	6.078%
14	14.539	1940	1947	1956	rVB2	2083073	3161535	43.01%	4.423%
15	14.780	1982	1988	2006	rBV	983158	1673707	22.77%	2.342%
16	15.533	2107	2116	2124	rBV	4122692	5696485	77.49%	7.970%
17	15.657	2131	2137	2145	rBV	1222282	1702137	23.16%	2.382%
18	15.768	2152	2156	2166	rVB5	52584	88108	1.20%	0.123%
19	17.286	2407	2414	2423	rBV	2627147	3916434	53.28%	5.480%
20	17.386	2425	2431	2439	rBV	5000731	6662864	90.64%	9.322%
21	19.309	2754	2758	2761	rBV4	67643	93251	1.27%	0.130%
22	19.674	2815	2820	2827	rBV	5440956	7350790	100.00%	10.285%
23	21.456	3118	3123	3127	rBV	3178216	4089196	55.63%	5.721%
24	23.644	3489	3495	3503	rVB2	3298441	6203672	84.39%	8.680%
25	23.797	3515	3521	3531	rVB	1884866	3810849	51.84%	5.332%


Sum of corrected areas: 71472493

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
Data File : BM010447.D
Acq On : 09 Jun 2017 11:16
Operator : SJ/MA
Sample : PB99575BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK75

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

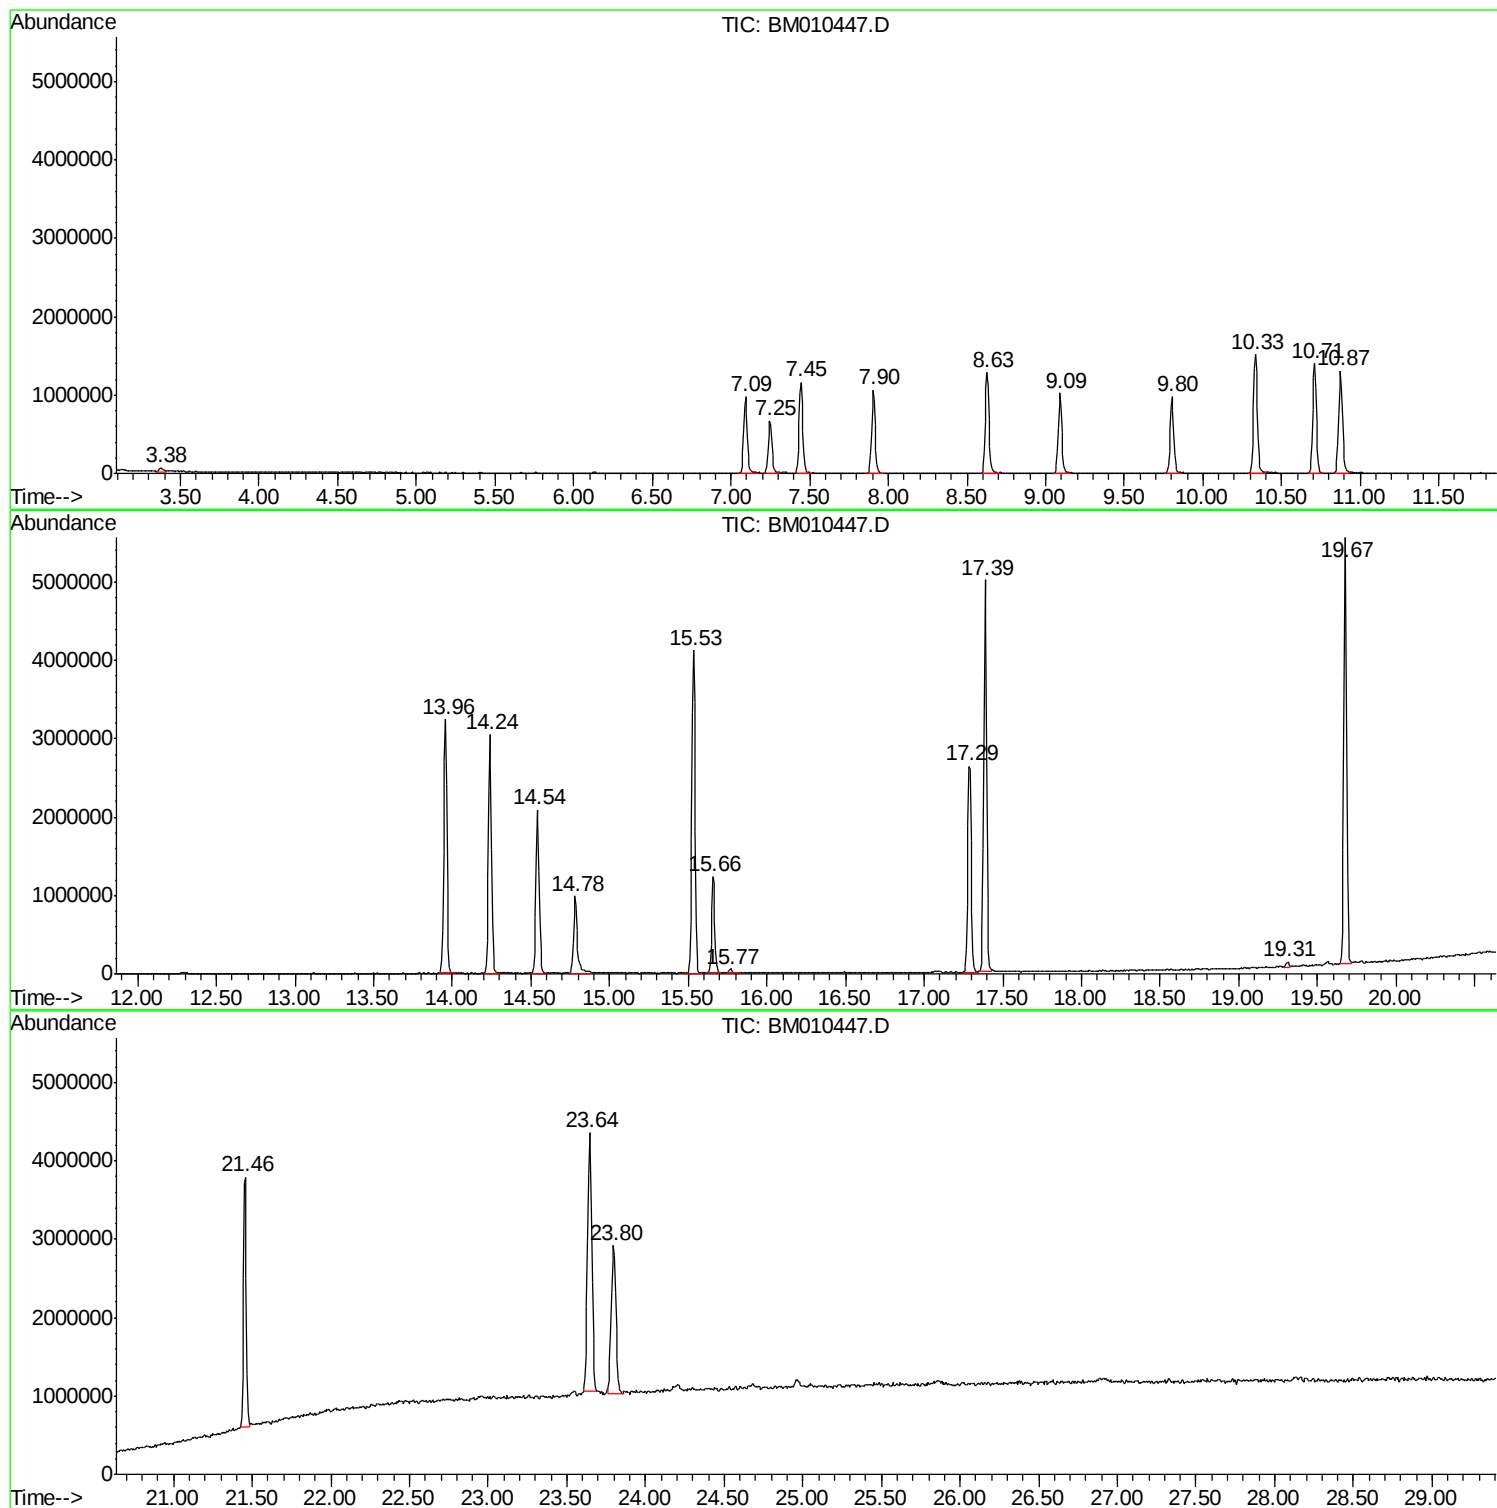

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
Data File : BM010447.D
Acq On : 09 Jun 2017 11:16
Operator : SJ/MA
Sample : PB99575BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK75

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
Data File : BM010447.D
Acq On : 09 Jun 2017 11:16
Operator : SJ/MA
Sample : PB99575BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK75

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc