

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
 Data File : BM010453.D
 Acq On : 09 Jun 2017 14:51
 Operator : SJ/MA
 Sample : PB99573BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	46	49	55	rVB	56966	70324	1.02%	0.096%
2	7.087	674	680	688	rBV	994210	1646635	23.98%	2.257%
3	7.246	701	707	719	rVB	734453	1118722	16.29%	1.533%
4	7.446	733	741	749	rBV	1225694	1953283	28.45%	2.677%
5	7.904	812	819	827	rBV	1183909	1794550	26.14%	2.459%
6	8.628	935	942	952	rBV	1345740	2164986	31.53%	2.967%
7	9.092	1013	1021	1032	rBV	1047796	1780836	25.94%	2.440%
8	9.804	1134	1142	1152	rBV	1020783	1725572	25.13%	2.365%
9	10.334	1224	1232	1251	rBV	1604317	2727708	39.73%	3.738%
10	10.704	1286	1295	1304	rBV	1367468	2351223	34.24%	3.222%
11	10.875	1315	1324	1338	rBV	1358496	2343842	34.14%	3.212%
12	13.957	1841	1848	1858	rBV	3201700	4504392	65.60%	6.173%
13	14.239	1888	1896	1904	rBV	3185174	4553458	66.32%	6.240%
14	14.539	1940	1947	1956	rBV2	2153915	3263252	47.53%	4.472%
15	14.780	1981	1988	1999	rBV	1016445	1678620	24.45%	2.300%
16	15.533	2109	2116	2126	rBV	4249400	5831495	84.93%	7.991%
17	15.657	2131	2137	2145	rBV	1295969	1773865	25.83%	2.431%
18	15.769	2152	2156	2162	rVB2	49457	72881	1.06%	0.100%
19	17.286	2407	2414	2422	rVB2	2734054	3885091	56.58%	5.324%
20	17.386	2422	2431	2439	rBV	4705221	6495700	94.60%	8.902%
21	19.674	2814	2820	2830	rBV	5258910	6866286	100.00%	9.409%
22	21.450	3118	3122	3128	rVB	3171858	3923687	57.14%	5.377%
23	23.644	3488	3495	3505	rVB2	3493019	6680066	97.29%	9.154%
24	23.797	3515	3521	3528	rVB	1959870	3765727	54.84%	5.160%


Sum of corrected areas: 72972201

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
Data File : BM010453.D
Acq On : 09 Jun 2017 14:51
Operator : SJ/MA
Sample : PB99573BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK73

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

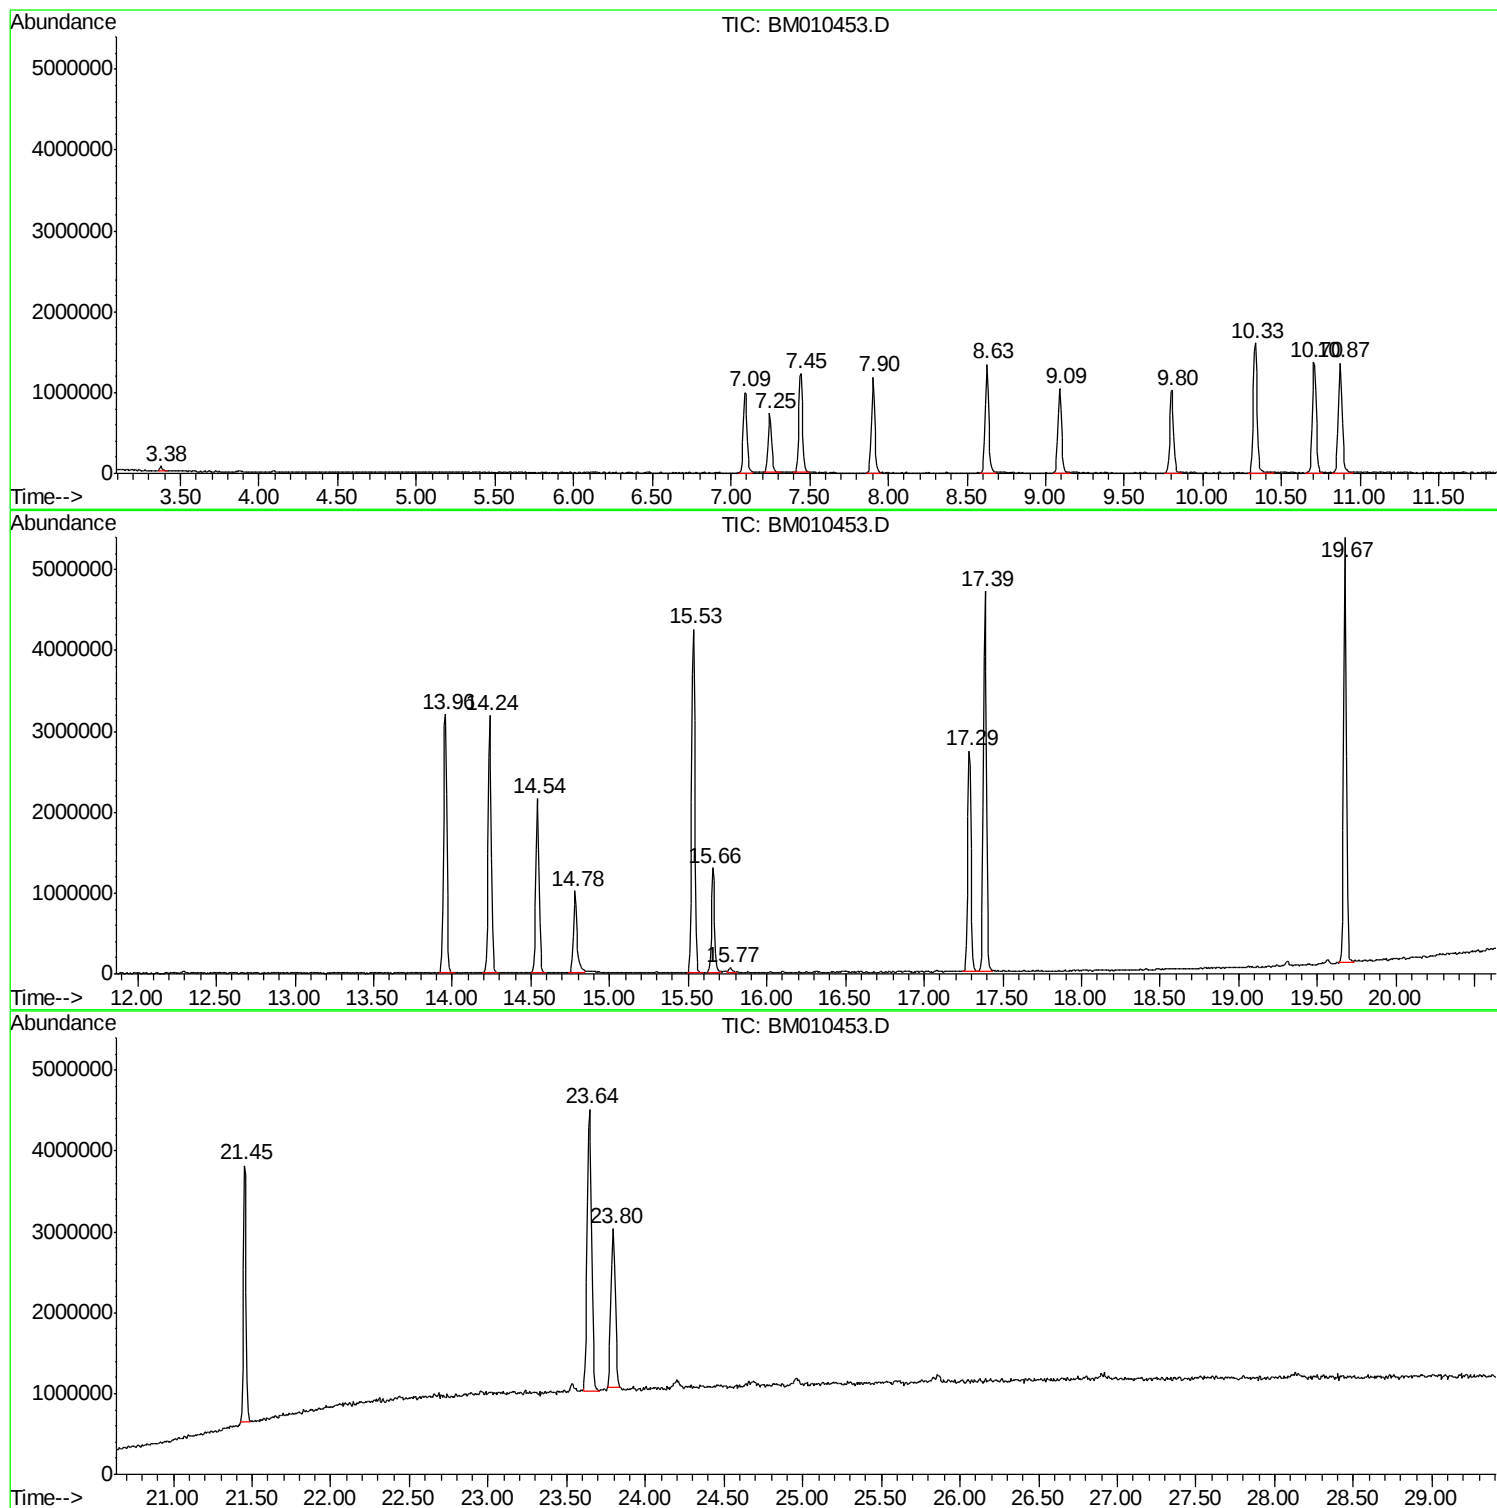

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
Data File : BM010453.D
Acq On : 09 Jun 2017 14:51
Operator : SJ/MA
Sample : PB99573BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK73

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
Data File : BM010453.D
Acq On : 09 Jun 2017 14:51
Operator : SJ/MA
Sample : PB99573BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK73

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc