

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
 Data File : BM010456.D
 Acq On : 09 Jun 2017 16:40
 Operator : SJ/MA
 Sample : I3520-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5A34

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	45	49	56	rBV	39103	55438	1.20%	0.096%
2	7.087	671	680	699	rBV	692290	1307591	28.27%	2.267%
3	7.245	701	707	716	rBV	532481	828953	17.92%	1.437%
4	7.439	732	740	749	rBV	878021	1439824	31.13%	2.497%
5	7.904	811	819	827	rBV	1108488	1743099	37.69%	3.023%
6	8.628	935	942	951	rBV	792022	1347035	29.12%	2.336%
7	9.086	1014	1020	1030	rBV	780049	1290690	27.90%	2.238%
8	9.798	1132	1141	1151	rBV	731433	1267012	27.39%	2.197%
9	10.333	1223	1232	1246	rBV	1158905	2015615	43.58%	3.495%
10	10.704	1289	1295	1303	rBV	1359506	2306153	49.86%	3.999%
11	10.875	1316	1324	1336	rBV	818600	1489443	32.20%	2.583%
12	13.957	1841	1848	1852	rBV	2183520	3094068	66.89%	5.365%
13	13.998	1852	1855	1863	rVB	677962	900370	19.47%	1.561%
14	14.239	1889	1896	1902	rBV	2314806	3210064	69.40%	5.566%
15	14.539	1940	1947	1956	rBV2	2148823	3194260	69.06%	5.539%
16	14.780	1980	1988	1996	rBV	527662	937324	20.27%	1.625%
17	15.321	2076	2080	2084	rBV3	44190	60793	1.31%	0.105%
18	15.533	2109	2116	2123	rVB	2868018	4090769	88.44%	7.094%
19	15.657	2131	2137	2146	rBV	850251	1141249	24.67%	1.979%
20	15.768	2152	2156	2161	rBV5	45482	64479	1.39%	0.112%
21	16.180	2221	2226	2231	rBV8	40866	62776	1.36%	0.109%
22	17.286	2406	2414	2421	rBV	2632398	3745319	80.97%	6.495%
23	17.386	2425	2431	2441	rVB	3110652	4280029	92.53%	7.422%
24	18.133	2553	2558	2564	rBV2	210807	308110	6.66%	0.534%
25	19.403	2771	2774	2777	rBV5	108861	137812	2.98%	0.239%
26	19.674	2814	2820	2826	rBV	3470893	4566159	98.72%	7.918%
27	21.450	3117	3122	3129	rBV	3231779	4136215	89.43%	7.172%
28	23.644	3489	3495	3504	rVB2	2357803	4625330	100.00%	8.020%
29	23.797	3515	3521	3531	rVB2	2009676	4023093	86.98%	6.976%


Sum of corrected areas: 57669072

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
Data File : BM010456.D
Acq On : 09 Jun 2017 16:40
Operator : SJ/MA
Sample : I3520-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5A34

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

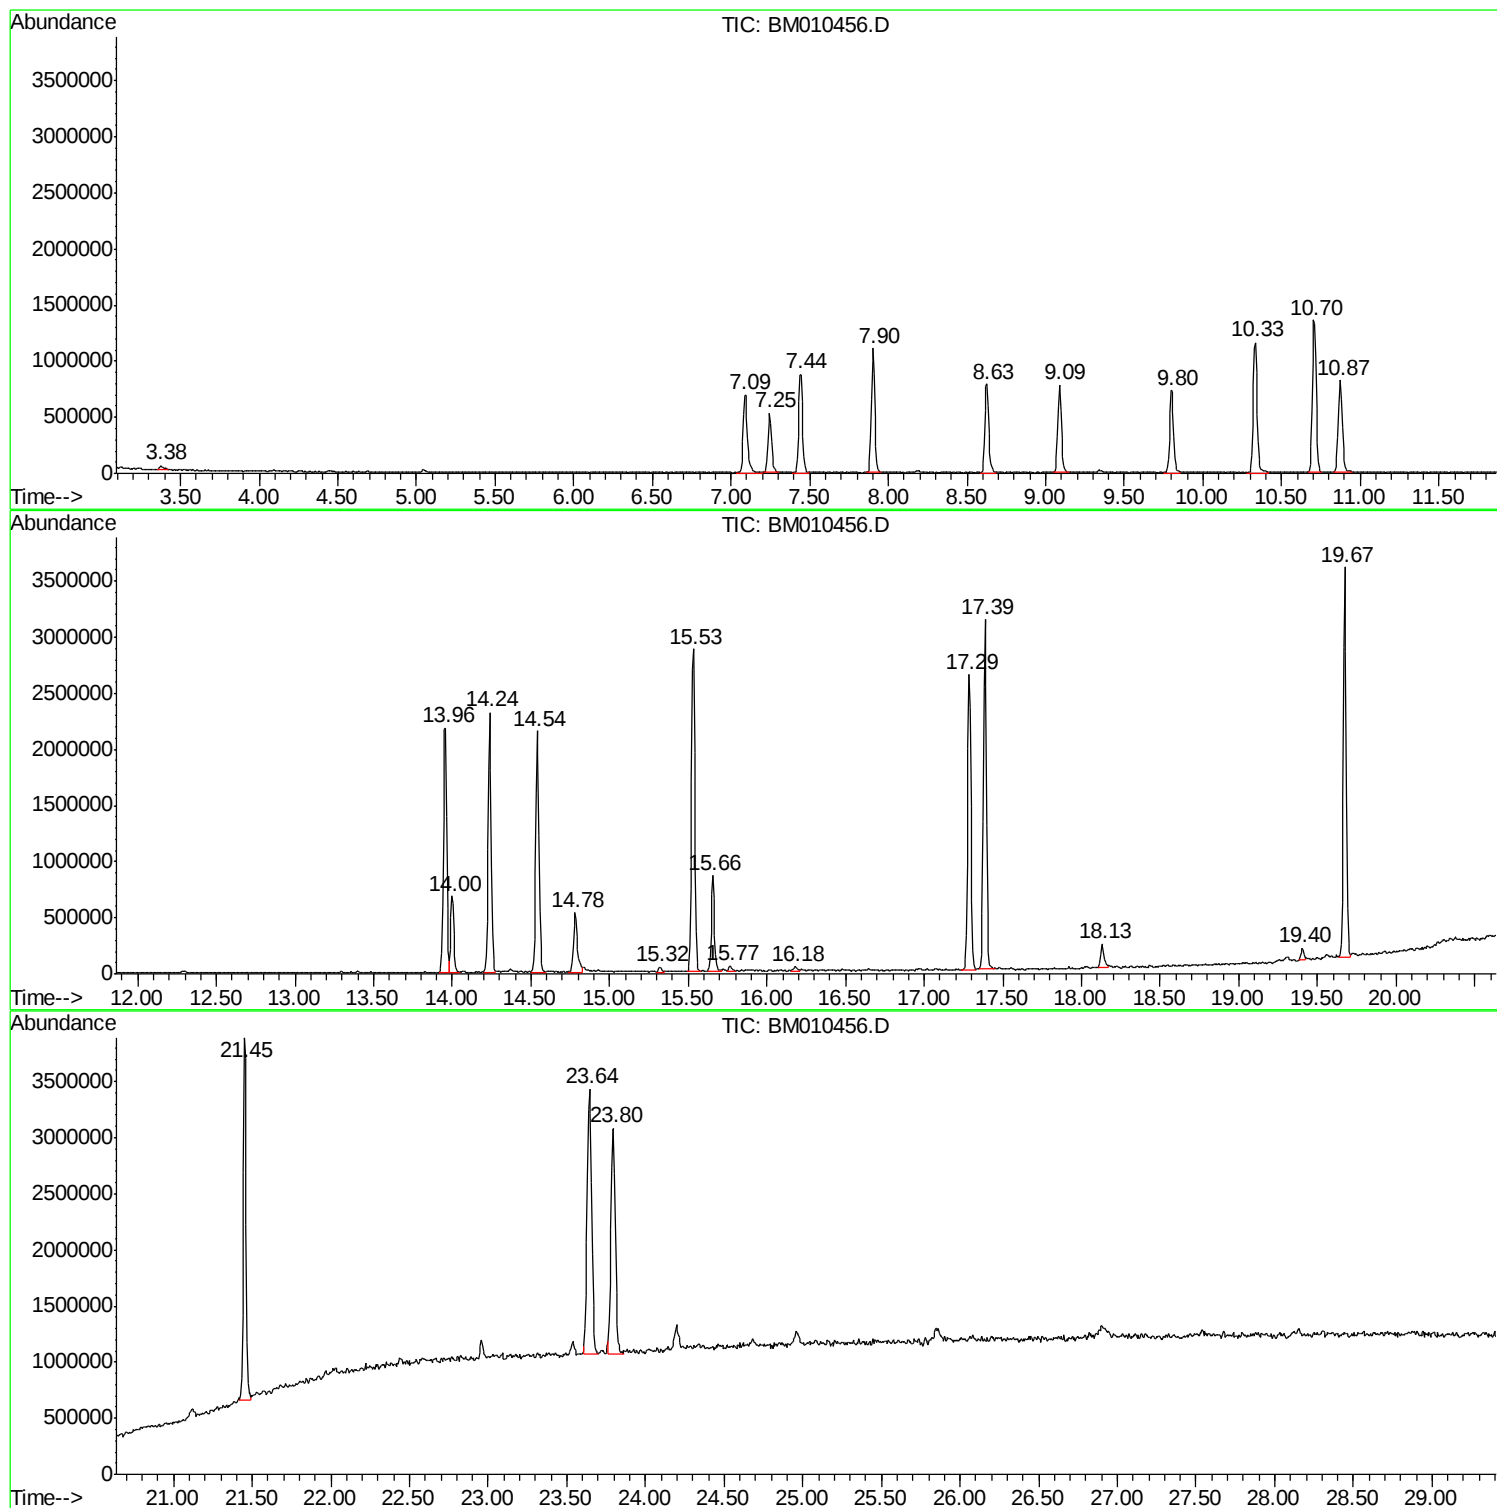

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
Data File : BM010456.D
Acq On : 09 Jun 2017 16:40
Operator : SJ/MA
Sample : I3520-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5A34

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060917\
Data File : BM010456.D
Acq On : 09 Jun 2017 16:40
Operator : SJ/MA
Sample : I3520-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5A34

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc