
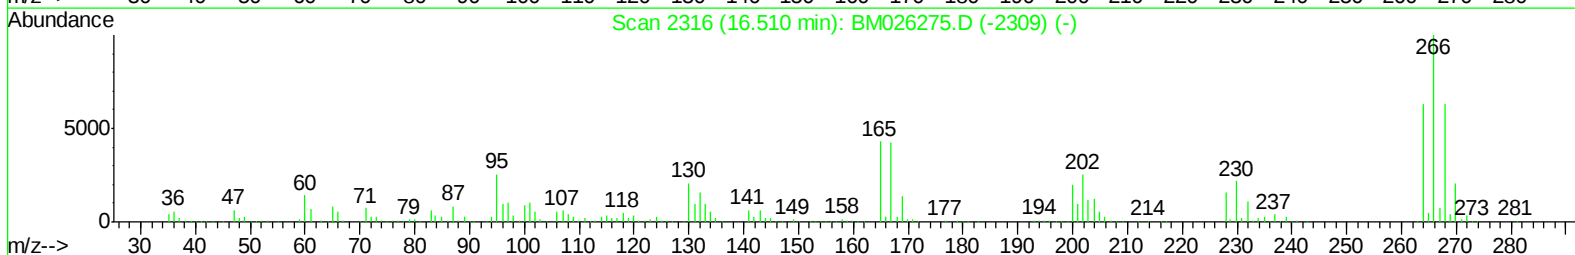
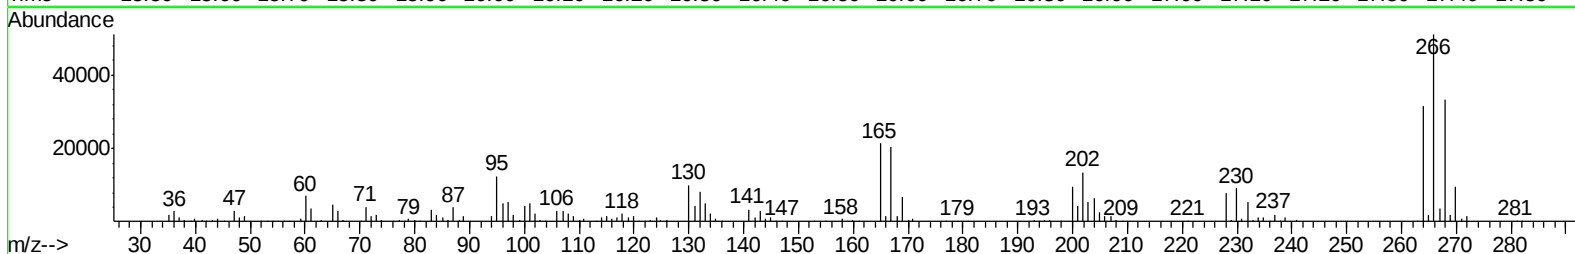


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060920\
 Data File : BM026300.D
 Acq On : 09 Jun 2020 12:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 00:59:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 09 14:46:47 2020
 Response via : Initial Calibration

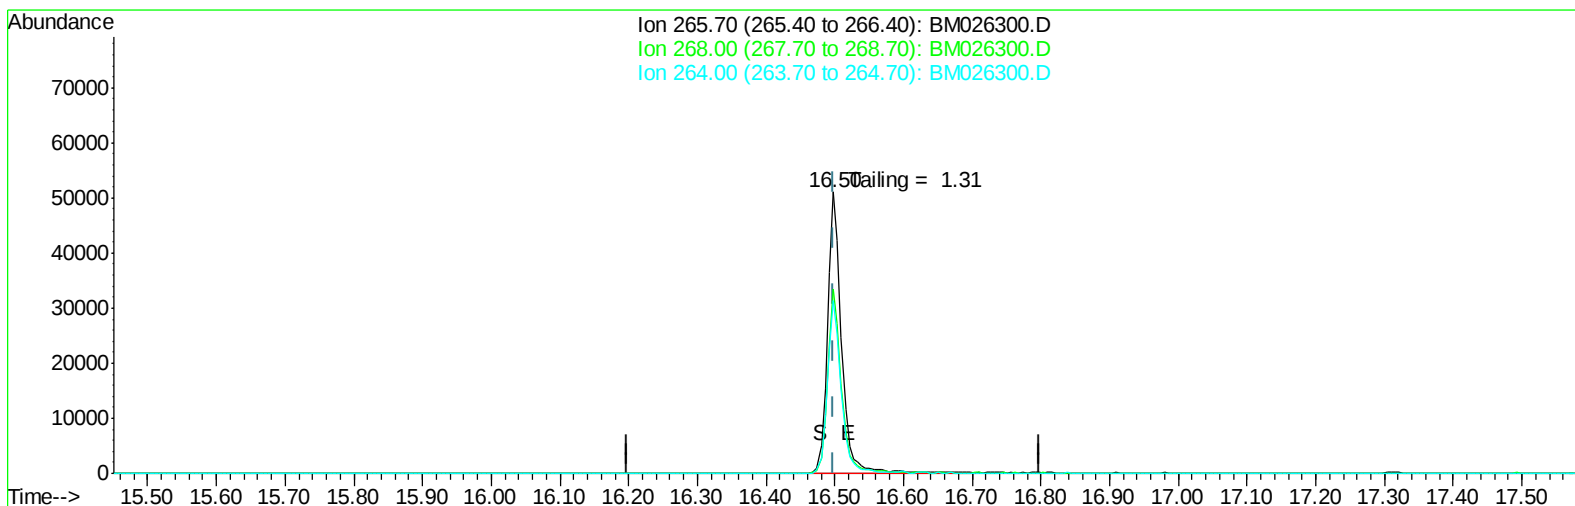

TIC: BM026300.D

(70) Pentachlorophenol (C)




16.498min (-0.000) 0.00ng

response 71853

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	65.32
264.00	62.80	61.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060920\
 Data File : BM026300.D
 Acq On : 09 Jun 2020 12:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 00:59:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 09 14:46:47 2020
 Response via : Initial Calibration

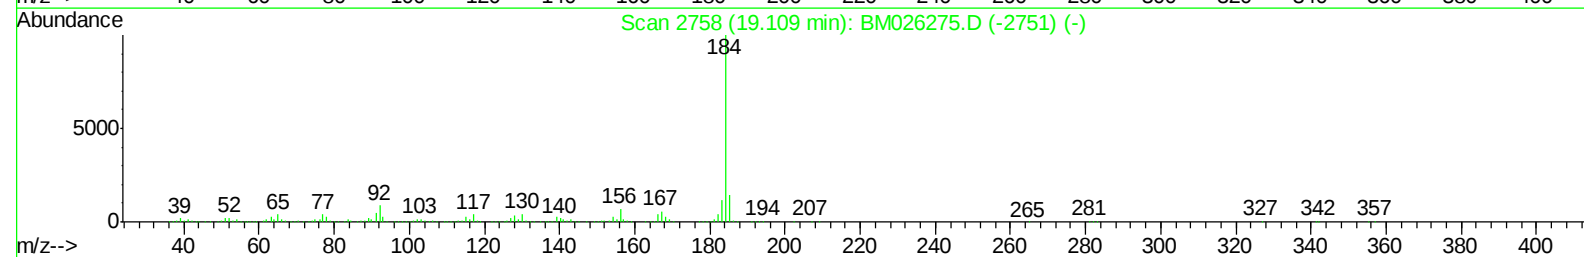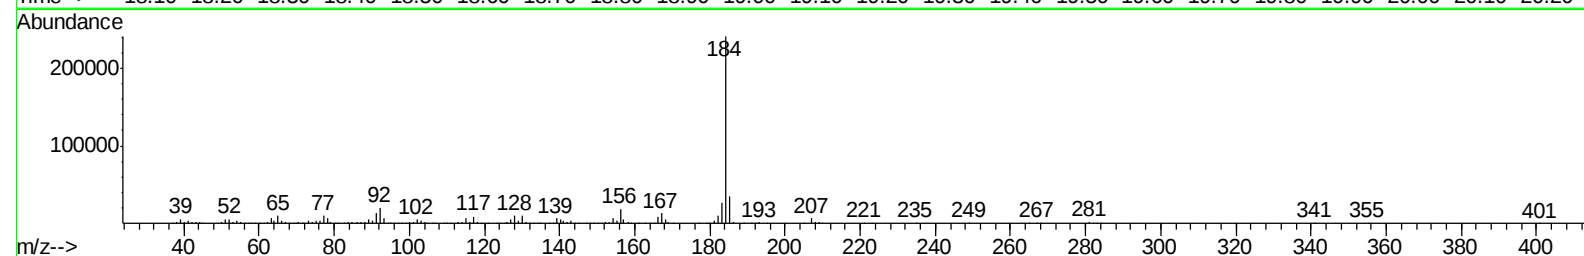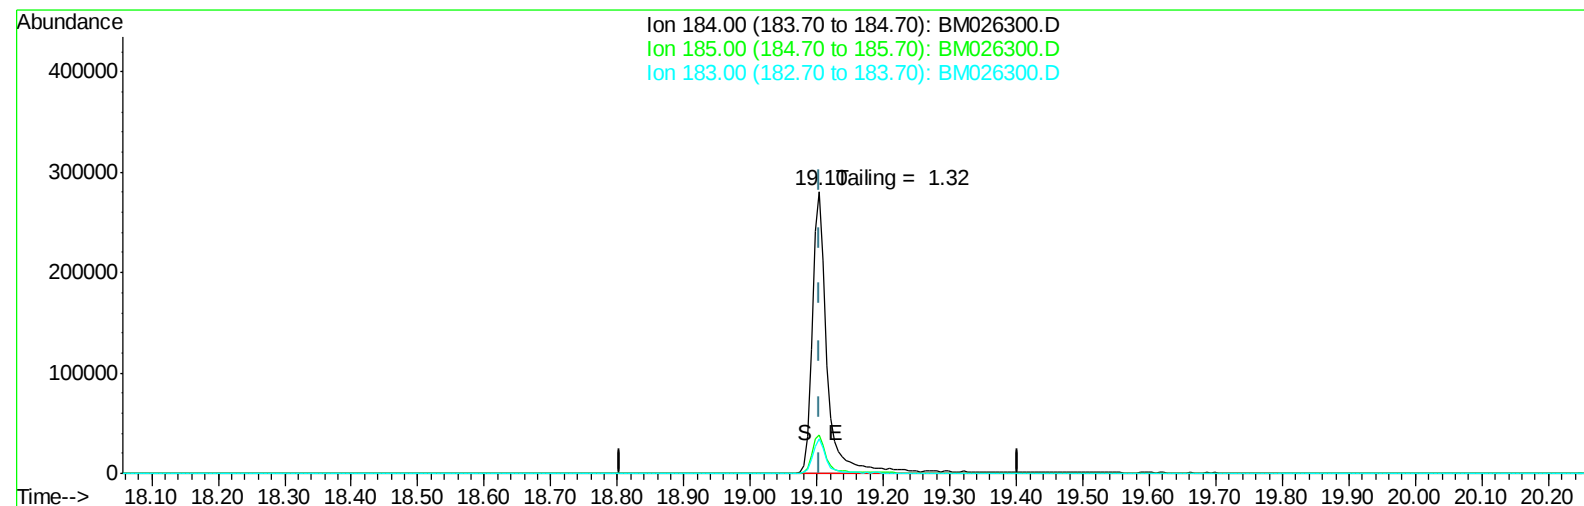

TIC: BM026300.D

(77) Benzidine

19.103min (-0.000) 24861.79ng

response 439988

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	13.53
183.00	11.60	12.07
0.00	0.00	0.00