

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060920\
 Data File : BM026302.D
 Acq On : 09 Jun 2020 14:03
 Operator : JU/CG
 Sample : L2941-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 RBF-TS-001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.063	363	370	383	rBV	1721117	2460271	35.96%	3.686%
2	6.634	629	637	649	rBV	1783179	2673182	39.07%	4.005%
3	7.428	765	772	783	rVB	610611	923544	13.50%	1.384%
4	7.740	818	825	833	rBV	1369406	2155650	31.51%	3.230%
5	8.575	959	967	977	rBV	1107161	1762729	25.76%	2.641%
6	10.187	1230	1241	1254	rBV	764813	1254199	18.33%	1.879%
7	12.692	1660	1667	1674	rBV	2532804	3567398	52.14%	5.345%
8	13.551	1808	1813	1819	rBV	263779	368085	5.38%	0.551%
9	14.080	1896	1903	1911	rBV	1091103	1548663	22.63%	2.320%
10	15.580	2150	2158	2165	rBV	1964418	2697945	39.43%	4.042%
11	16.833	2365	2371	2376	rBV	1264302	1726395	25.23%	2.587%
12	16.874	2376	2378	2382	rVB	83529	89664	1.31%	0.134%
13	16.921	2382	2386	2389	rBV3	56575	74211	1.08%	0.111%
14	16.963	2389	2393	2398	rVB2	82205	104933	1.53%	0.157%
15	18.045	2569	2577	2581	rBV3	92349	162454	2.37%	0.243%
16	18.798	2701	2705	2715	rVB3	79900	137850	2.01%	0.207%
17	18.904	2718	2723	2727	rBV	141368	194722	2.85%	0.292%
18	18.974	2730	2735	2740	rBV	417851	524808	7.67%	0.786%
19	19.168	2764	2768	2773	rVB	117289	142292	2.08%	0.213%
20	19.262	2781	2784	2795	rVB	118692	187259	2.74%	0.281%
21	19.486	2817	2822	2831	rVB	3907922	4828775	70.58%	7.235%
22	19.833	2878	2881	2884	rBV2	77460	84718	1.24%	0.127%
23	20.139	2930	2933	2939	rBV3	123924	174987	2.56%	0.262%
24	20.304	2958	2961	2964	rBV	92405	107456	1.57%	0.161%
25	20.792	3040	3044	3049	rBV2	551820	738072	10.79%	1.106%
26	20.927	3064	3067	3071	rBV	84830	100897	1.47%	0.151%
27	21.039	3081	3086	3091	rBV	1611444	2055853	30.05%	3.080%
28	21.233	3117	3119	3124	rVB2	113297	107091	1.57%	0.160%
29	21.650	3186	3190	3200	rBV2	1302627	1817013	26.56%	2.722%
30	22.086	3261	3264	3273	rVB	221436	289610	4.23%	0.434%
31	22.198	3281	3283	3288	rVB	288461	332922	4.87%	0.499%
32	22.562	3339	3345	3349	rBV	5222764	6841959	100.00%	10.251%
33	23.145	3438	3444	3451	rBV	1160643	2016475	29.47%	3.021%
34	23.562	3512	3515	3521	rVB	262116	405613	5.93%	0.608%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060920\
Data File : BM026302.D
Acq On : 09 Jun 2020 14:03
Operator : JU/CG
Sample : L2941-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RBF-TS-001

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	23.674	3528	3534	3541	rVV	3307486	5784584	84.55%	8.667%
36	23.744	3542	3546	3555	rVB	624733	1082381	15.82%	1.622%
37	24.086	3599	3604	3616	rVB	744074	1656118	24.21%	2.481%
38	25.944	3914	3920	3926	rBV3	971273	2395653	35.01%	3.589%
39	26.009	3927	3931	3939	rVB2	983855	2036412	29.76%	3.051%
40	26.621	4027	4035	4050	rVB2	1327389	3892415	56.89%	5.832%
41	27.091	4107	4115	4121	rBV3	1029160	3179367	46.47%	4.763%
42	27.162	4122	4127	4143	rVB2	1333828	4060134	59.34%	6.083%


Sum of corrected areas: 66744759

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060920\
Data File : BM026302.D
Acq On : 09 Jun 2020 14:03
Operator : JU/CG
Sample : L2941-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RBF-TS-001

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

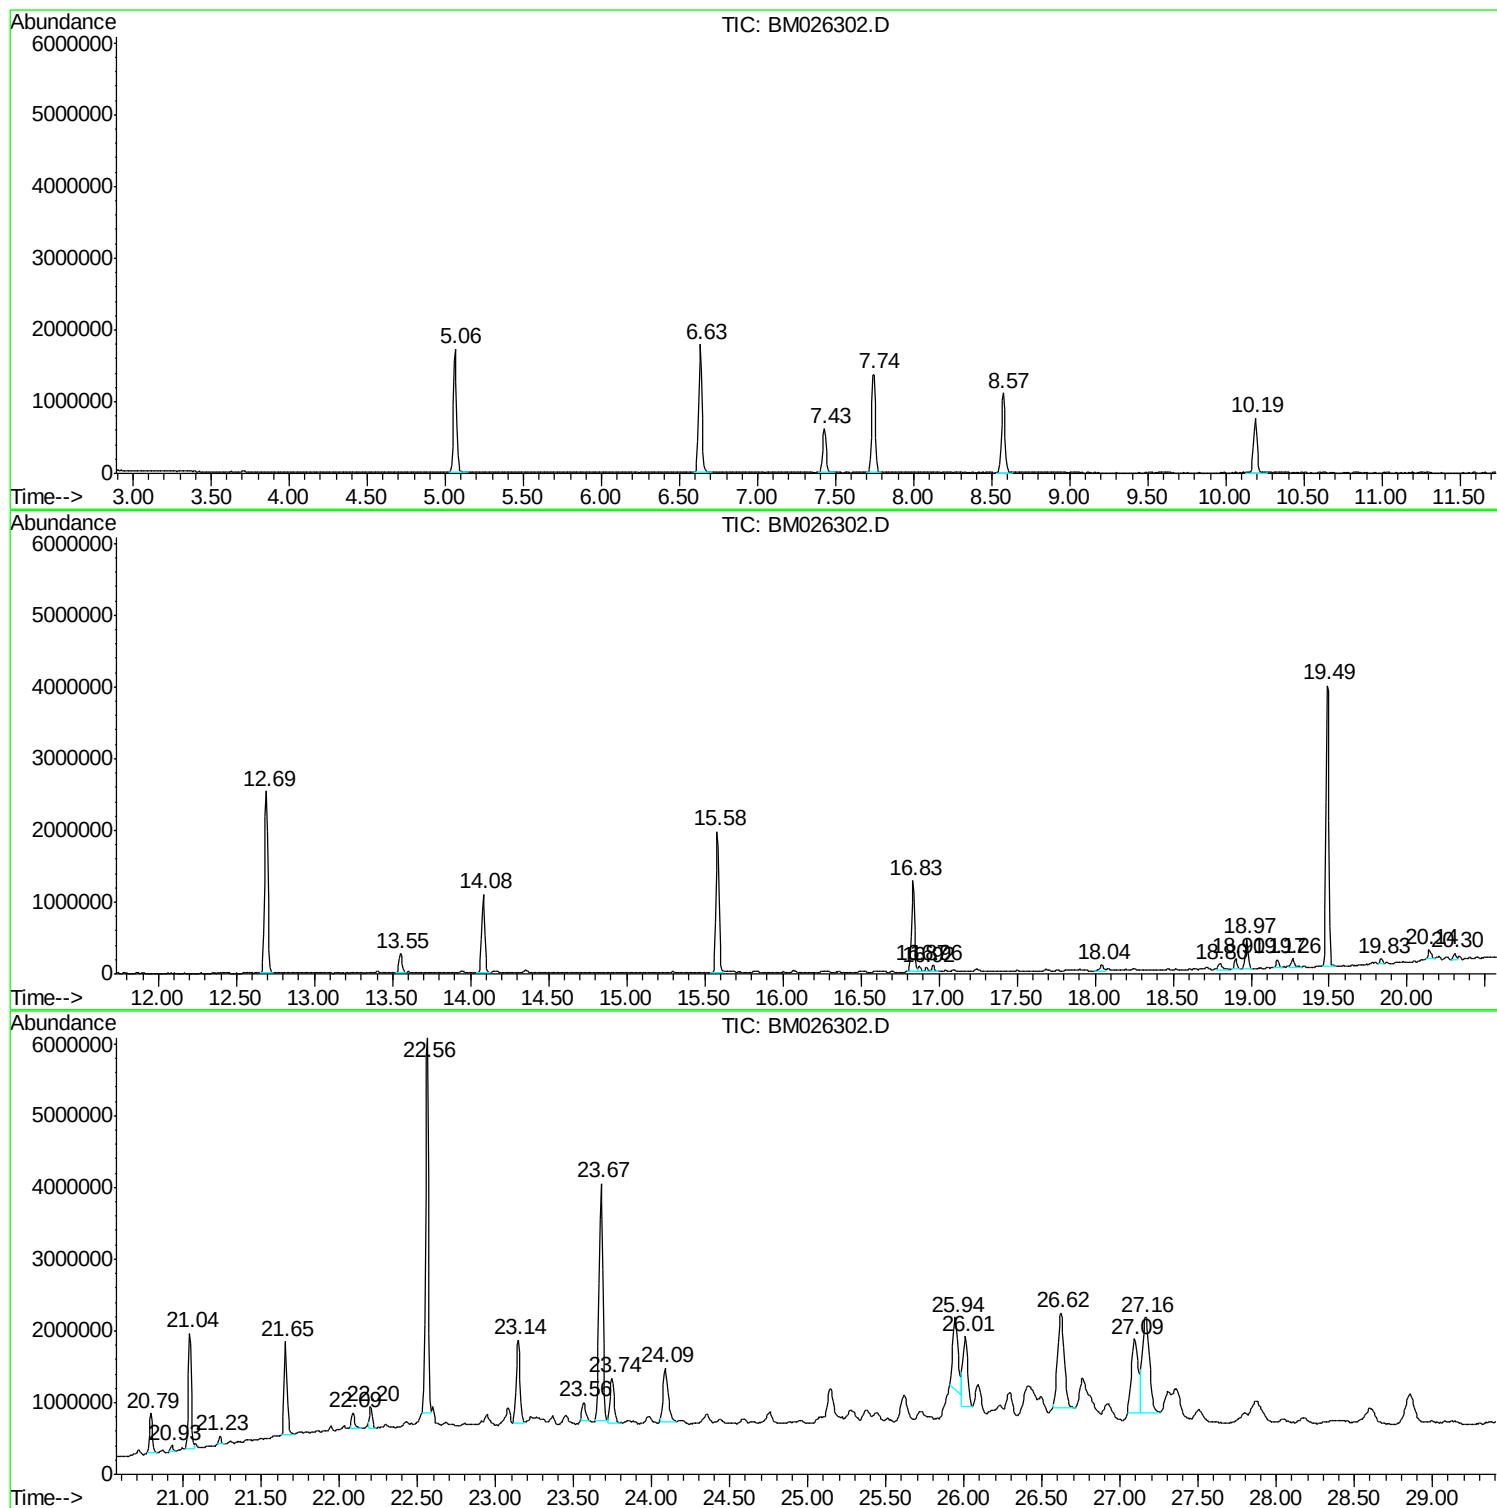

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060920\
Data File : BM026302.D
Acq On : 09 Jun 2020 14:03
Operator : JU/CG
Sample : L2941-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RBF-TS-001

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060920\
Data File : BM026302.D
Acq On : 09 Jun 2020 14:03
Operator : JU/CG
Sample : L2941-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RBF-TS-001

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc