

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060920\
 Data File : BM026304.D
 Acq On : 09 Jun 2020 15:17
 Operator : JU/CG
 Sample : L2939-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PHC-326FB-010

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.069	364	371	384	rBV	1889424	2741646	49.15%	4.023%
2	6.640	631	638	653	rVB	2021677	2979560	53.42%	4.373%
3	7.087	708	714	720	rBV6	34250	76375	1.37%	0.112%
4	7.428	766	772	779	rBV	696625	1050777	18.84%	1.542%
5	7.745	816	826	834	rBV	1625977	2460961	44.12%	3.612%
6	7.934	853	858	863	rBV2	46599	81921	1.47%	0.120%
7	8.216	896	906	916	rBV7	20883	63985	1.15%	0.094%
8	8.575	960	967	979	rVB	1262649	1983047	35.55%	2.910%
9	9.710	1154	1160	1167	rBV	98532	166959	2.99%	0.245%
10	10.192	1235	1242	1248	rBV	843086	1390866	24.93%	2.041%
11	11.028	1377	1384	1393	rBV	333525	537319	9.63%	0.789%
12	12.286	1592	1598	1605	rBV5	38843	72786	1.30%	0.107%
13	12.427	1617	1622	1629	rVB2	51195	86295	1.55%	0.127%
14	12.692	1660	1667	1678	rVB	2918609	4060546	72.80%	5.959%
15	13.398	1782	1787	1792	rBV	34651	71665	1.28%	0.105%
16	13.557	1807	1814	1821	rVB	258874	411828	7.38%	0.604%
17	13.757	1845	1848	1852	rBV4	51320	81709	1.46%	0.120%
18	13.804	1852	1856	1862	rVB3	87113	152761	2.74%	0.224%
19	14.080	1897	1903	1910	rBV	1180400	1754631	31.46%	2.575%
20	14.157	1910	1916	1923	rVB7	32620	77030	1.38%	0.113%
21	14.551	1979	1983	1991	rVB6	35406	66677	1.20%	0.098%
22	15.457	2133	2137	2144	rVB5	63321	99053	1.78%	0.145%
23	15.586	2153	2159	2167	rVB	2244311	3027404	54.27%	4.443%
24	15.998	2226	2229	2234	rBV5	44362	65358	1.17%	0.096%
25	16.639	2335	2338	2343	rVB3	43113	69409	1.24%	0.102%
26	16.833	2366	2371	2376	rBV	1383073	1954972	35.05%	2.869%
27	16.874	2376	2378	2383	rVB	352844	415395	7.45%	0.610%
28	16.968	2390	2394	2399	rVB	138418	188766	3.38%	0.277%
29	18.027	2571	2574	2578	rBV	161504	205941	3.69%	0.302%
30	18.245	2606	2611	2614	rBV	1046311	1449771	25.99%	2.128%
31	18.280	2614	2617	2621	rVB	329073	421909	7.56%	0.619%
32	18.633	2674	2677	2678	rBV3	124143	137073	2.46%	0.201%
33	18.662	2679	2682	2687	rVB	813937	1035230	18.56%	1.519%
34	18.904	2719	2723	2728	rVB	602382	775952	13.91%	1.139%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060920\
Data File : BM026304.D
Acq On : 09 Jun 2020 15:17
Operator : JU/CG
Sample : L2939-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PHC-326FB-010

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	19.062	2747	2750	2755	rBV4	399628	559547	10.03%	0.821%
36	19.221	2773	2777	2780	rBV2	423798	585241	10.49%	0.859%
37	19.268	2782	2785	2789	rVB	583974	662184	11.87%	0.972%
38	19.392	2803	2806	2810	rVB	421502	457780	8.21%	0.672%
39	19.492	2818	2823	2831	rVB	4651472	5578003	100.00%	8.186%
40	19.780	2869	2872	2879	rVB3	357075	482711	8.65%	0.708%
41	20.062	2917	2920	2924	rVB3	513525	608628	10.91%	0.893%
42	20.221	2944	2947	2953	rVB3	734083	925435	16.59%	1.358%
43	20.533	2996	3000	3004	rVB	2608088	3016373	54.08%	4.427%
44	20.592	3008	3010	3014	rVB	467993	485518	8.70%	0.713%
45	20.798	3041	3045	3050	rBV	1567874	1916475	34.36%	2.812%
46	20.868	3054	3057	3061	rVB	1102840	1337839	23.98%	1.963%
47	21.050	3083	3088	3091	rBV2	1762571	2427842	43.53%	3.563%
48	21.086	3091	3094	3101	rVB	2455921	2877328	51.58%	4.223%
49	21.450	3153	3156	3162	rVB	3865790	4500087	80.68%	6.604%
50	21.515	3163	3167	3174	rVV	3374086	3972642	71.22%	5.830%
51	22.050	3254	3258	3263	rBV2	1821032	2345417	42.05%	3.442%
52	22.468	3325	3329	3333	rBV	2394304	3082215	55.26%	4.523%
53	23.162	3444	3447	3453	rVB	1446810	2105177	37.74%	3.089%


Sum of corrected areas: 68142019

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060920\
Data File : BM026304.D
Acq On : 09 Jun 2020 15:17
Operator : JU/CG
Sample : L2939-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PHC-326FB-010

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

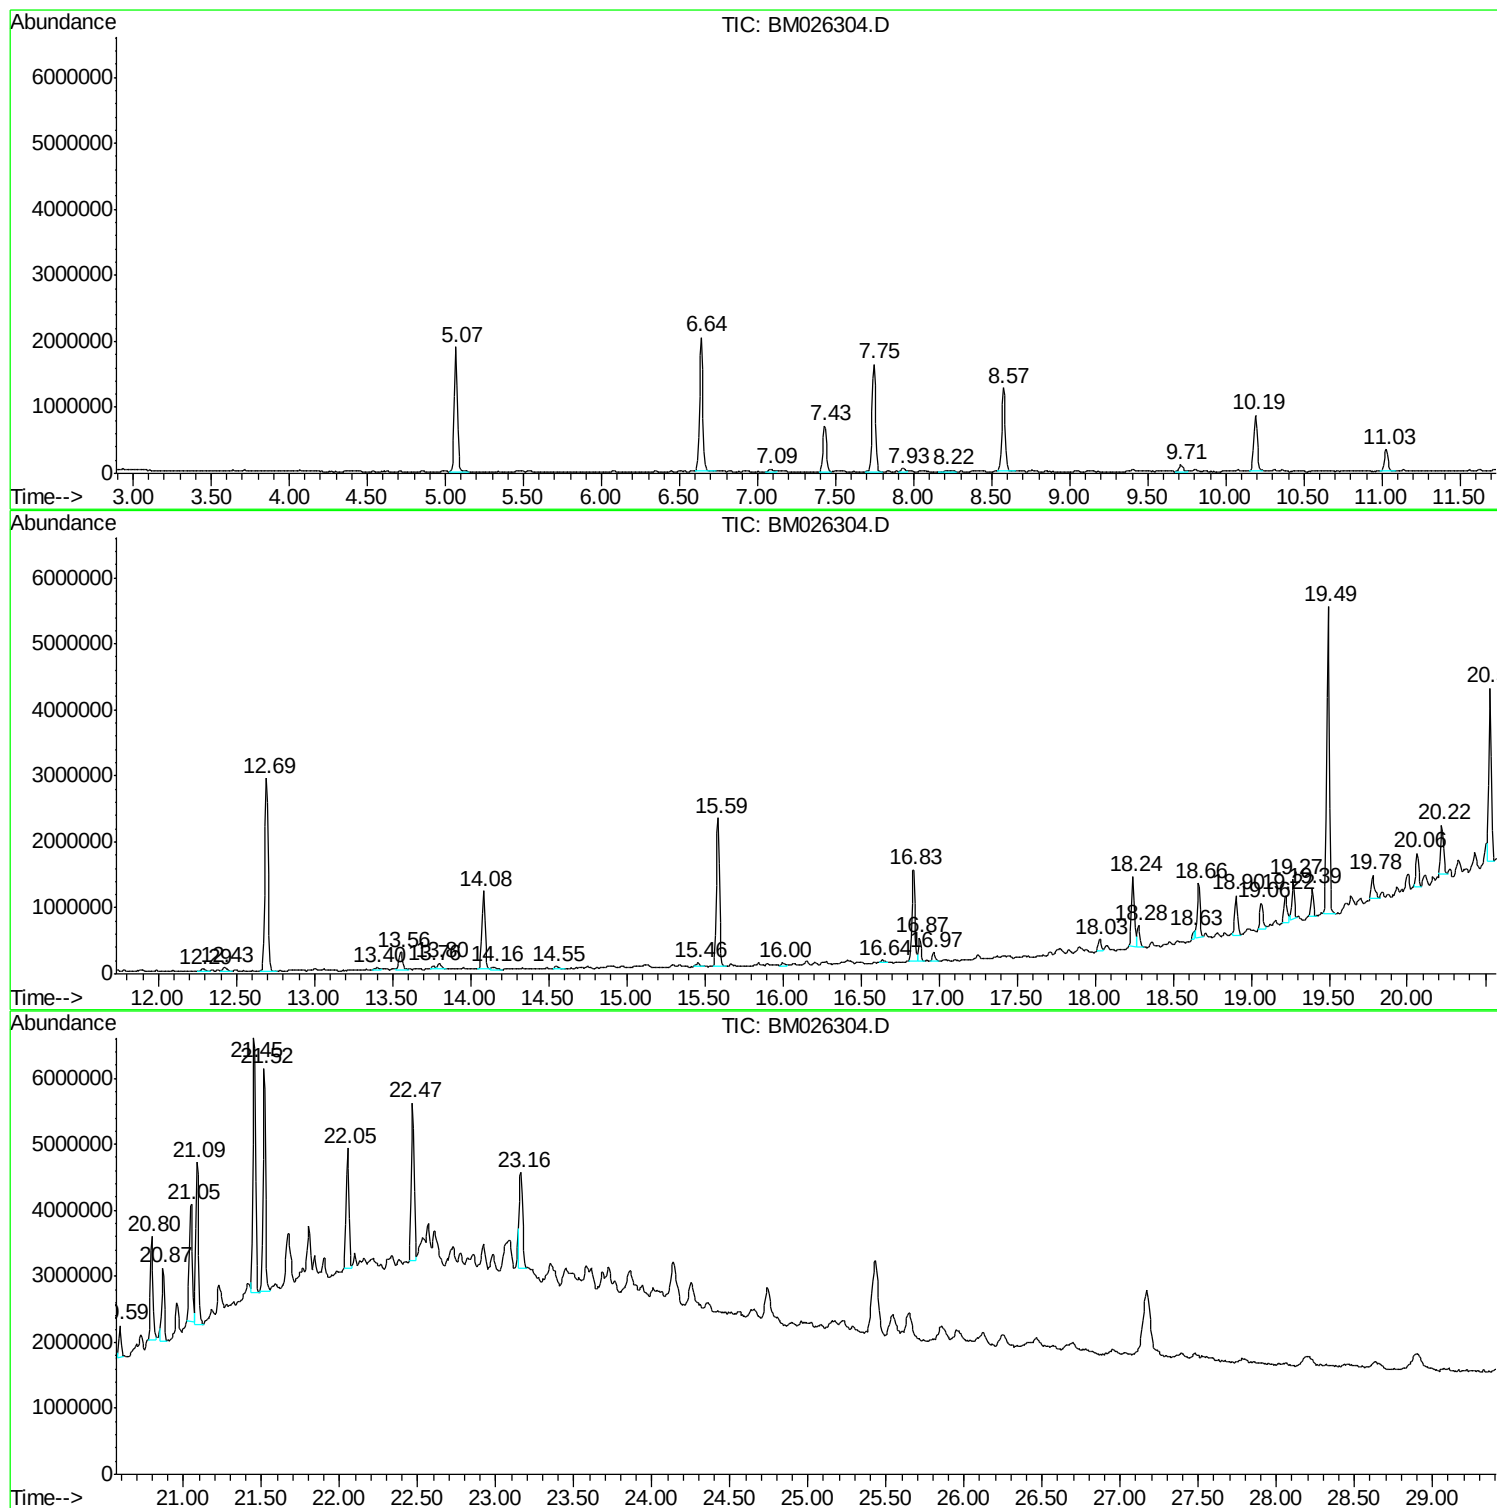

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060920\
Data File : BM026304.D
Acq On : 09 Jun 2020 15:17
Operator : JU/CG
Sample : L2939-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PHC-326FB-010

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060920\
Data File : BM026304.D
Acq On : 09 Jun 2020 15:17
Operator : JU/CG
Sample : L2939-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PHC-326FB-010

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc