

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060920\
 Data File : BM026305.D
 Acq On : 09 Jun 2020 15:53
 Operator : JU/CG
 Sample : L2939-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PHC-326FB-011

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.069	364	371	382	rBV	1426270	2031479	52.64%	5.073%
2	6.640	630	638	650	rBV	1413207	2144245	55.56%	5.354%
3	7.087	707	714	721	rBV5	15787	40951	1.06%	0.102%
4	7.434	766	773	780	rBV	631985	968365	25.09%	2.418%
5	7.745	819	826	833	rBV	1156506	1754125	45.45%	4.380%
6	7.934	852	858	863	rBV	28061	47070	1.22%	0.118%
7	8.581	961	968	978	rVB	843773	1375340	35.64%	3.434%
8	9.716	1154	1161	1167	rBV5	21978	39026	1.01%	0.097%
9	10.192	1235	1242	1249	rBV	816719	1311340	33.98%	3.274%
10	11.033	1378	1385	1392	rVB2	81373	142150	3.68%	0.355%
11	11.145	1395	1404	1411	rBV3	19920	45206	1.17%	0.113%
12	12.433	1616	1623	1630	rVB2	36937	67024	1.74%	0.167%
13	12.692	1661	1667	1674	rBV	1916942	2806396	72.72%	7.008%
14	13.404	1784	1788	1792	rBV	19770	39223	1.02%	0.098%
15	13.557	1808	1814	1823	rBV	179749	270596	7.01%	0.676%
16	13.798	1852	1855	1864	rVB2	27505	52271	1.35%	0.131%
17	14.086	1898	1904	1912	rVB2	1100830	1597026	41.38%	3.988%
18	15.586	2151	2159	2169	rBV	1586861	2193671	56.84%	5.478%
19	16.839	2366	2372	2376	rBV	1368383	1817465	47.10%	4.538%
20	16.880	2376	2379	2384	rVB2	101237	131456	3.41%	0.328%
21	16.968	2391	2394	2400	rVB	38200	52606	1.36%	0.131%
22	18.033	2570	2575	2579	rBV	375609	486330	12.60%	1.214%
23	18.245	2606	2611	2615	rBV	1161204	1516313	39.29%	3.786%
24	18.280	2615	2617	2623	rVB	128636	146611	3.80%	0.366%
25	18.362	2628	2631	2637	rVB2	94397	120555	3.12%	0.301%
26	18.633	2673	2677	2679	rBV3	175755	257283	6.67%	0.642%
27	18.668	2679	2683	2688	rVB	819619	1077047	27.91%	2.689%
28	18.903	2720	2723	2731	rBV	156341	219375	5.68%	0.548%
29	19.068	2747	2751	2757	rBV2	206567	348987	9.04%	0.871%
30	19.221	2774	2777	2780	rBV	130369	147933	3.83%	0.369%
31	19.268	2783	2785	2789	rVB	147776	153292	3.97%	0.383%
32	19.392	2803	2806	2811	rVB	196550	238873	6.19%	0.596%
33	19.492	2818	2823	2833	rVB	3188438	3859124	100.00%	9.636%
34	20.003	2907	2910	2915	rVB2	334718	370921	9.61%	0.926%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060920\
Data File : BM026305.D
Acq On : 09 Jun 2020 15:53
Operator : JU/CG
Sample : L2939-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PHC-326FB-011

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	20.103	2924	2927	2933	rVB2	186190	246008	6.37%	0.614%
36	20.527	2996	2999	3005	rVB	664546	807805	20.93%	2.017%
37	20.792	3041	3044	3049	rVB2	616068	699927	18.14%	1.748%
38	21.044	3083	3087	3091	rBV	1662626	2117138	54.86%	5.287%
39	21.086	3091	3094	3098	rVB	689873	744120	19.28%	1.858%
40	21.450	3152	3156	3162	rVV	1053775	1208196	31.31%	3.017%
41	21.515	3163	3167	3173	rVB	920426	1147581	29.74%	2.866%
42	22.044	3254	3257	3261	rBV2	596583	780398	20.22%	1.949%
43	22.462	3325	3328	3333	rVB	817062	1060254	27.47%	2.648%
44	23.156	3441	3446	3454	rVB	1301917	2190923	56.77%	5.471%
45	23.709	3537	3540	3551	rVB	653627	1175064	30.45%	2.934%


Sum of corrected areas: 40047089

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060920\
Data File : BM026305.D
Acq On : 09 Jun 2020 15:53
Operator : JU/CG
Sample : L2939-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PHC-326FB-011

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

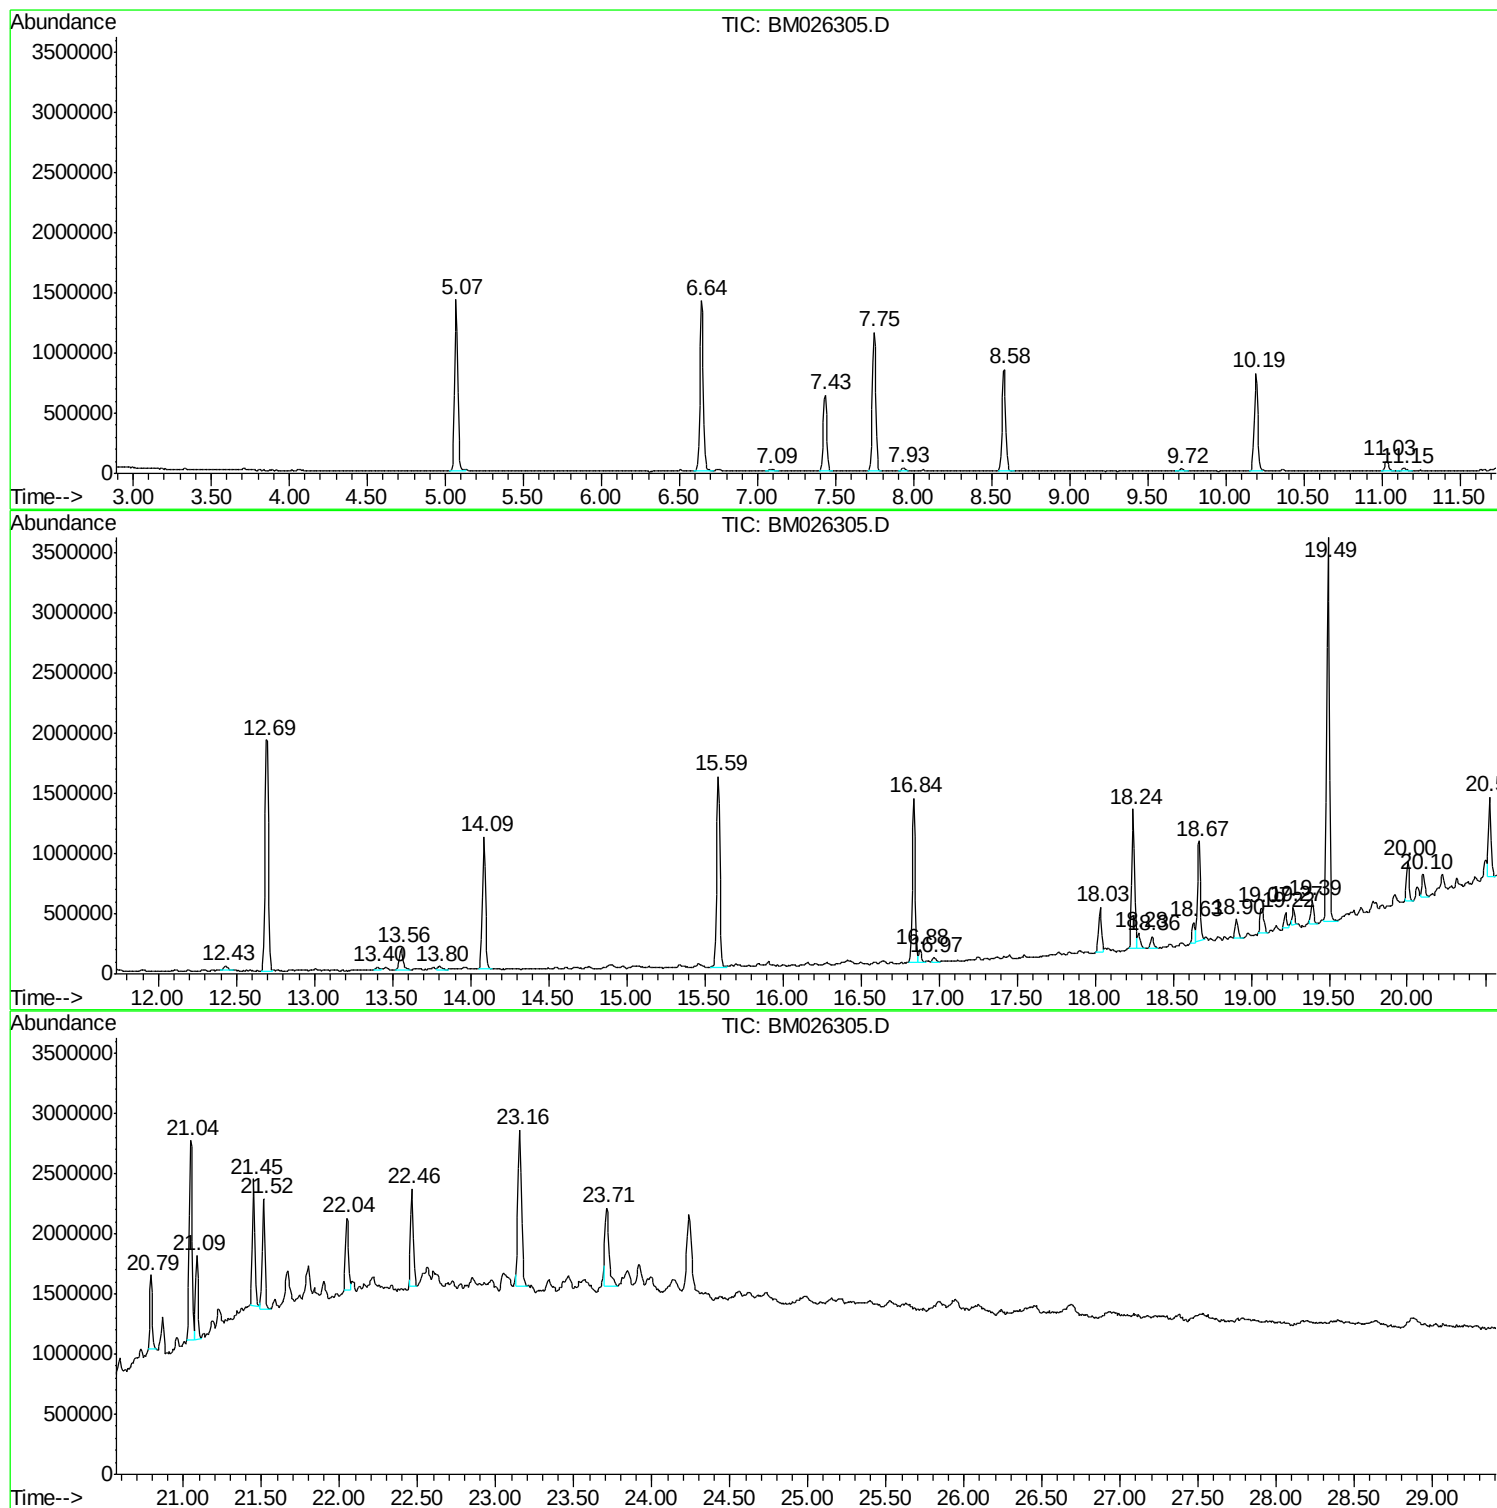

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060920\
Data File : BM026305.D
Acq On : 09 Jun 2020 15:53
Operator : JU/CG
Sample : L2939-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PHC-326FB-011

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060920\
Data File : BM026305.D
Acq On : 09 Jun 2020 15:53
Operator : JU/CG
Sample : L2939-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PHC-326FB-011

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc