


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060920\
 Data File : BM026300.D
 Acq On : 09 Jun 2020 12:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 09 14:46:47 2020

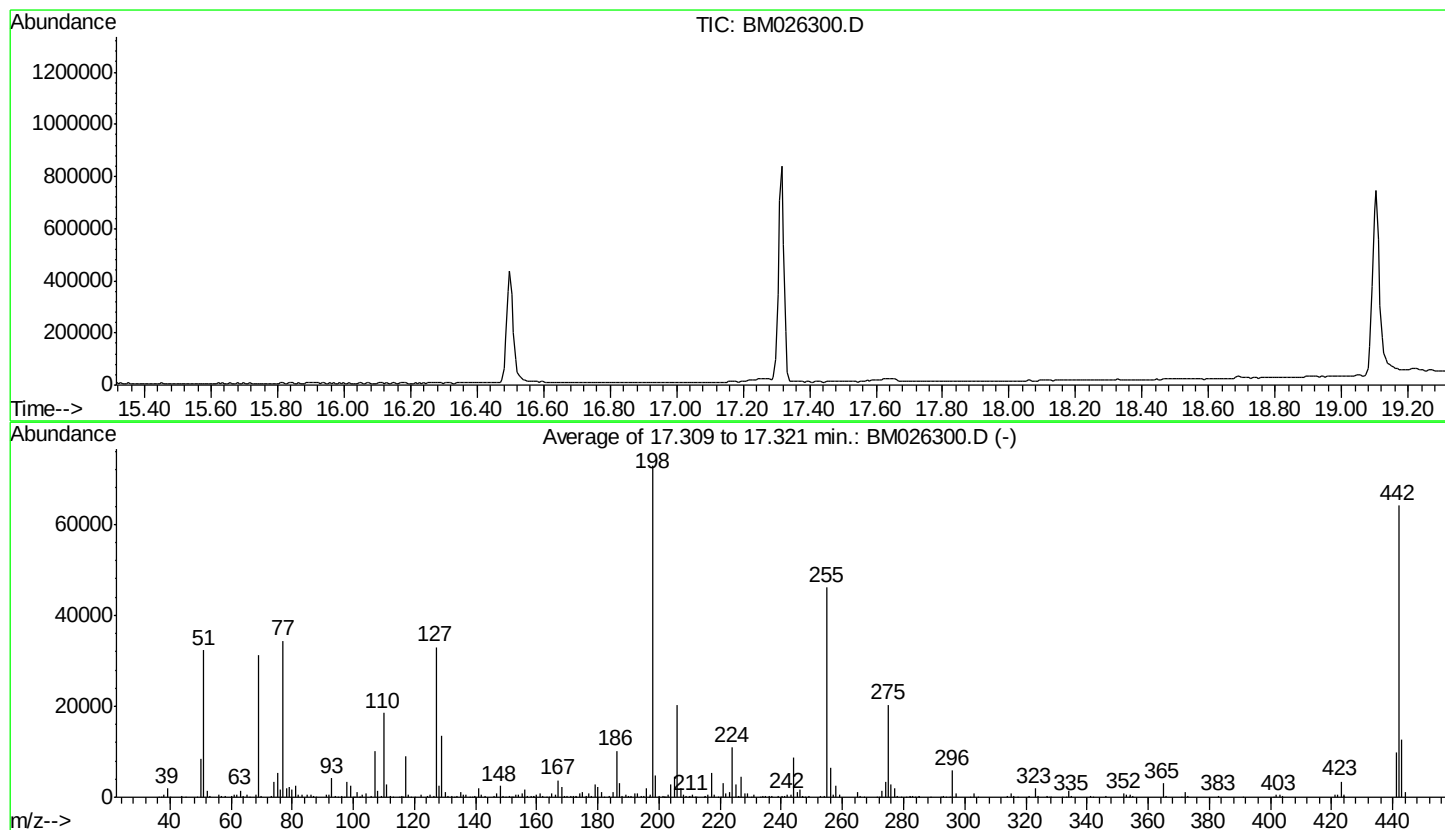

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	32270	PASS
68	69	0.00	2	1.9	587	PASS
69	198	0.00	100	42.8	31221	PASS
70	69	0.00	2	0.6	200	PASS
127	198	10	80	45.3	33032	PASS
197	198	0.00	2	0.6	465	PASS
198	198	100	100	100.0	72912	PASS
199	198	5	9	6.7	4911	PASS
275	198	10	60	28.0	20389	PASS
365	198	1	100	4.2	3079	PASS
441	198	0.01	100	13.5	9876	PASS
442	198	50	100	88.0	64146	PASS
443	442	15	24	19.8	12671	PASS