


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060920\
 Data File : BM026308.D
 Acq On : 09 Jun 2020 18:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 09 14:46:47 2020

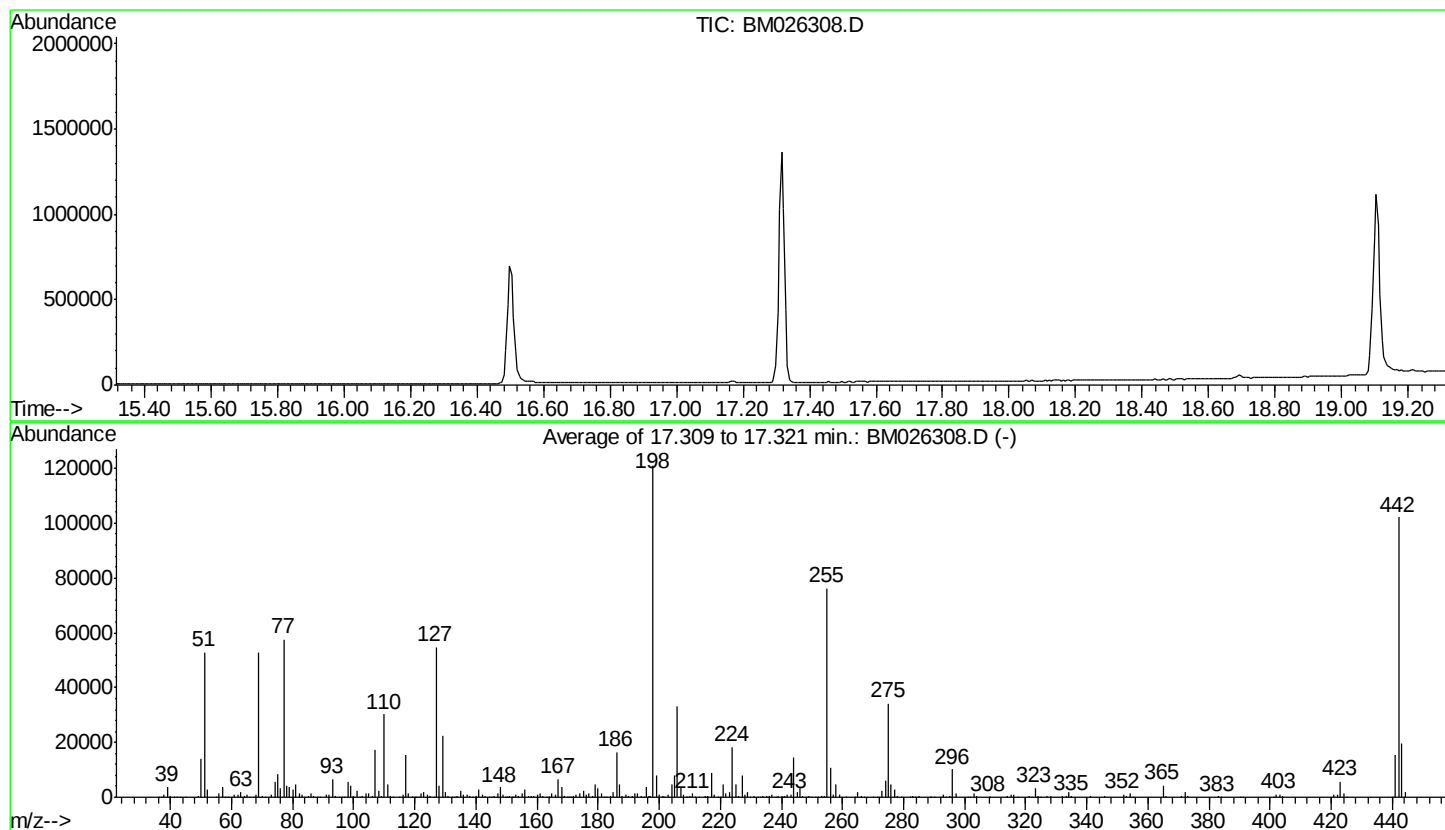

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	52843	PASS
68	69	0.00	2	2.0	1049	PASS
69	198	0.00	100	43.5	52653	PASS
70	69	0.00	2	0.6	313	PASS
127	198	10	80	45.3	54829	PASS
197	198	0.00	2	0.5	575	PASS
198	198	100	100	100.0	120962	PASS
199	198	5	9	6.6	7955	PASS
275	198	10	60	28.2	34152	PASS
365	198	1	100	3.7	4433	PASS
441	198	0.01	100	12.8	15523	PASS
442	198	50	100	84.5	102205	PASS
443	442	15	24	19.4	19798	PASS