

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050237.D
Acq On : 09 Jun 2025 11:26
Operator : RC/JU
Sample : PB168340BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB168340BL

Quant Time: Jun 09 12:21:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	308898	20.000	ng	0.00
21) Naphthalene-d8	10.557	136	1157442	20.000	ng	0.00
39) Acenaphthene-d10	14.398	164	647360	20.000	ng	0.00
64) Phenanthrene-d10	17.133	188	1268443	20.000	ng	0.00
76) Chrysene-d12	21.368	240	1357312	20.000	ng	0.00
86) Perylene-d12	24.344	264	1477668	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	2728386	147.341	ng	0.00
7) Phenol-d6	6.934	99	3343794	137.173	ng	0.00
23) Nitrobenzene-d5	8.916	82	1971126	88.570	ng	0.00
42) 2,4,6-Tribromophenol	15.880	330	1112019	151.023	ng	0.00
45) 2-Fluorobiphenyl	13.027	172	4271637	89.335	ng	0.00
79) Terphenyl-d14	19.768	244	6189153	86.410	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050237.D
Acq On : 09 Jun 2025 11:26
Operator : RC/JU
Sample : PB168340BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB168340BL

Quant Time: Jun 09 12:21:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

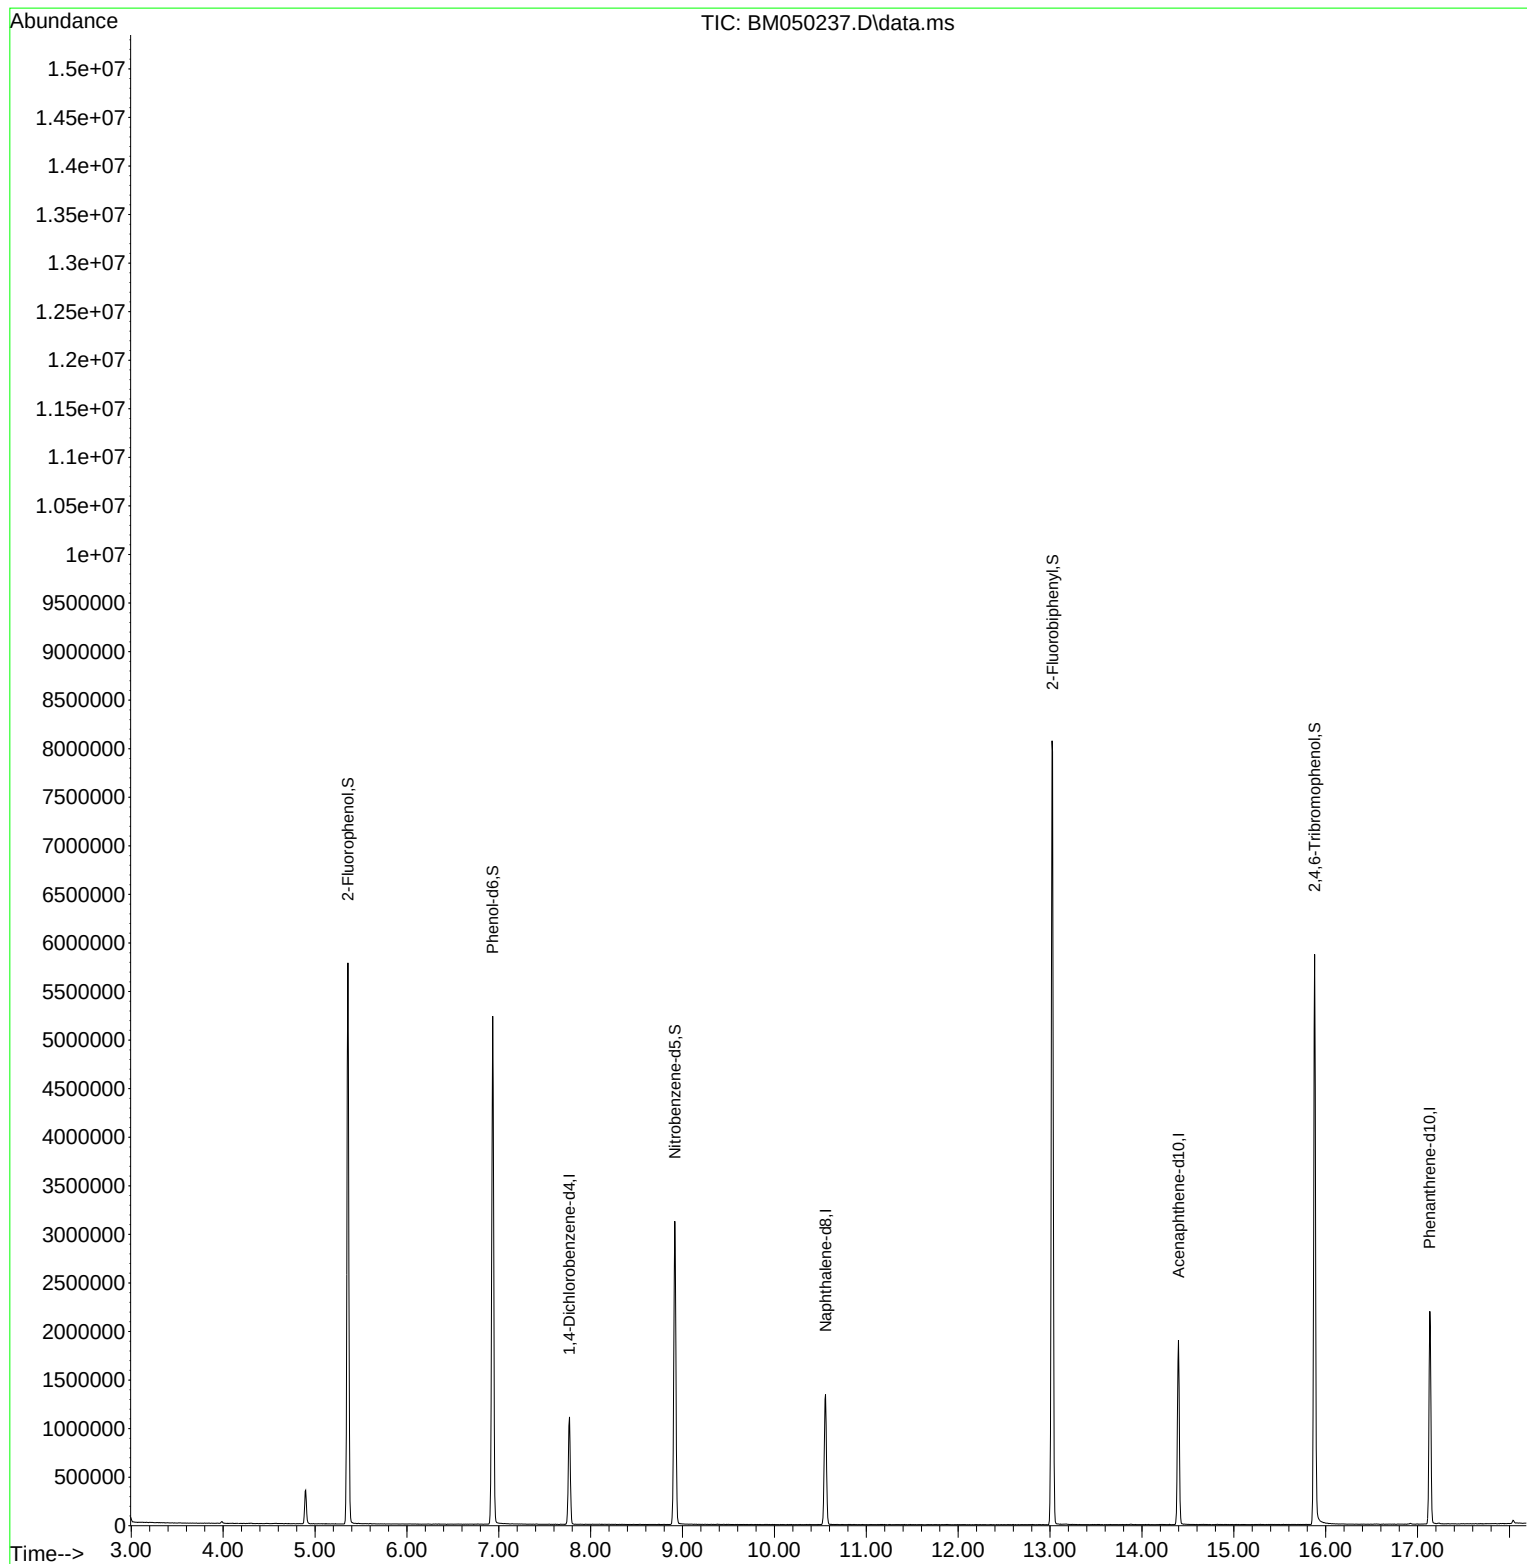

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050237.D
Acq On : 09 Jun 2025 11:26
Operator : RC/JU
Sample : PB168340BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB168340BL

Quant Time: Jun 09 12:21:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

