

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
 Data File : BM050240.D
 Acq On : 09 Jun 2025 13:29
 Operator : RC/JU
 Sample : Q2125-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GSB3

Quant Time: Jun 09 14:03:19 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 09 11:54:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	258819	20.000	ng	0.00
21) Naphthalene-d8	10.551	136	1009931	20.000	ng	0.00
39) Acenaphthene-d10	14.398	164	581596	20.000	ng	0.00
64) Phenanthrene-d10	17.133	188	1095565	20.000	ng	0.00
76) Chrysene-d12	21.362	240	1122304	20.000	ng	-0.01
86) Perylene-d12	24.338	264	1282474	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.351	112	1263506	81.436	ng	0.00
7) Phenol-d6	6.928	99	987737	48.360	ng	0.00
23) Nitrobenzene-d5	8.916	82	1883291	96.983	ng	0.00
42) 2,4,6-Tribromophenol	15.880	330	1022118	154.510	ng	0.00
45) 2-Fluorobiphenyl	13.022	172	3795297	88.348	ng	0.00
79) Terphenyl-d14	19.762	244	5334082	90.067	ng	0.00
Target Compounds						
						Qvalue
37) 2-Methylnaphthalene	12.216	142	628927	19.966	ng	99
38) 1-Methylnaphthalene	12.439	142	813617	24.335	ng	100
50) Dimethylphthalate	13.857	163	1440398	36.620	ng	100
52) Acenaphthene	14.463	154	101935	2.976	ng	96
55) Dibenzofuran	14.798	168	110355	2.202	ng	# 64
58) Fluorene	15.445	166	176099	4.588	ng	# 94
60) Diethylphthalate	15.221	149	548102	14.044	ng	99
70) Pentachlorophenol	16.786	266	20129	2.268	ng	93
71) Phenanthrene	17.174	178	297659	4.756	ng	98
74) Di-n-butylphthalate	18.115	149	638718	10.291	ng	99
78) Pyrene	19.550	202	167785	2.218	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050240.D
Acq On : 09 Jun 2025 13:29
Operator : RC/JU
Sample : Q2125-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GSB3

Quant Time: Jun 09 14:03:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

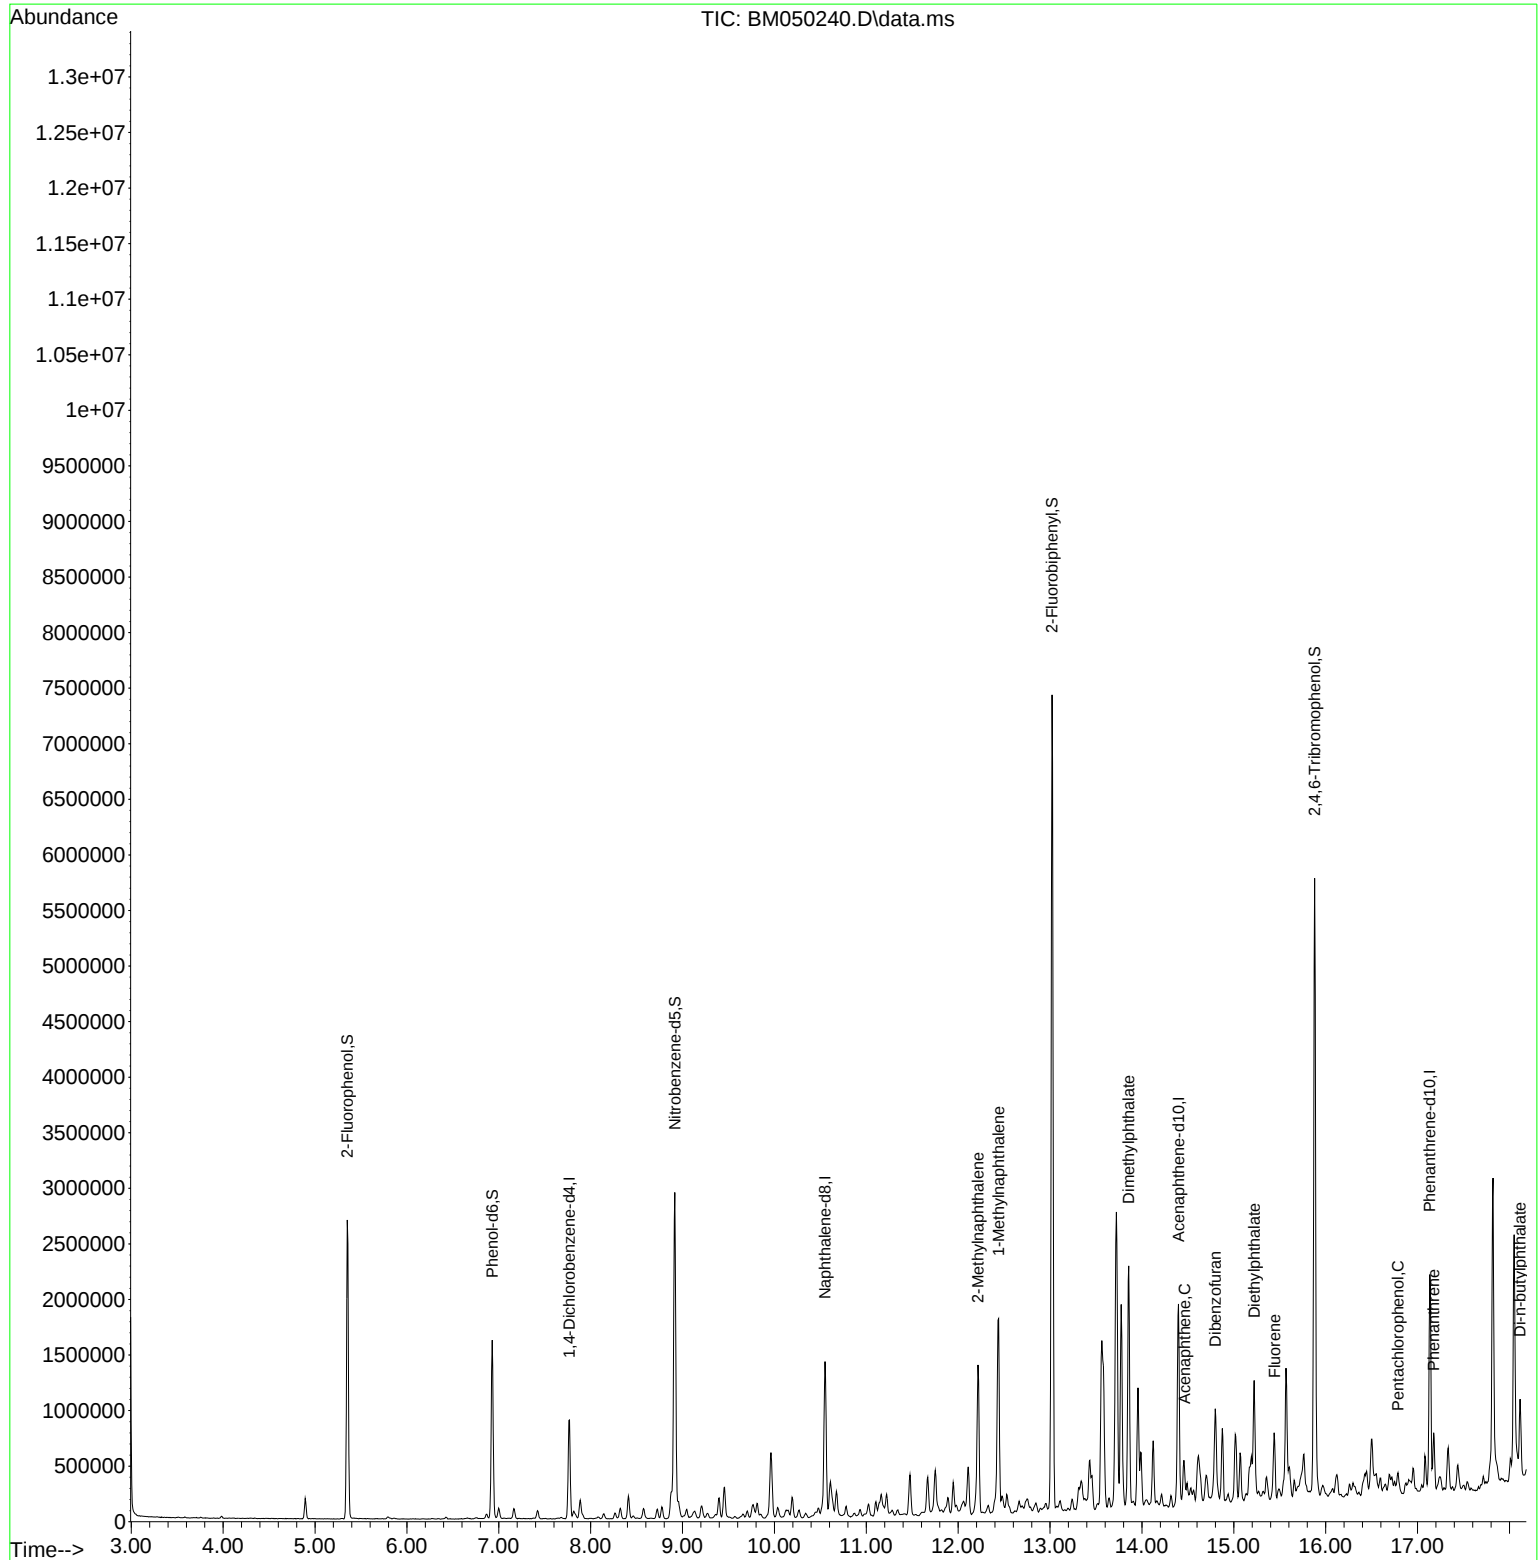

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050240.D
Acq On : 09 Jun 2025 13:29
Operator : RC/JU
Sample : Q2125-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GSB3

Quant Time: Jun 09 14:03:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

