

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
 Data File : BM050243.D
 Acq On : 09 Jun 2025 15:39
 Operator : RC/JU
 Sample : Q2226-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP06-MHI-WC

Quant Time: Jun 09 18:03:36 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 09 11:54:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	247754	20.000	ng	0.00
21) Naphthalene-d8	10.551	136	951828	20.000	ng	0.00
39) Acenaphthene-d10	14.398	164	560933	20.000	ng	0.00
64) Phenanthrene-d10	17.133	188	1131568	20.000	ng	0.00
76) Chrysene-d12	21.368	240	1170195	20.000	ng	0.00
86) Perylene-d12	24.344	264	1198696	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.352	112	1845574	124.264	ng	0.00
7) Phenol-d6	6.928	99	2157993	110.375	ng	0.00
23) Nitrobenzene-d5	8.916	82	1475680	80.632	ng	0.00
42) 2,4,6-Tribromophenol	15.880	330	929059	145.616	ng	0.00
45) 2-Fluorobiphenyl	13.022	172	3258348	78.642	ng	0.00
79) Terphenyl-d14	19.762	244	4763358	77.138	ng	0.00
Target Compounds						
74) Di-n-butylphthalate	18.115	149	196233	3.061	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050243.D
Acq On : 09 Jun 2025 15:39
Operator : RC/JU
Sample : Q2226-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP06-MHI-WC

Quant Time: Jun 09 18:03:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

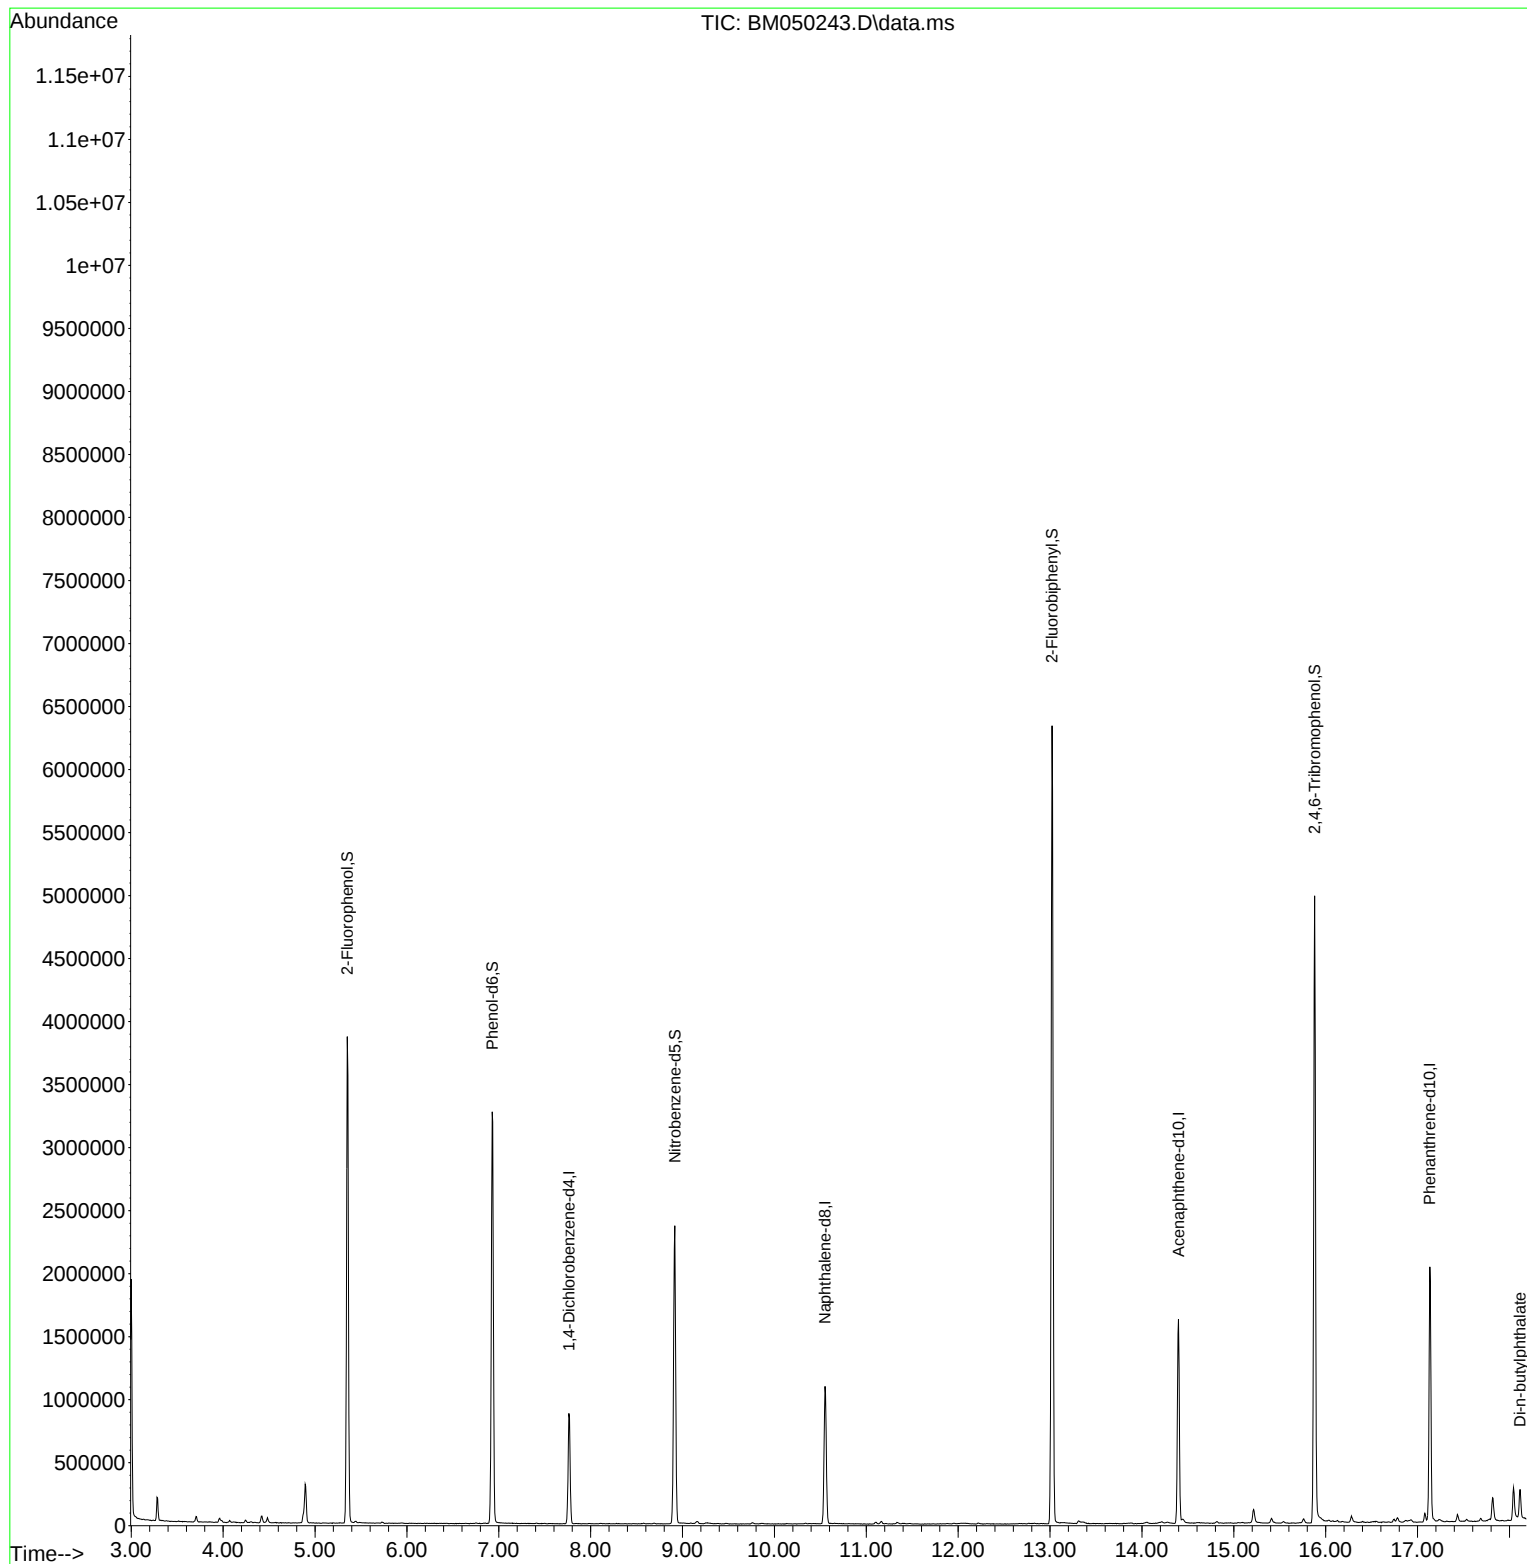

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050243.D
Acq On : 09 Jun 2025 15:39
Operator : RC/JU
Sample : Q2226-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP06-MHI-WC

Quant Time: Jun 09 18:03:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

