

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050257.D
Acq On : 10 Jun 2025 00:54
Operator : RC/JU
Sample : Q2241-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-N

Quant Time: Jun 10 02:45:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	341683	20.000	ng	0.00
21) Naphthalene-d8	10.551	136	1294464	20.000	ng	0.00
39) Acenaphthene-d10	14.398	164	727849	20.000	ng	0.00
64) Phenanthrene-d10	17.133	188	1368430	20.000	ng	0.00
76) Chrysene-d12	21.362	240	1266156	20.000	ng	-0.01
86) Perylene-d12	24.339	264	1292650	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	2659752	129.853	ng	0.00
7) Phenol-d6	6.934	99	3007408	111.535	ng	0.00
23) Nitrobenzene-d5	8.916	82	2141465	86.038	ng	0.00
42) 2,4,6-Tribromophenol	15.880	330	1157919	139.866	ng	0.00
45) 2-Fluorobiphenyl	13.022	172	4317303	80.305	ng	0.00
79) Terphenyl-d14	19.762	244	5527795	82.733	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050257.D
Acq On : 10 Jun 2025 00:54
Operator : RC/JU
Sample : Q2241-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-N

Quant Time: Jun 10 02:45:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

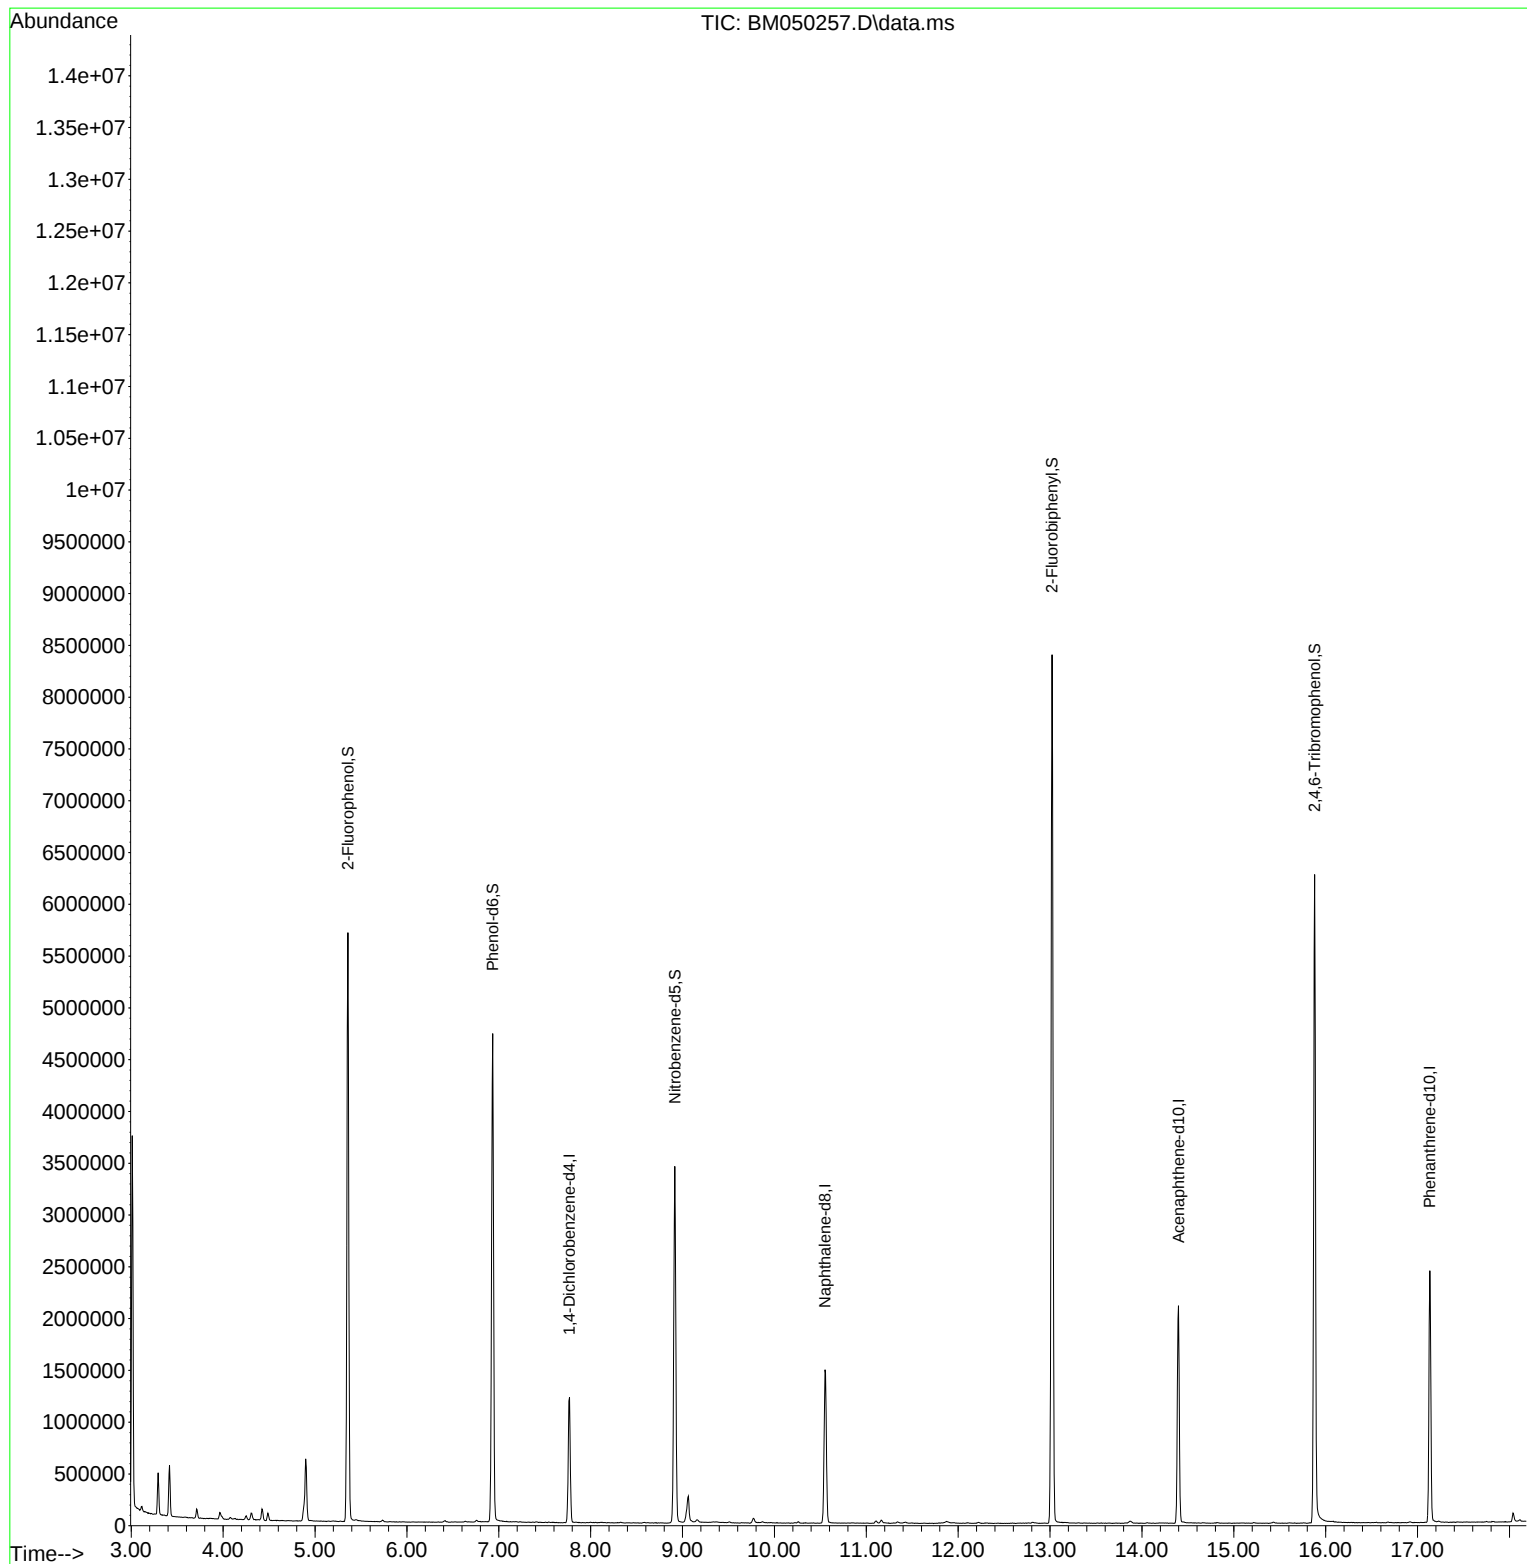

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050257.D
Acq On : 10 Jun 2025 00:54
Operator : RC/JU
Sample : Q2241-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-N

Quant Time: Jun 10 02:45:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

