

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
 Data File : BM050258.D
 Acq On : 10 Jun 2025 01:33
 Operator : RC/JU
 Sample : Q2241-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-S

Quant Time: Jun 10 02:46:00 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 09 11:54:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	330437	20.000	ng	0.00
21) Naphthalene-d8	10.551	136	1247685	20.000	ng	0.00
39) Acenaphthene-d10	14.398	164	684088	20.000	ng	0.00
64) Phenanthrene-d10	17.133	188	1275149	20.000	ng	0.00
76) Chrysene-d12	21.362	240	1269974	20.000	ng	-0.01
86) Perylene-d12	24.338	264	1345088	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	2598965	131.203	ng	0.00
7) Phenol-d6	6.934	99	2922010	112.056	ng	0.00
23) Nitrobenzene-d5	8.916	82	2196705	91.567	ng	0.00
42) 2,4,6-Tribromophenol	15.880	330	1052708	135.292	ng	0.00
45) 2-Fluorobiphenyl	13.022	172	4322201	85.539	ng	0.00
79) Terphenyl-d14	19.762	244	5799289	86.535	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050258.D
Acq On : 10 Jun 2025 01:33
Operator : RC/JU
Sample : Q2241-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-S

Quant Time: Jun 10 02:46:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

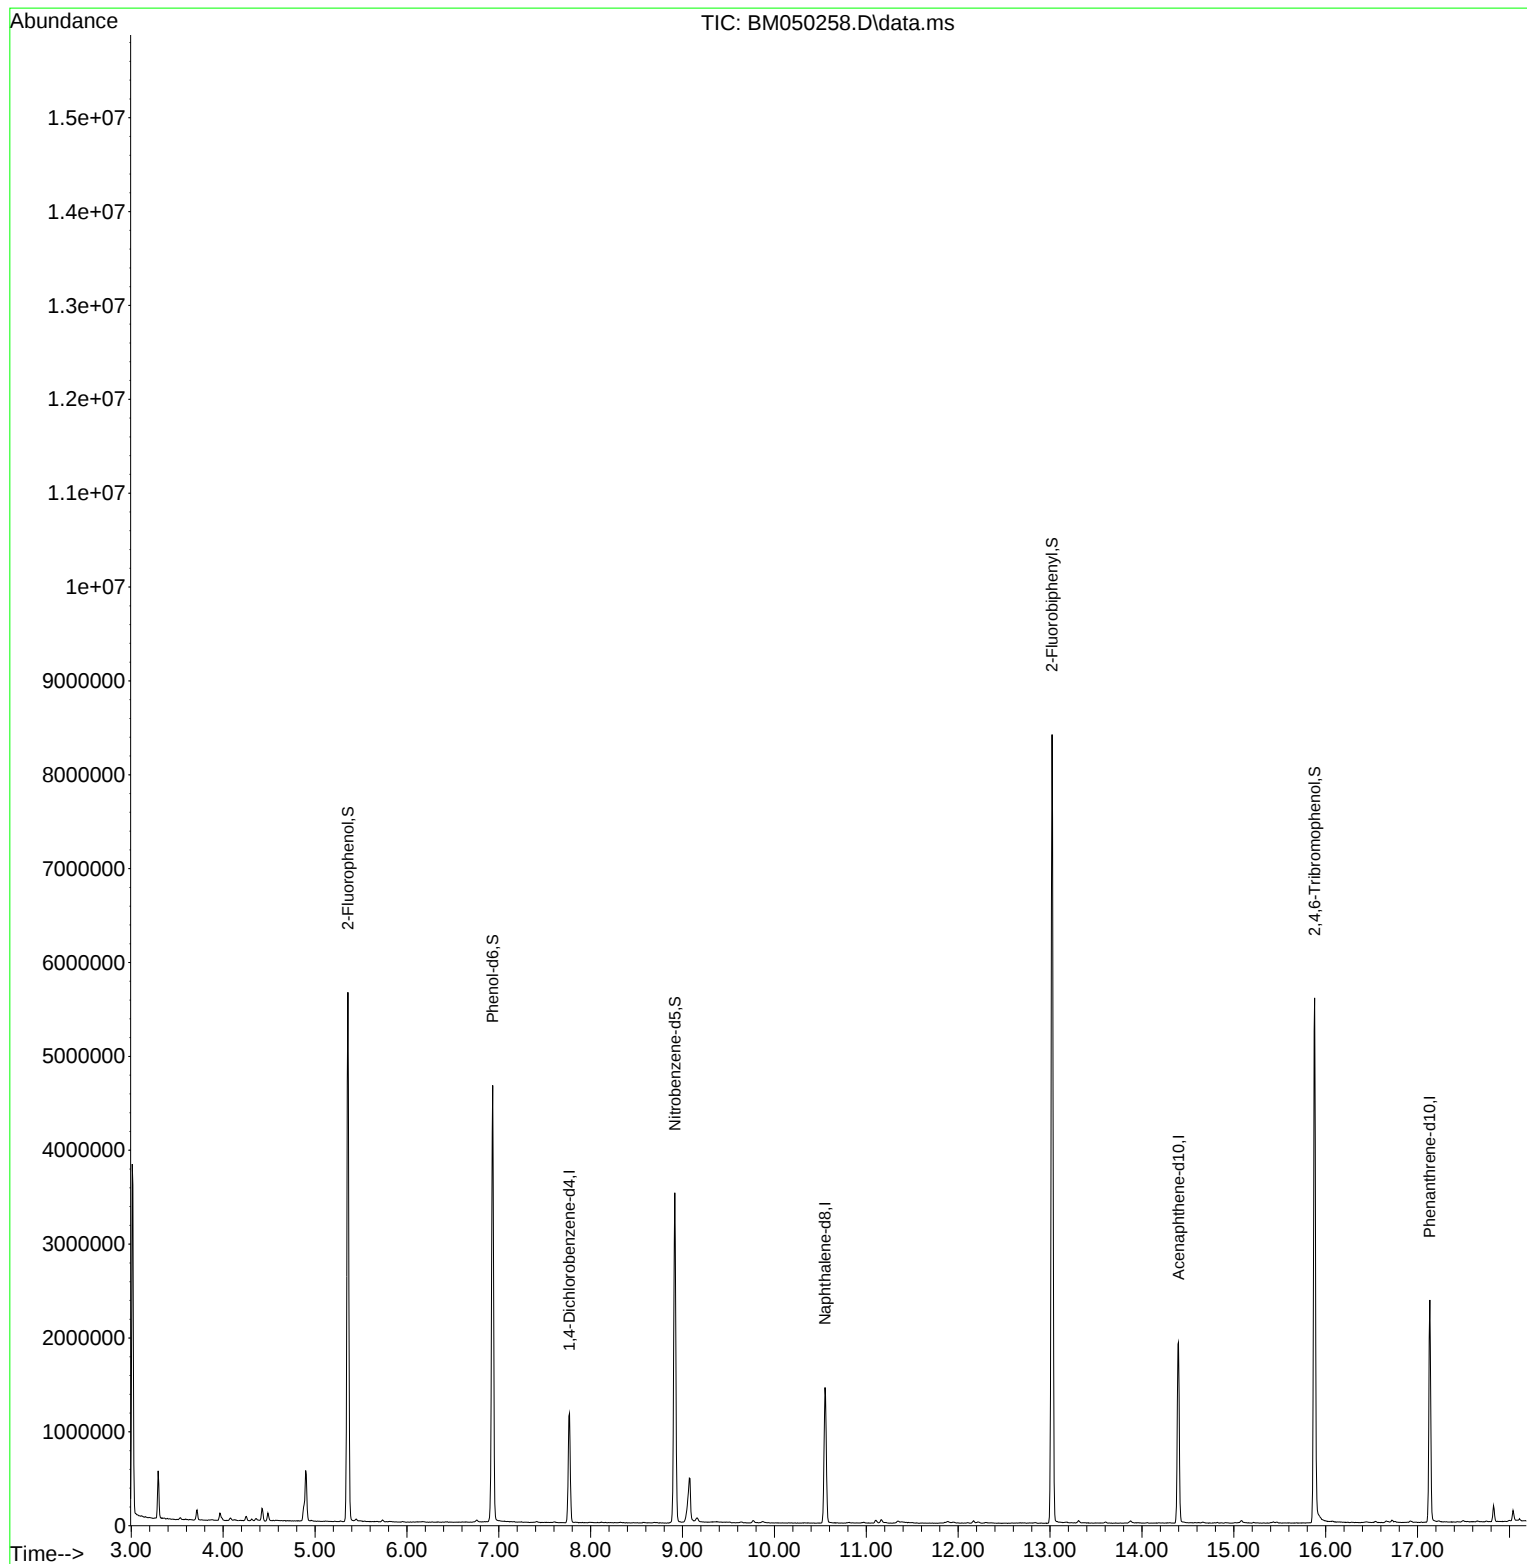

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050258.D
Acq On : 10 Jun 2025 01:33
Operator : RC/JU
Sample : Q2241-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-S

Quant Time: Jun 10 02:46:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

