

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM060925\  
 Data File : BM050266.D  
 Acq On : 10 Jun 2025 07:25  
 Operator : RC/JU  
 Sample : Q2242-04  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 TP09-MHJ

Quant Time: Jun 10 08:00:50 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM060525.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Jun 09 11:54:38 2025  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc    | Units | Dev(Min) |
|-----------------------------|--------|------|----------|---------|-------|----------|
| -----                       |        |      |          |         |       |          |
| Internal Standards          |        |      |          |         |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.769  | 152  | 378144   | 20.000  | ng    | 0.00     |
| 21) Naphthalene-d8          | 10.551 | 136  | 1426774  | 20.000  | ng    | 0.00     |
| 39) Acenaphthene-d10        | 14.392 | 164  | 770403   | 20.000  | ng    | 0.00     |
| 64) Phenanthrene-d10        | 17.133 | 188  | 1411866  | 20.000  | ng    | 0.00     |
| 76) Chrysene-d12            | 21.362 | 240  | 1364339  | 20.000  | ng    | -0.01    |
| 86) Perylene-d12            | 24.338 | 264  | 1393729  | 20.000  | ng    | 0.00     |
| System Monitoring Compounds |        |      |          |         |       |          |
| 5) 2-Fluorophenol           | 5.357  | 112  | 3133912  | 138.249 | ng    | 0.00     |
| 7) Phenol-d6                | 6.934  | 99   | 3601411  | 120.686 | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 8.916  | 82   | 2618225  | 95.438  | ng    | 0.00     |
| 42) 2,4,6-Tribromophenol    | 15.880 | 330  | 1256160  | 143.352 | ng    | 0.00     |
| 45) 2-Fluorobiphenyl        | 13.022 | 172  | 5145824  | 90.429  | ng    | 0.00     |
| 79) Terphenyl-d14           | 19.762 | 244  | 6410059  | 89.034  | ng    | 0.00     |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM060925\  
Data File : BM050266.D  
Acq On : 10 Jun 2025 07:25  
Operator : RC/JU  
Sample : Q2242-04  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
TP09-MHJ

Quant Time: Jun 10 08:00:50 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM060525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jun 09 11:54:38 2025  
Response via : Initial Calibration

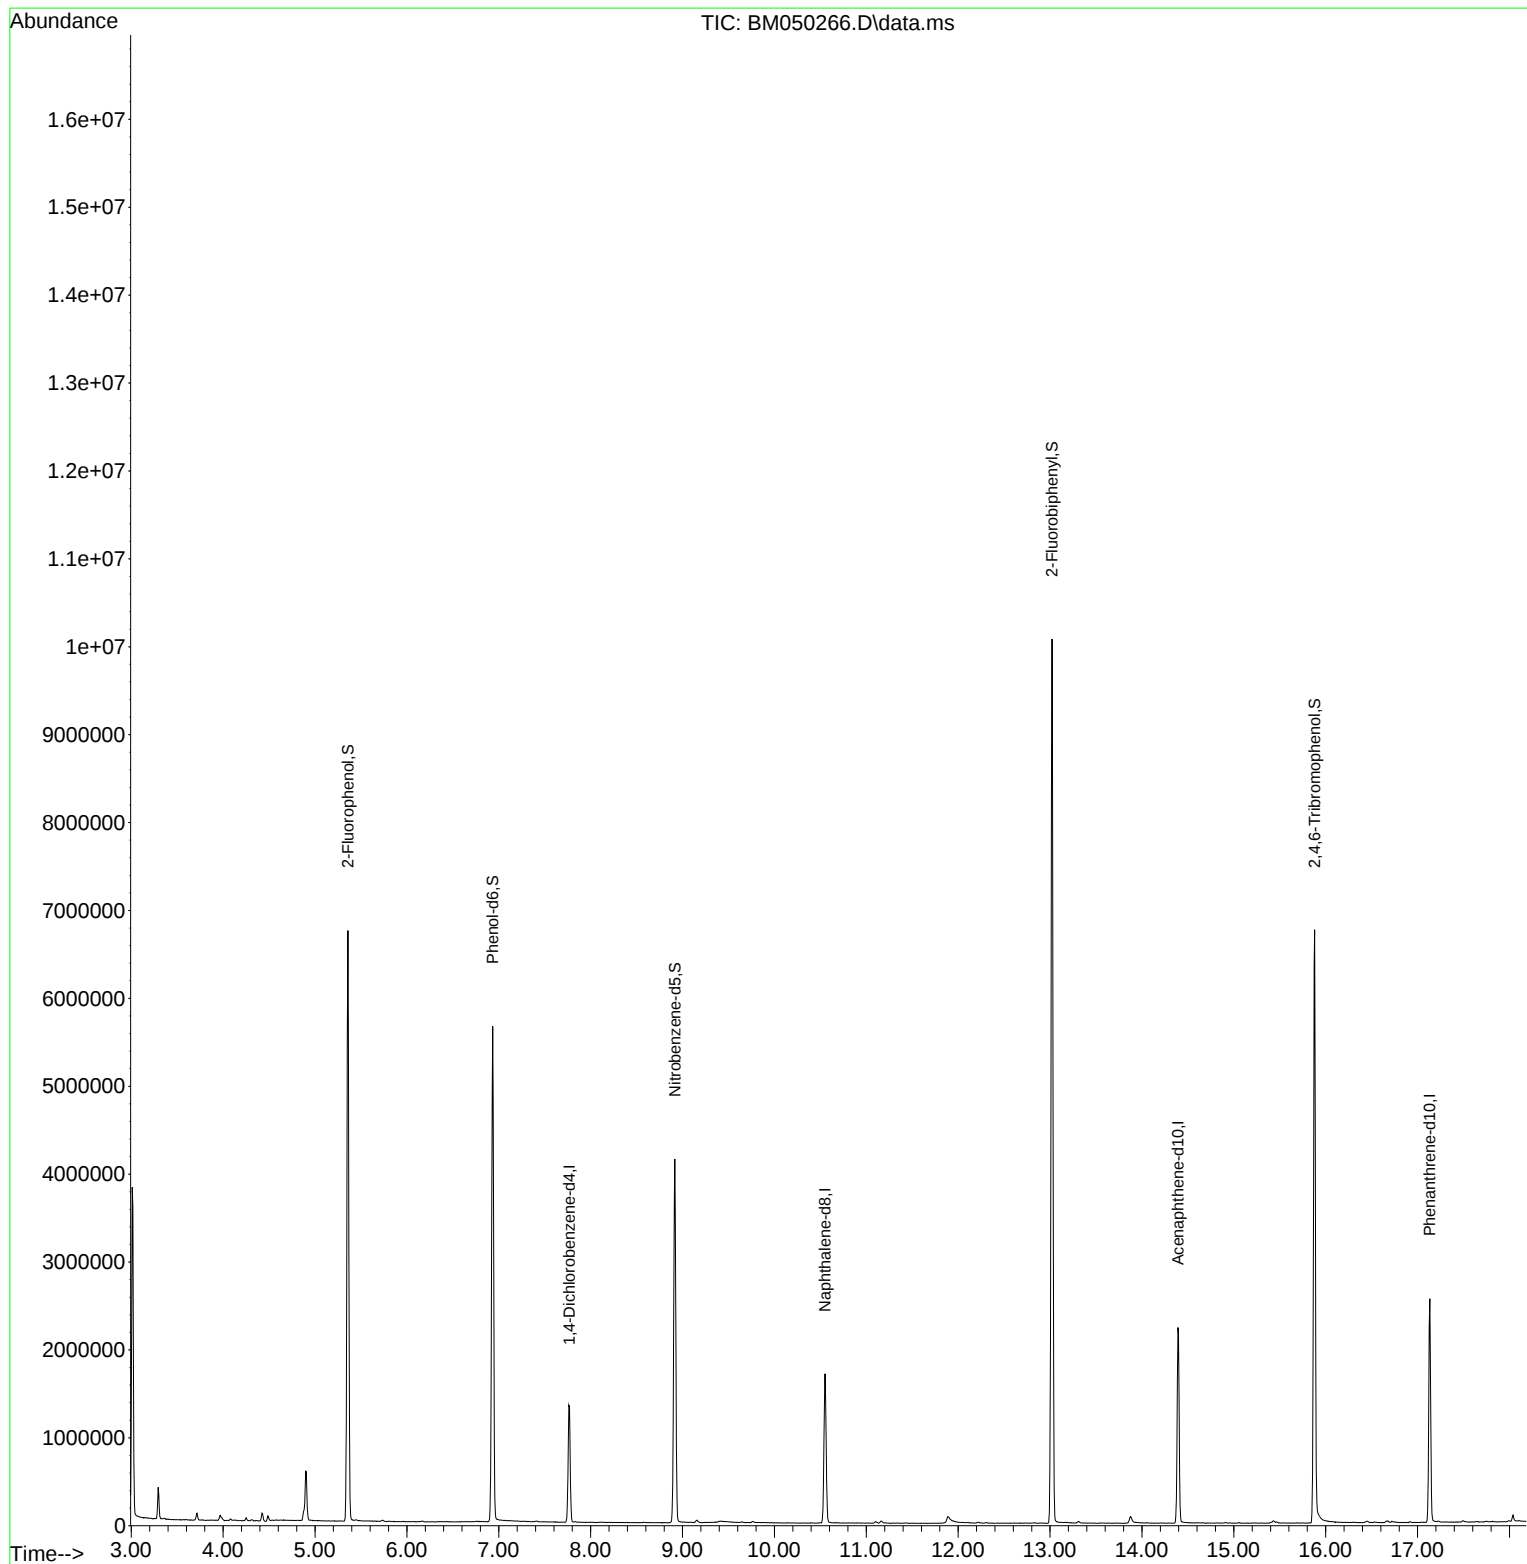

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM060925\  
Data File : BM050266.D  
Acq On : 10 Jun 2025 07:25  
Operator : RC/JU  
Sample : Q2242-04  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
TP09-MHJ

Quant Time: Jun 10 08:00:50 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM060525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jun 09 11:54:38 2025  
Response via : Initial Calibration

