

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
 Data File : BM050272.D
 Acq On : 10 Jun 2025 11:20
 Operator : RC/JU
 Sample : Q2240-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-1

Quant Time: Jun 10 11:56:25 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 09 11:54:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	328626	20.000	ng	0.00
21) Naphthalene-d8	10.551	136	1237861	20.000	ng	0.00
39) Acenaphthene-d10	14.392	164	601449	20.000	ng	0.00
64) Phenanthrene-d10	17.133	188	1172270	20.000	ng	0.00
76) Chrysene-d12	21.362	240	1033423	20.000	ng	-0.01
86) Perylene-d12	24.333	264	237701	20.000	ng	#-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	2857853	145.068	ng	0.00
7) Phenol-d6	6.934	99	3123222	120.433	ng	0.00
23) Nitrobenzene-d5	8.916	82	2288323	96.143	ng	0.00
42) 2,4,6-Tribromophenol	15.880	330	1046315	152.946	ng	0.00
45) 2-Fluorobiphenyl	13.022	172	4380014	98.593	ng	0.00
79) Terphenyl-d14	19.762	244	5661847	103.823	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050272.D
Acq On : 10 Jun 2025 11:20
Operator : RC/JU
Sample : Q2240-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-1

Quant Time: Jun 10 11:56:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

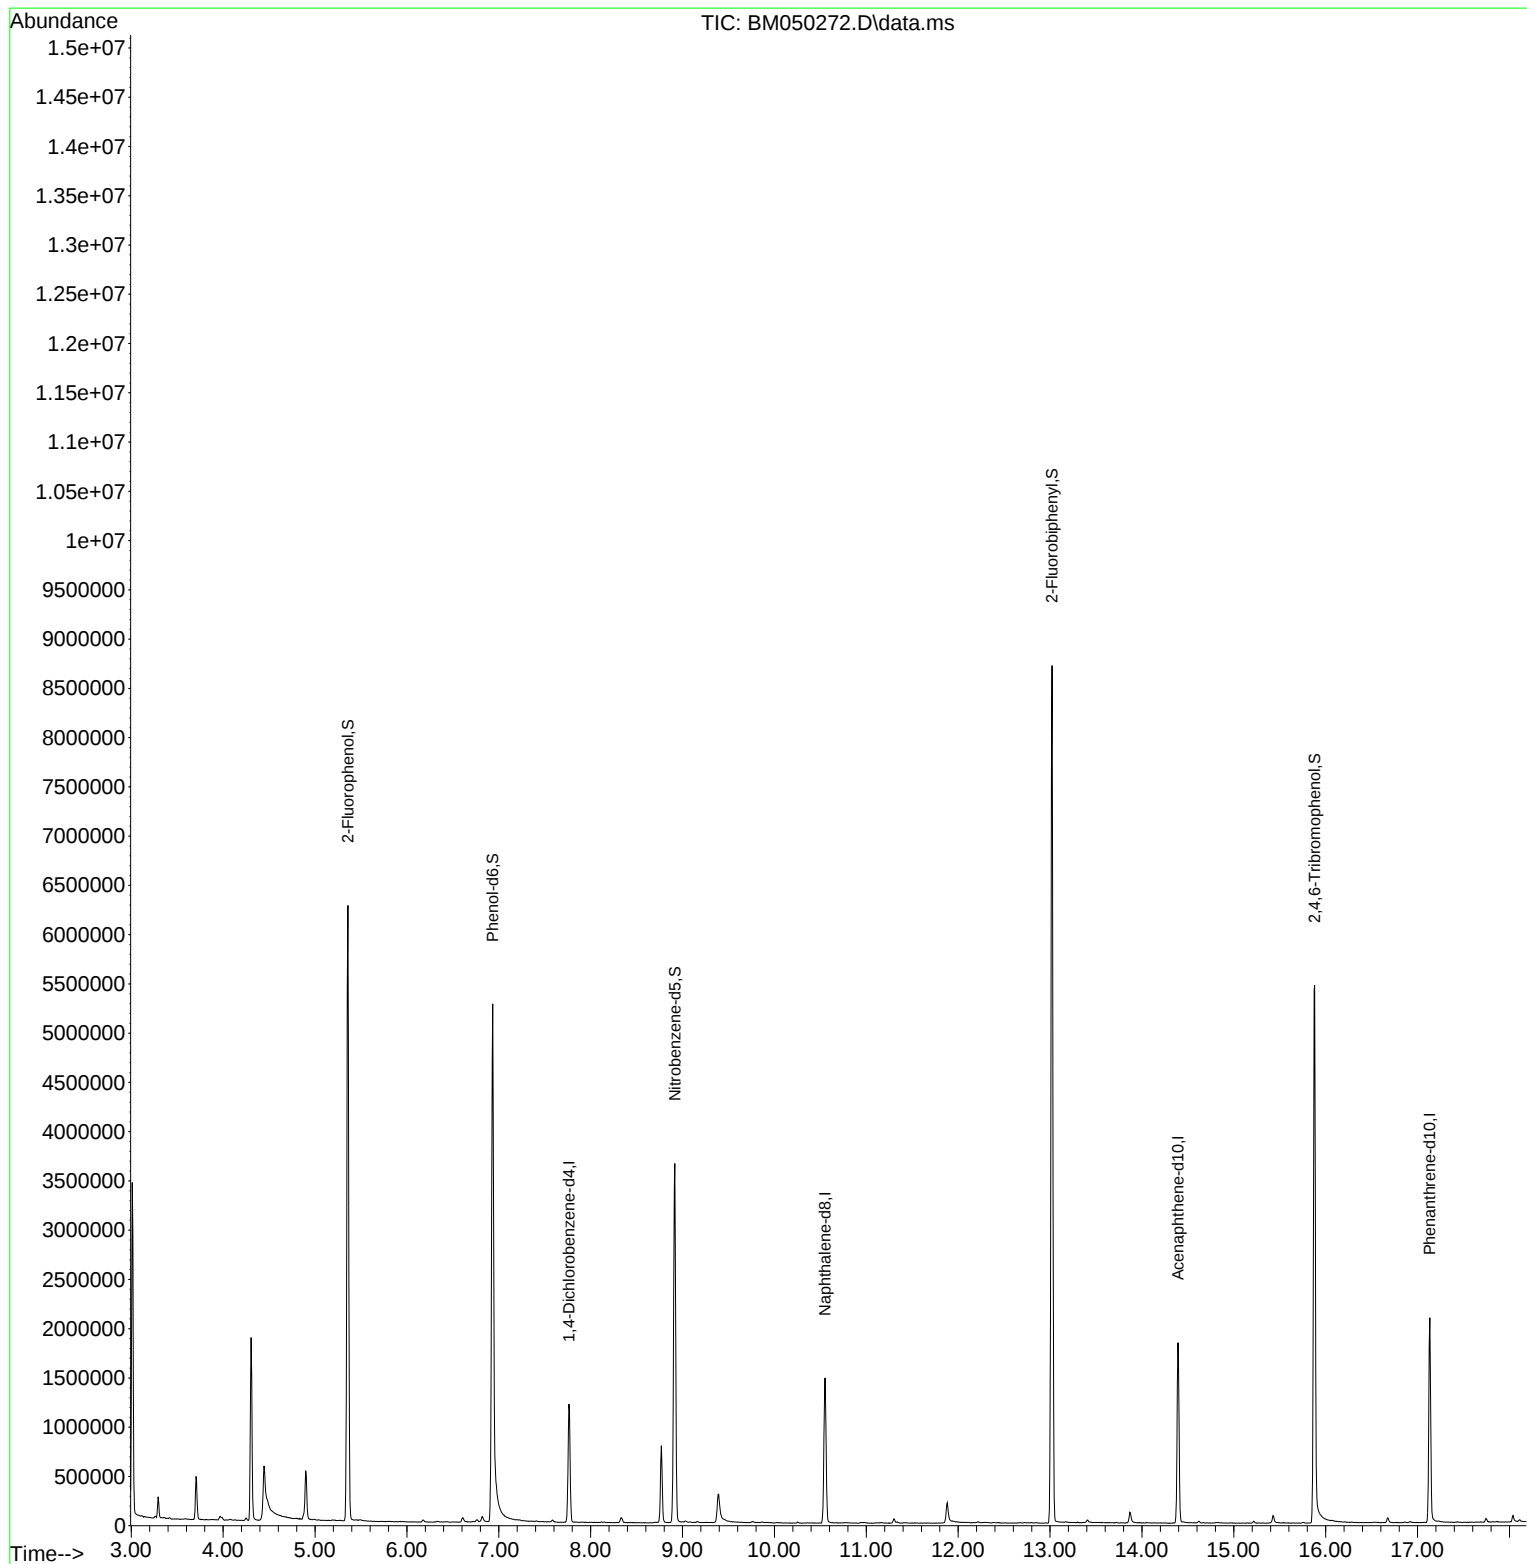

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050272.D
Acq On : 10 Jun 2025 11:20
Operator : RC/JU
Sample : Q2240-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-1

Quant Time: Jun 10 11:56:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

