

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
 Data File : BM050275.D
 Acq On : 10 Jun 2025 13:28
 Operator : RC/JU
 Sample : Q2231-02DL2 50X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MW-14-20250604DL2

Quant Time: Jun 10 16:35:47 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 09 11:54:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	323093	20.000	ng	0.00
21) Naphthalene-d8	10.551	136	1225983	20.000	ng	0.00
39) Acenaphthene-d10	14.392	164	643043	20.000	ng	0.00
64) Phenanthrene-d10	17.133	188	1187200	20.000	ng	0.00
76) Chrysene-d12	21.362	240	1262062	20.000	ng	-0.01
86) Perylene-d12	24.338	264	1332608	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.351	112	26344	1.360	ng	0.00
7) Phenol-d6	6.928	99	19909	0.781	ng	0.00
23) Nitrobenzene-d5	8.910	82	36491	1.548	ng	0.00
42) 2,4,6-Tribromophenol	15.880	330	12636	1.728	ng	0.00
45) 2-Fluorobiphenyl	13.016	172	90196	1.899	ng	-0.01
79) Terphenyl-d14	19.762	244	121962	1.831	ng	0.00
Target Compounds						Qvalue
31) Naphthalene	10.598	128	2724515	42.983	ng	100
37) 2-Methylnaphthalene	12.216	142	281390	7.359	ng	98
38) 1-Methylnaphthalene	12.433	142	386014	9.511	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050275.D
Acq On : 10 Jun 2025 13:28
Operator : RC/JU
Sample : Q2231-02DL2 50X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-14-20250604DL2

Quant Time: Jun 10 16:35:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

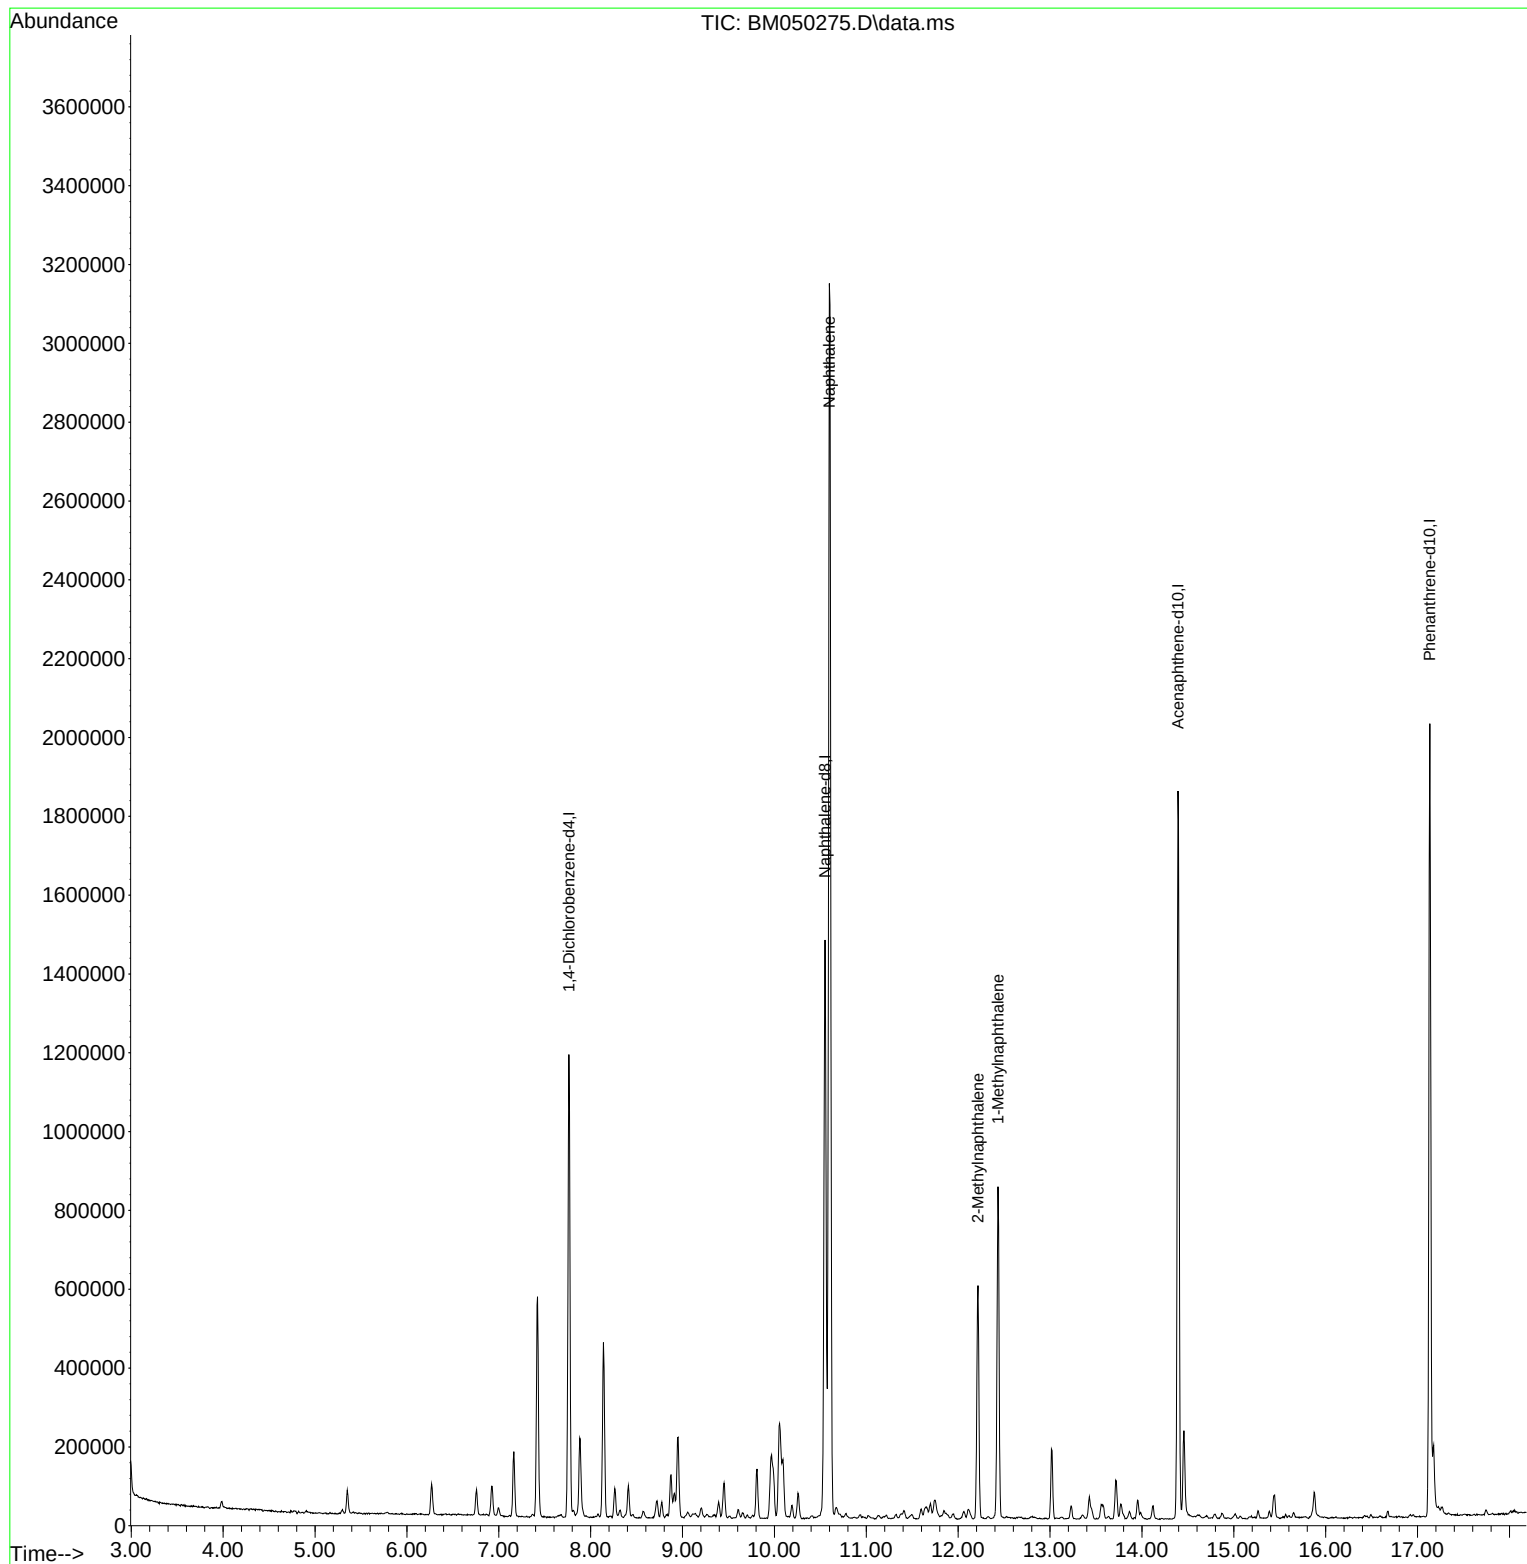

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050275.D
Acq On : 10 Jun 2025 13:28
Operator : RC/JU
Sample : Q2231-02DL2 50X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-14-20250604DL2

Quant Time: Jun 10 16:35:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

