
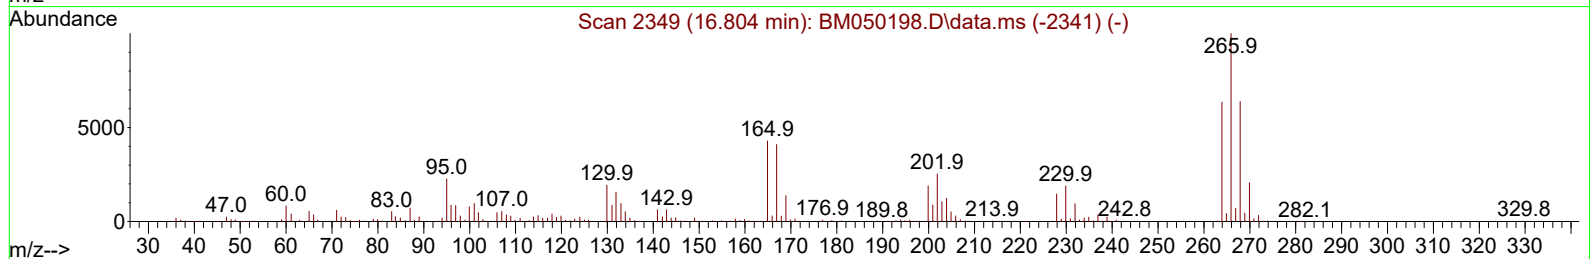
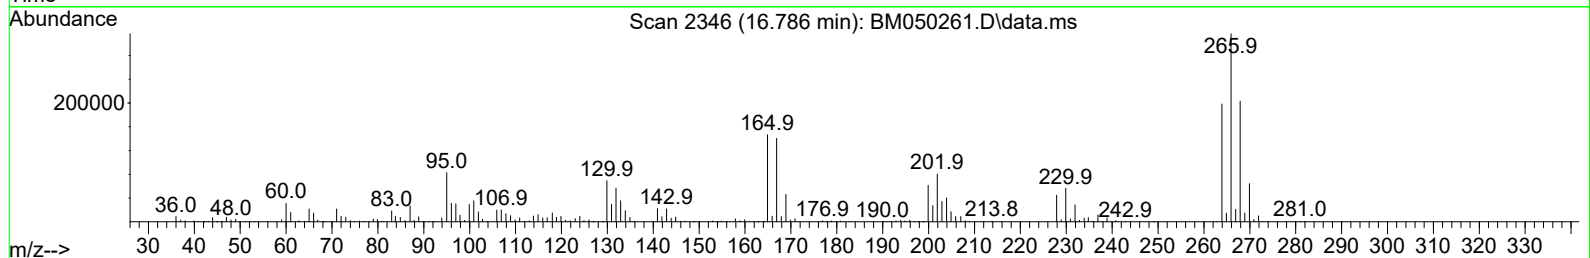


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050261.D
Acq On : 10 Jun 2025 04:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 05:34:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

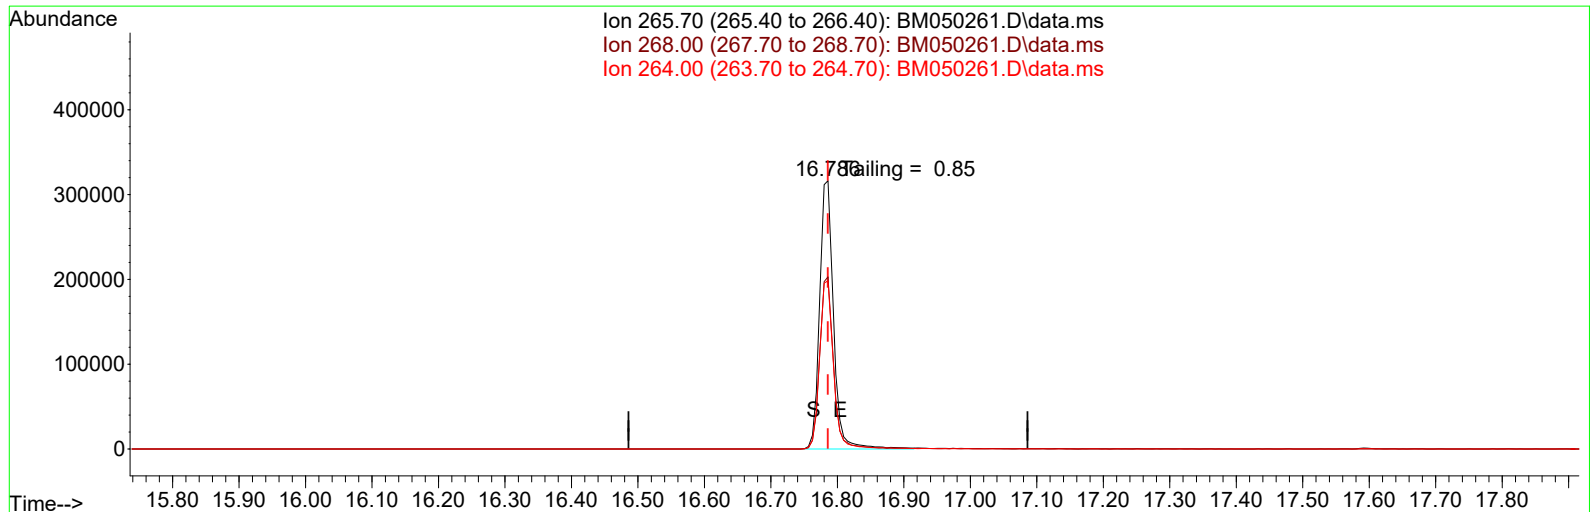

TIC: BM050261.D\data.ms

(70) Pentachlorophenol (C)




16.786min (-0.000) 158695.78 ng

response 460207

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.15
264.00	63.50	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050261.D
Acq On : 10 Jun 2025 04:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 05:34:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

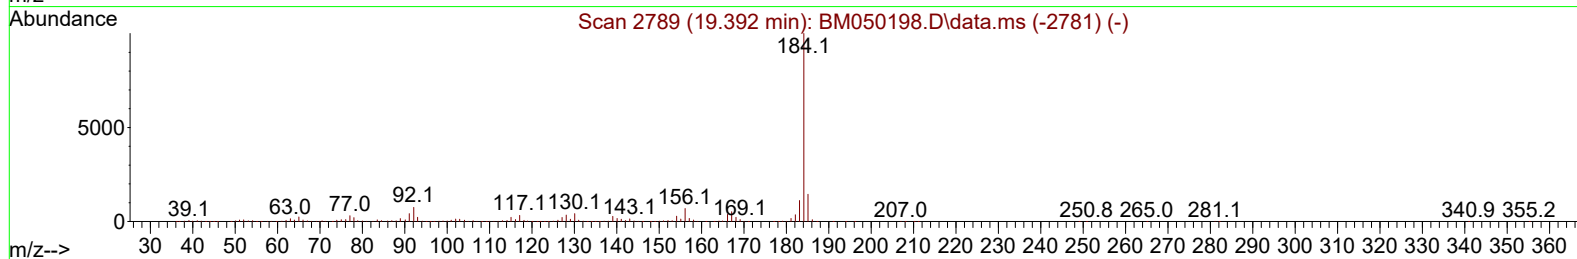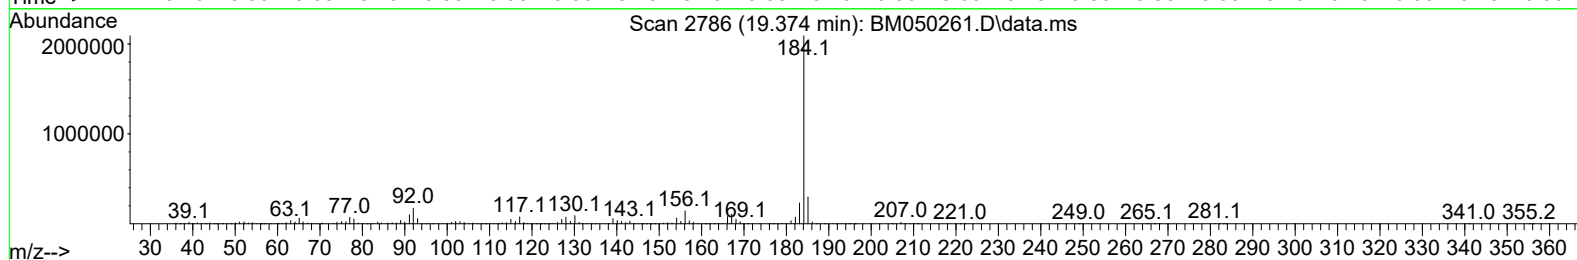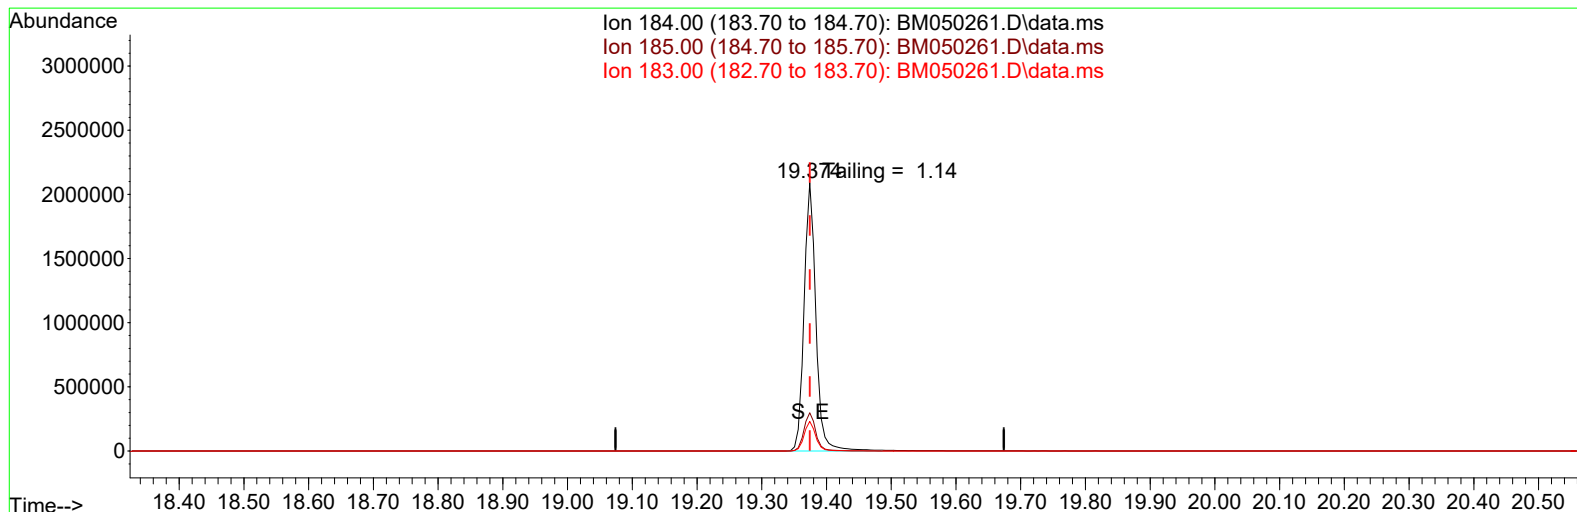

TIC: BM050261.D\data.ms

(77) Benzidine**19.374min (-0.000) 99825.69 ng****response 2680856**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.26
183.00	11.20	11.06
0.00	0.00	0.00