

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
 Data File : BM050258.D
 Acq On : 10 Jun 2025 01:33
 Operator : RC/JU
 Sample : Q2241-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-S

Quant Time: Jun 10 02:46:00 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 09 11:54:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	330437	20.000	ng	0.00
21) Naphthalene-d8	10.551	136	1247685	20.000	ng	0.00
39) Acenaphthene-d10	14.398	164	684088	20.000	ng	0.00
64) Phenanthrene-d10	17.133	188	1275149	20.000	ng	0.00
76) Chrysene-d12	21.362	240	1269974	20.000	ng	-0.01
86) Perylene-d12	24.338	264	1345088	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	2598965	131.203	ng	0.00
7) Phenol-d6	6.934	99	2922010	112.056	ng	0.00
23) Nitrobenzene-d5	8.916	82	2196705	91.567	ng	0.00
42) 2,4,6-Tribromophenol	15.880	330	1052708	135.292	ng	0.00
45) 2-Fluorobiphenyl	13.022	172	4322201	85.539	ng	0.00
79) Terphenyl-d14	19.762	244	5799289	86.535	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050258.D
Acq On : 10 Jun 2025 01:33
Operator : RC/JU
Sample : Q2241-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-S


Quant Time: Jun 10 02:46:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

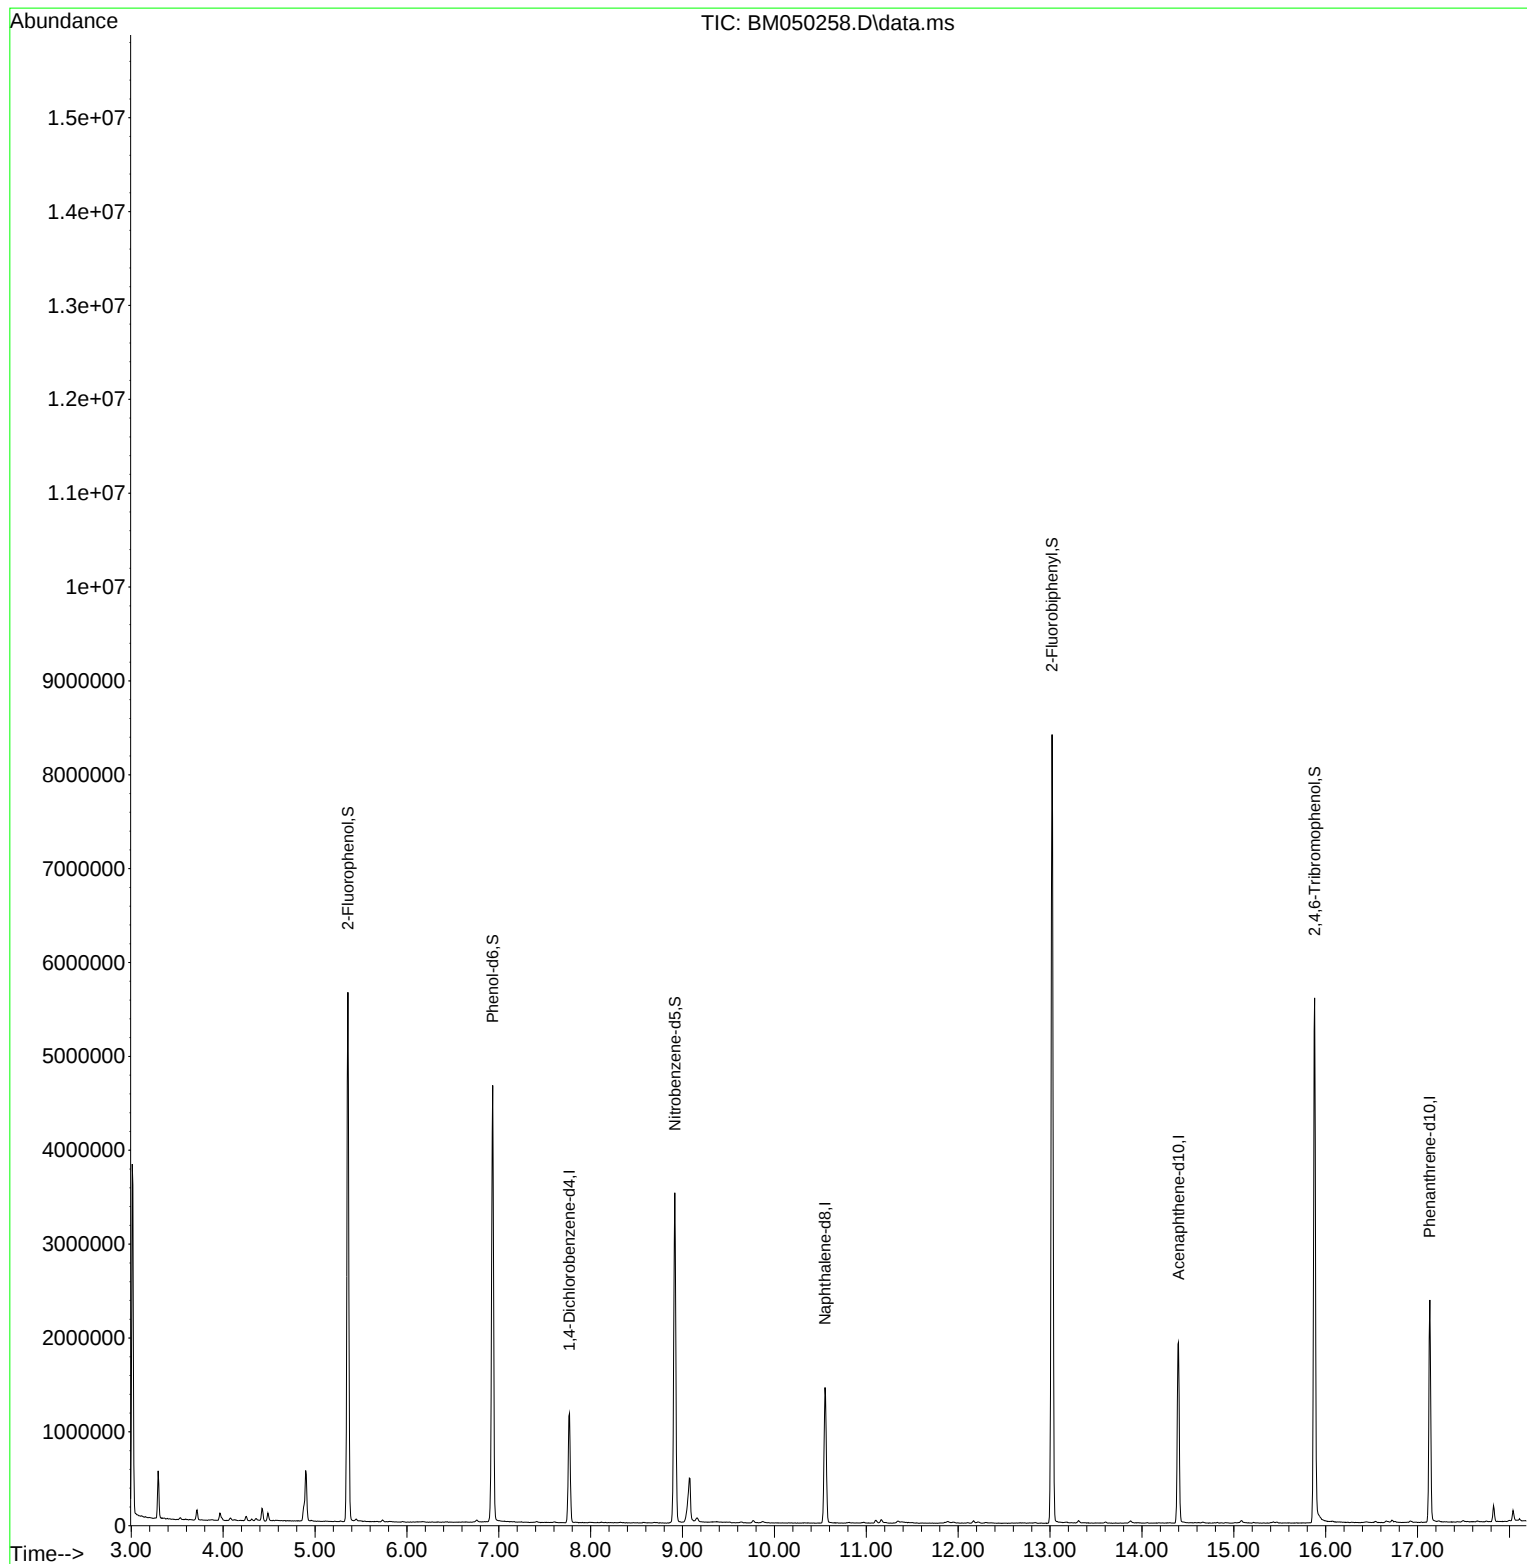


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050258.D
Acq On : 10 Jun 2025 01:33
Operator : RC/JU
Sample : Q2241-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-S

Quant Time: Jun 10 02:46:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration




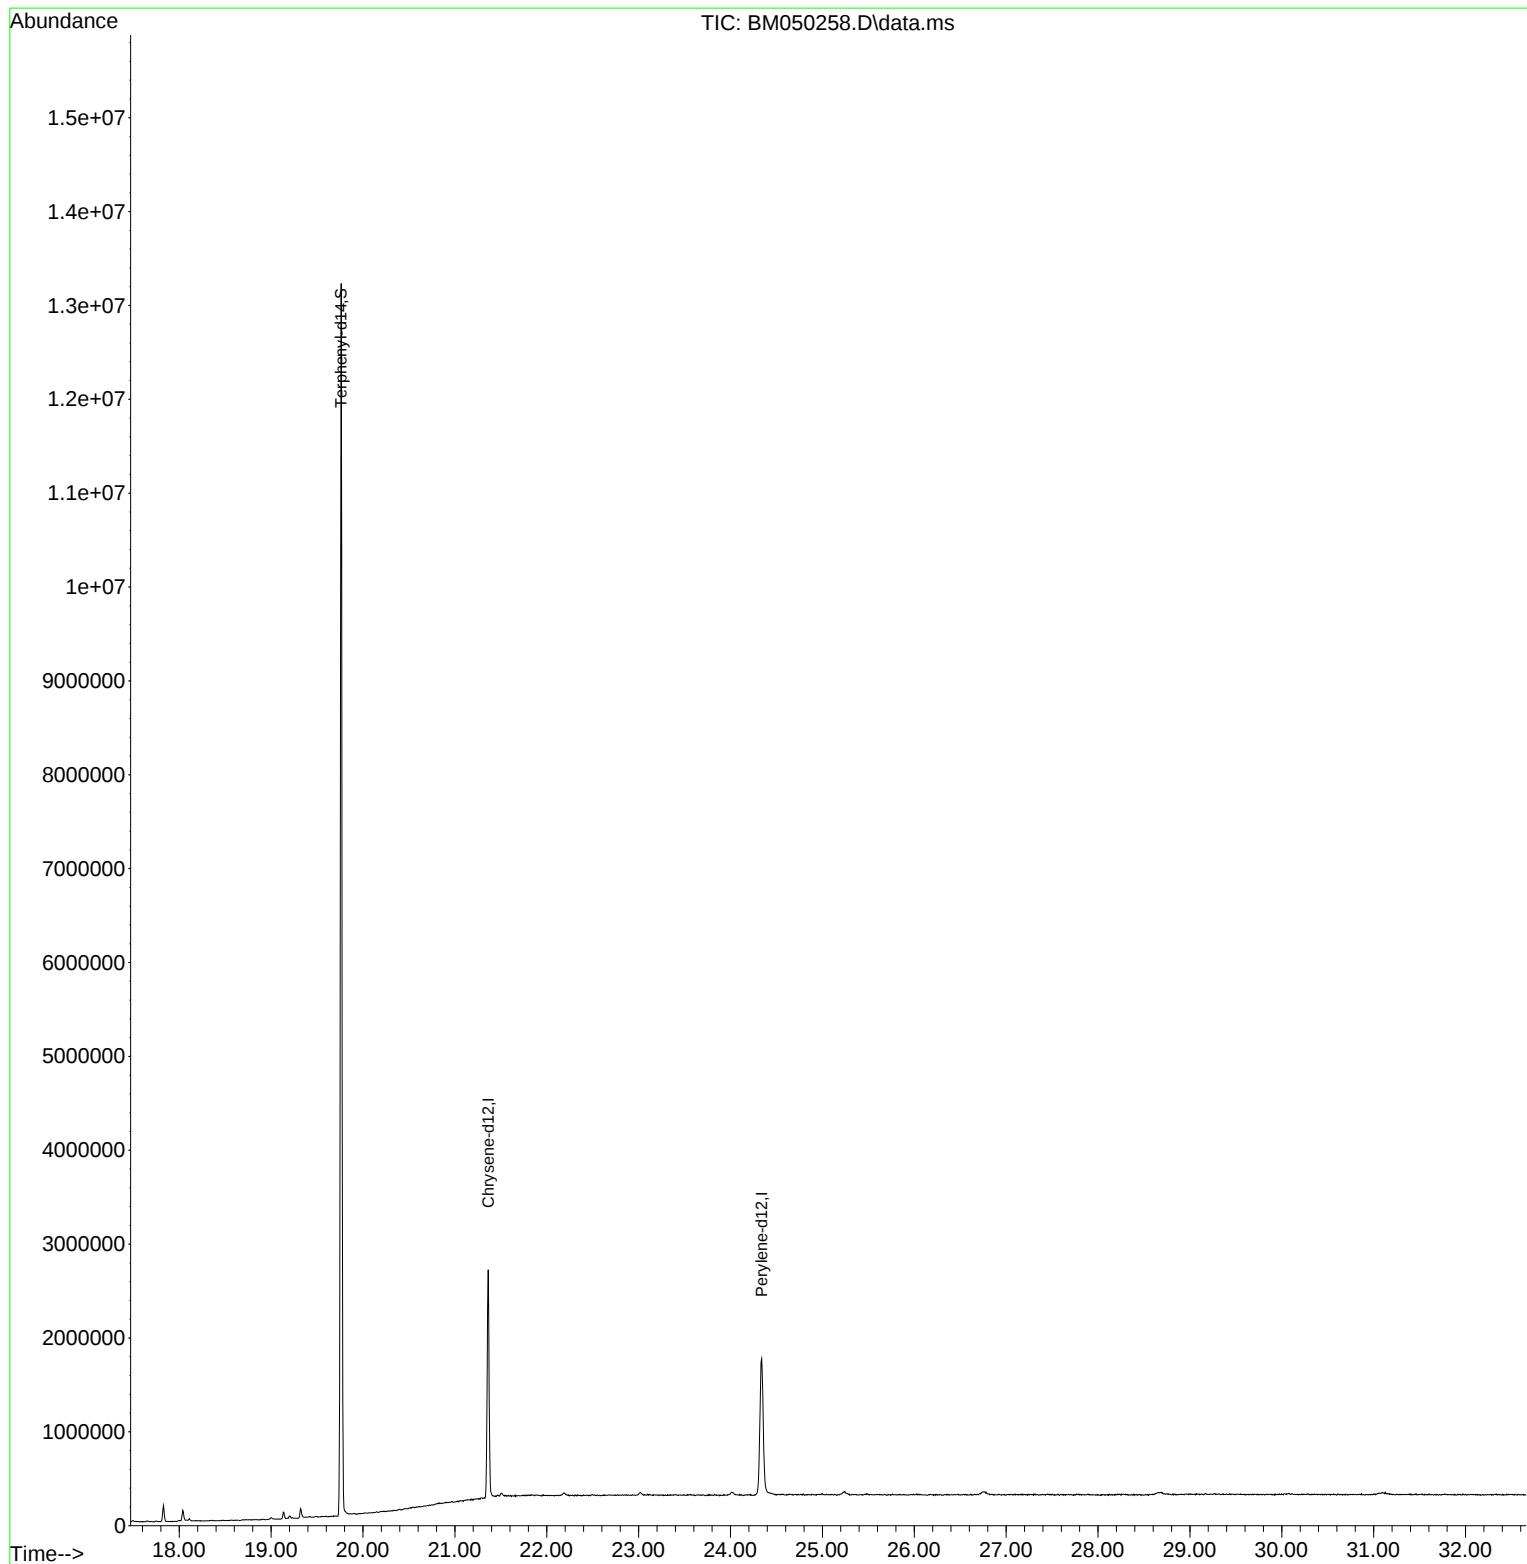


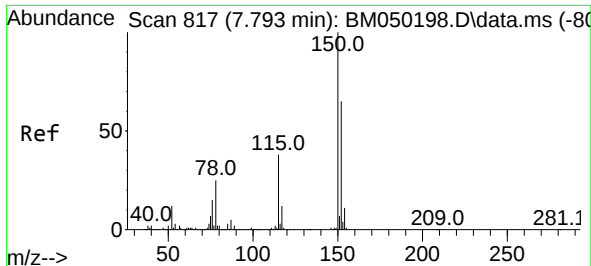

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.769 min Scan# 81
Delta R.T. -0.000 min
Lab File: BM050258.D
Acq: 10 Jun 2025 01:33




Instrument :
BNA_M
ClientSampleId :
TP-S


Tgt Ion:152 Resp: 330437
Ion Ratio Lower Upper
152 100
150 157.7 122.2 183.4
115 61.4 46.3 69.5

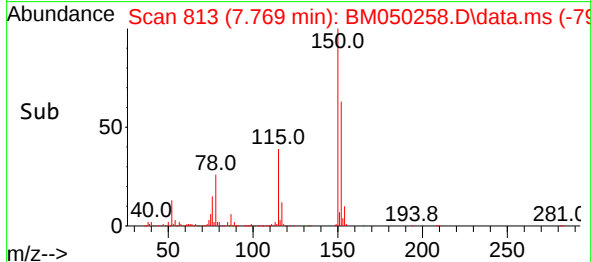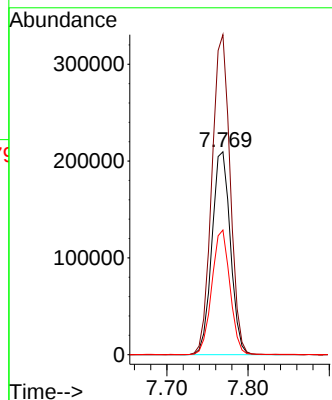

#5
2-Fluorophenol
Concen: 131.203 ng
RT: 5.357 min Scan# 403
Delta R.T. 0.000 min
Lab File: BM050258.D
Acq: 10 Jun 2025 01:33

Tgt Ion:112 Resp: 2598965
Ion Ratio Lower Upper
112 100
64 51.4 39.8 59.6
63 26.1 19.8 29.8


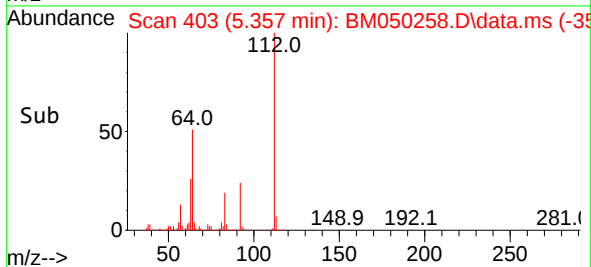
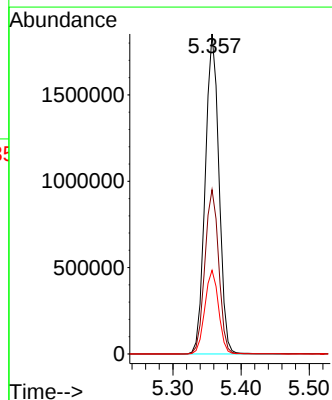
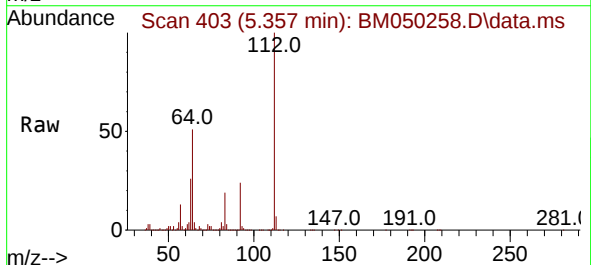


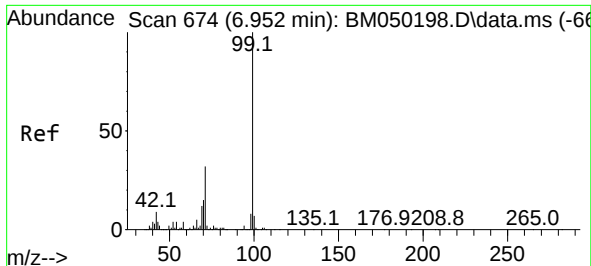

#7
Phenol-d6
Concen: 112.056 ng
RT: 6.934 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM050258.D
Acq: 10 Jun 2025 01:33




Instrument :
BNA_M
ClientSampleId :
TP-S


Tgt Ion: 99 Resp: 2922010
Ion Ratio Lower Upper
99 100
42 8.8 6.9 10.3
71 32.8 25.3 37.9

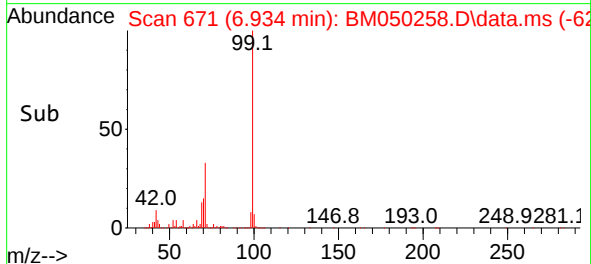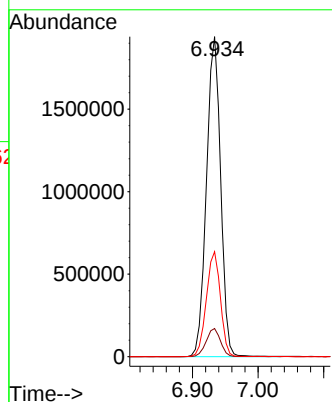

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.551 min Scan# 1286
Delta R.T. -0.006 min
Lab File: BM050258.D
Acq: 10 Jun 2025 01:33

Tgt Ion: 136 Resp: 1247685
Ion Ratio Lower Upper
136 100
137 10.7 8.6 13.0
54 5.8 3.8 5.8
68 6.1 4.9 7.3


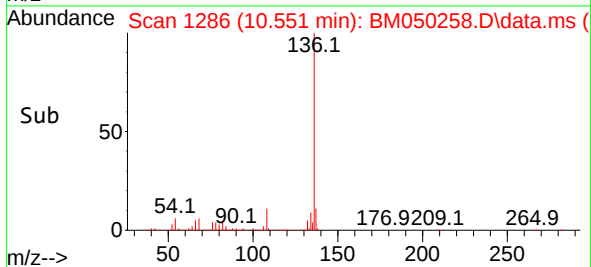
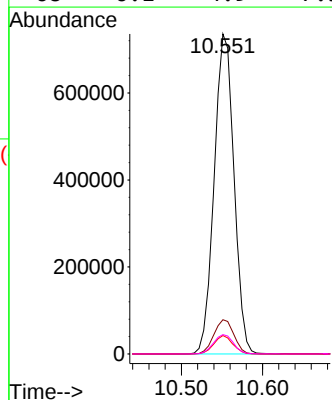
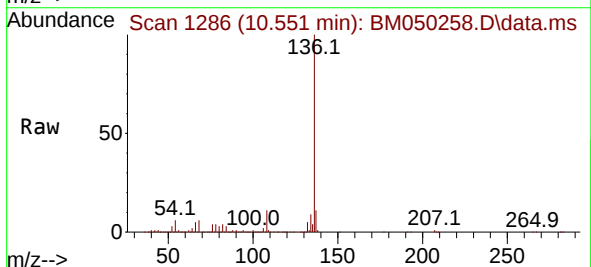


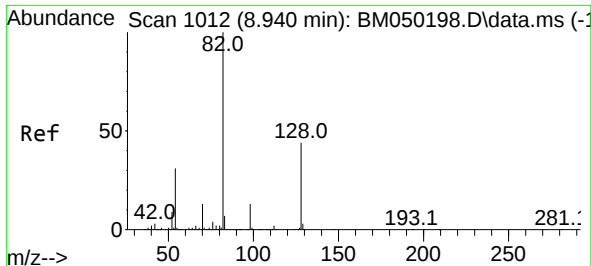

#23
Nitrobenzene-d5
Concen: 91.567 ng
RT: 8.916 min Scan# 1012
Delta R.T. 0.000 min
Lab File: BM050258.D
Acq: 10 Jun 2025 01:33




Instrument :
BNA_M
ClientSampleId :
TP-S


Tgt Ion: 82 Resp: 2196705
Ion Ratio Lower Upper
82 100
128 42.5 35.2 52.8
54 31.6 24.5 36.7

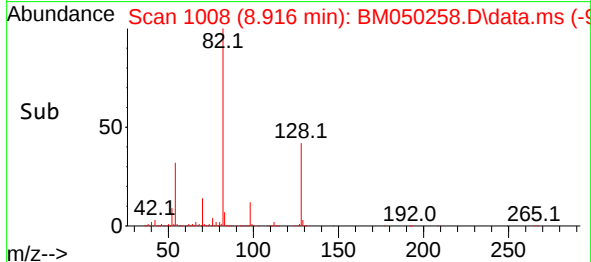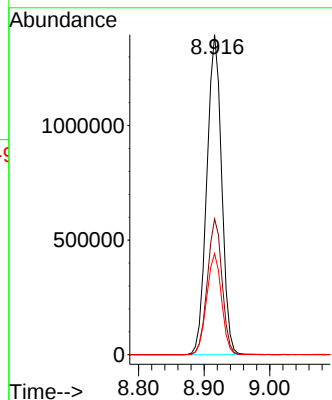

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.398 min Scan# 1940
Delta R.T. 0.000 min
Lab File: BM050258.D
Acq: 10 Jun 2025 01:33

Tgt Ion:164 Resp: 684088
Ion Ratio Lower Upper
164 100
162 99.8 80.2 120.4
160 45.0 35.7 53.5


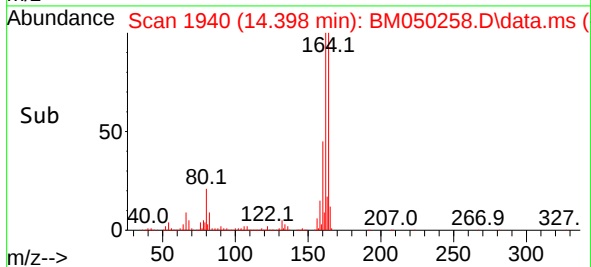
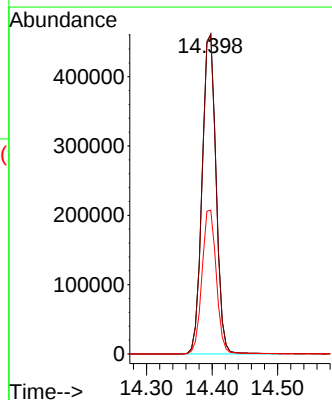
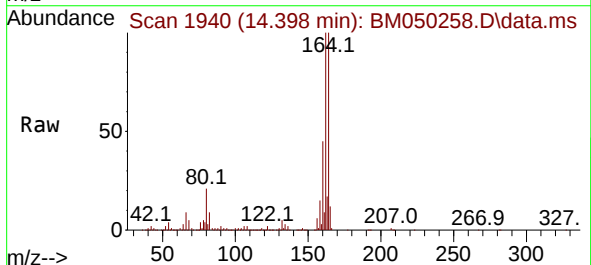


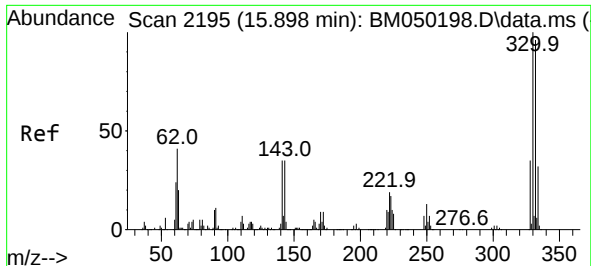

#42
2,4,6-Tribromophenol
Concen: 135.292 ng
RT: 15.880 min Scan# 2195
Delta R.T. 0.000 min
Lab File: BM050258.D
Acq: 10 Jun 2025 01:33




Instrument :
BNA_M
ClientSampleId :
TP-S


Tgt Ion:330 Resp: 1052708
Ion Ratio Lower Upper
330 100
332 95.6 77.5 116.3
141 38.5 28.8 43.2

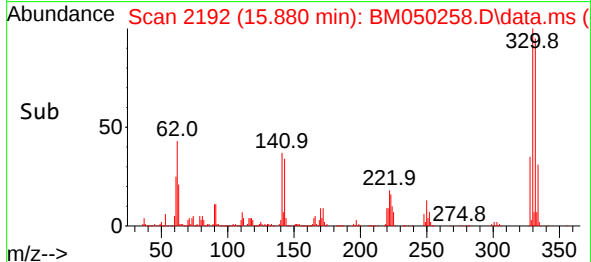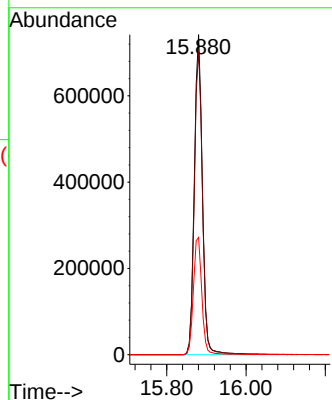

#45
2-Fluorobiphenyl
Concen: 85.539 ng
RT: 13.022 min Scan# 1706
Delta R.T. -0.006 min
Lab File: BM050258.D
Acq: 10 Jun 2025 01:33

Tgt Ion:172 Resp: 4322201
Ion Ratio Lower Upper
172 100
171 34.9 27.8 41.6
170 23.4 18.6 27.8

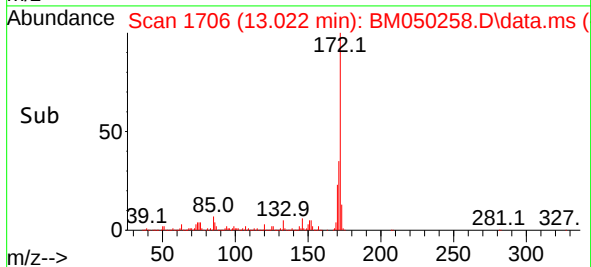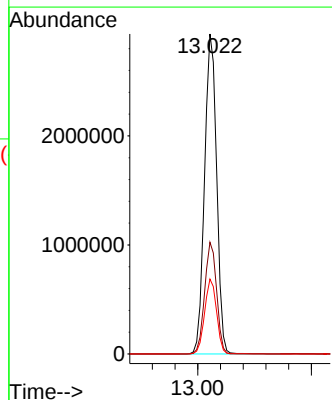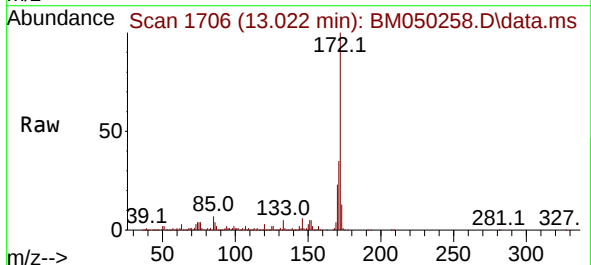



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.133 min Scan# 24

Delta R.T. -0.006 min

Lab File: BM050258.D

Acq: 10 Jun 2025 01:33

Instrument :

BNA_M

ClientSampleId :

TP-S





Tgt Ion:188 Resp: 1275149

Ion Ratio Lower Upper

188 100

94 10.4 8.1 12.1

80 11.1 8.6 13.0

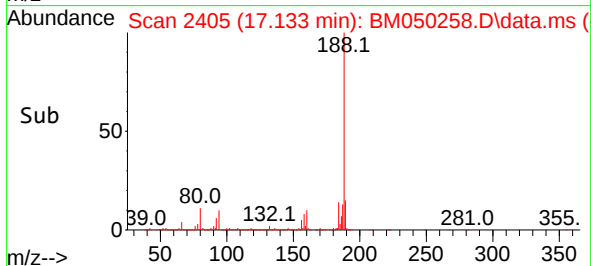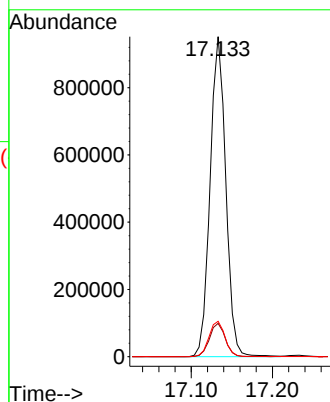

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.362 min Scan# 3124

Delta R.T. -0.012 min

Lab File: BM050258.D

Acq: 10 Jun 2025 01:33




Tgt Ion:240 Resp: 1269974


Ion Ratio Lower Upper

240 100

120 12.2 9.0 13.4

236 24.8 20.7 31.1


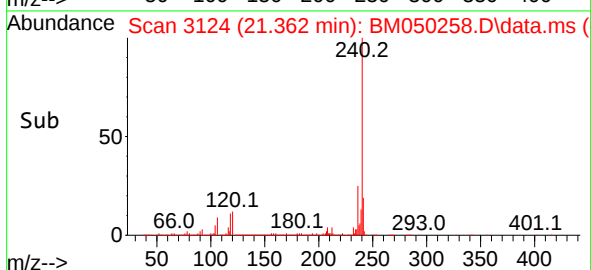
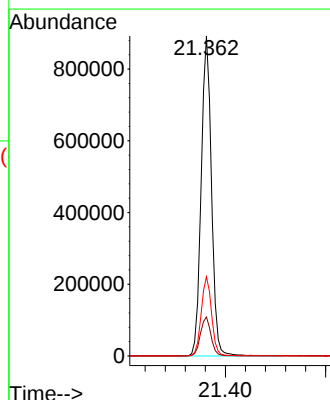
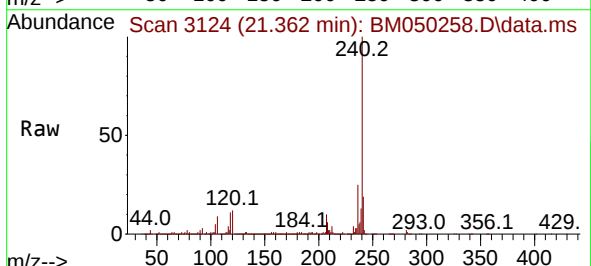


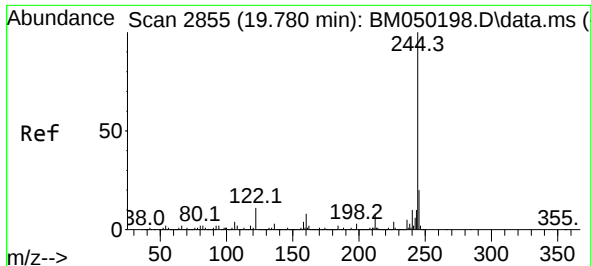

#79
 Terphenyl-d14
 Concen: 86.535 ng
 RT: 19.762 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BM050258.D
 Acq: 10 Jun 2025 01:33

Instrument :
 BNA_M
 ClientSampleId :
 TP-S

Tgt Ion:244 Resp: 5799289
 Ion Ratio Lower Upper
 244 100
 212 7.3 6.0 9.0
 122 10.9 8.6 12.8

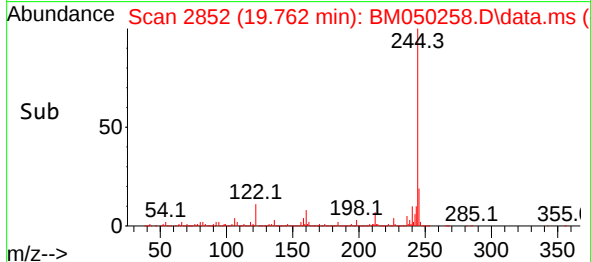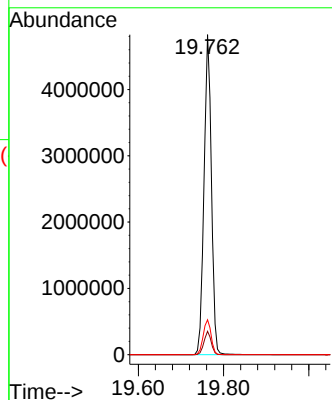

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.338 min Scan# 3630
 Delta R.T. -0.006 min
 Lab File: BM050258.D
 Acq: 10 Jun 2025 01:33

Tgt Ion:264 Resp: 1345088
 Ion Ratio Lower Upper
 264 100
 260 23.3 18.6 28.0
 265 21.6 16.8 25.2

