

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
 Data File : BM050259.D
 Acq On : 10 Jun 2025 02:12
 Operator : RC/JU
 Sample : Q2260-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP10-MHG-WC

Quant Time: Jun 10 02:46:13 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 09 11:54:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	381618	20.000	ng	0.00
21) Naphthalene-d8	10.551	136	1435649	20.000	ng	0.00
39) Acenaphthene-d10	14.398	164	781255	20.000	ng	0.00
64) Phenanthrene-d10	17.133	188	1399416	20.000	ng	0.00
76) Chrysene-d12	21.362	240	1250695	20.000	ng	-0.01
86) Perylene-d12	24.338	264	1291609	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	3340207	146.008	ng	0.00
7) Phenol-d6	6.934	99	3987283	132.401	ng	0.00
23) Nitrobenzene-d5	8.916	82	2571284	93.148	ng	0.00
42) 2,4,6-Tribromophenol	15.880	330	1228902	138.293	ng	0.00
45) 2-Fluorobiphenyl	13.022	172	4873058	84.446	ng	0.00
79) Terphenyl-d14	19.762	244	5988537	90.737	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050259.D
Acq On : 10 Jun 2025 02:12
Operator : RC/JU
Sample : Q2260-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP10-MHG-WC


Quant Time: Jun 10 02:46:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

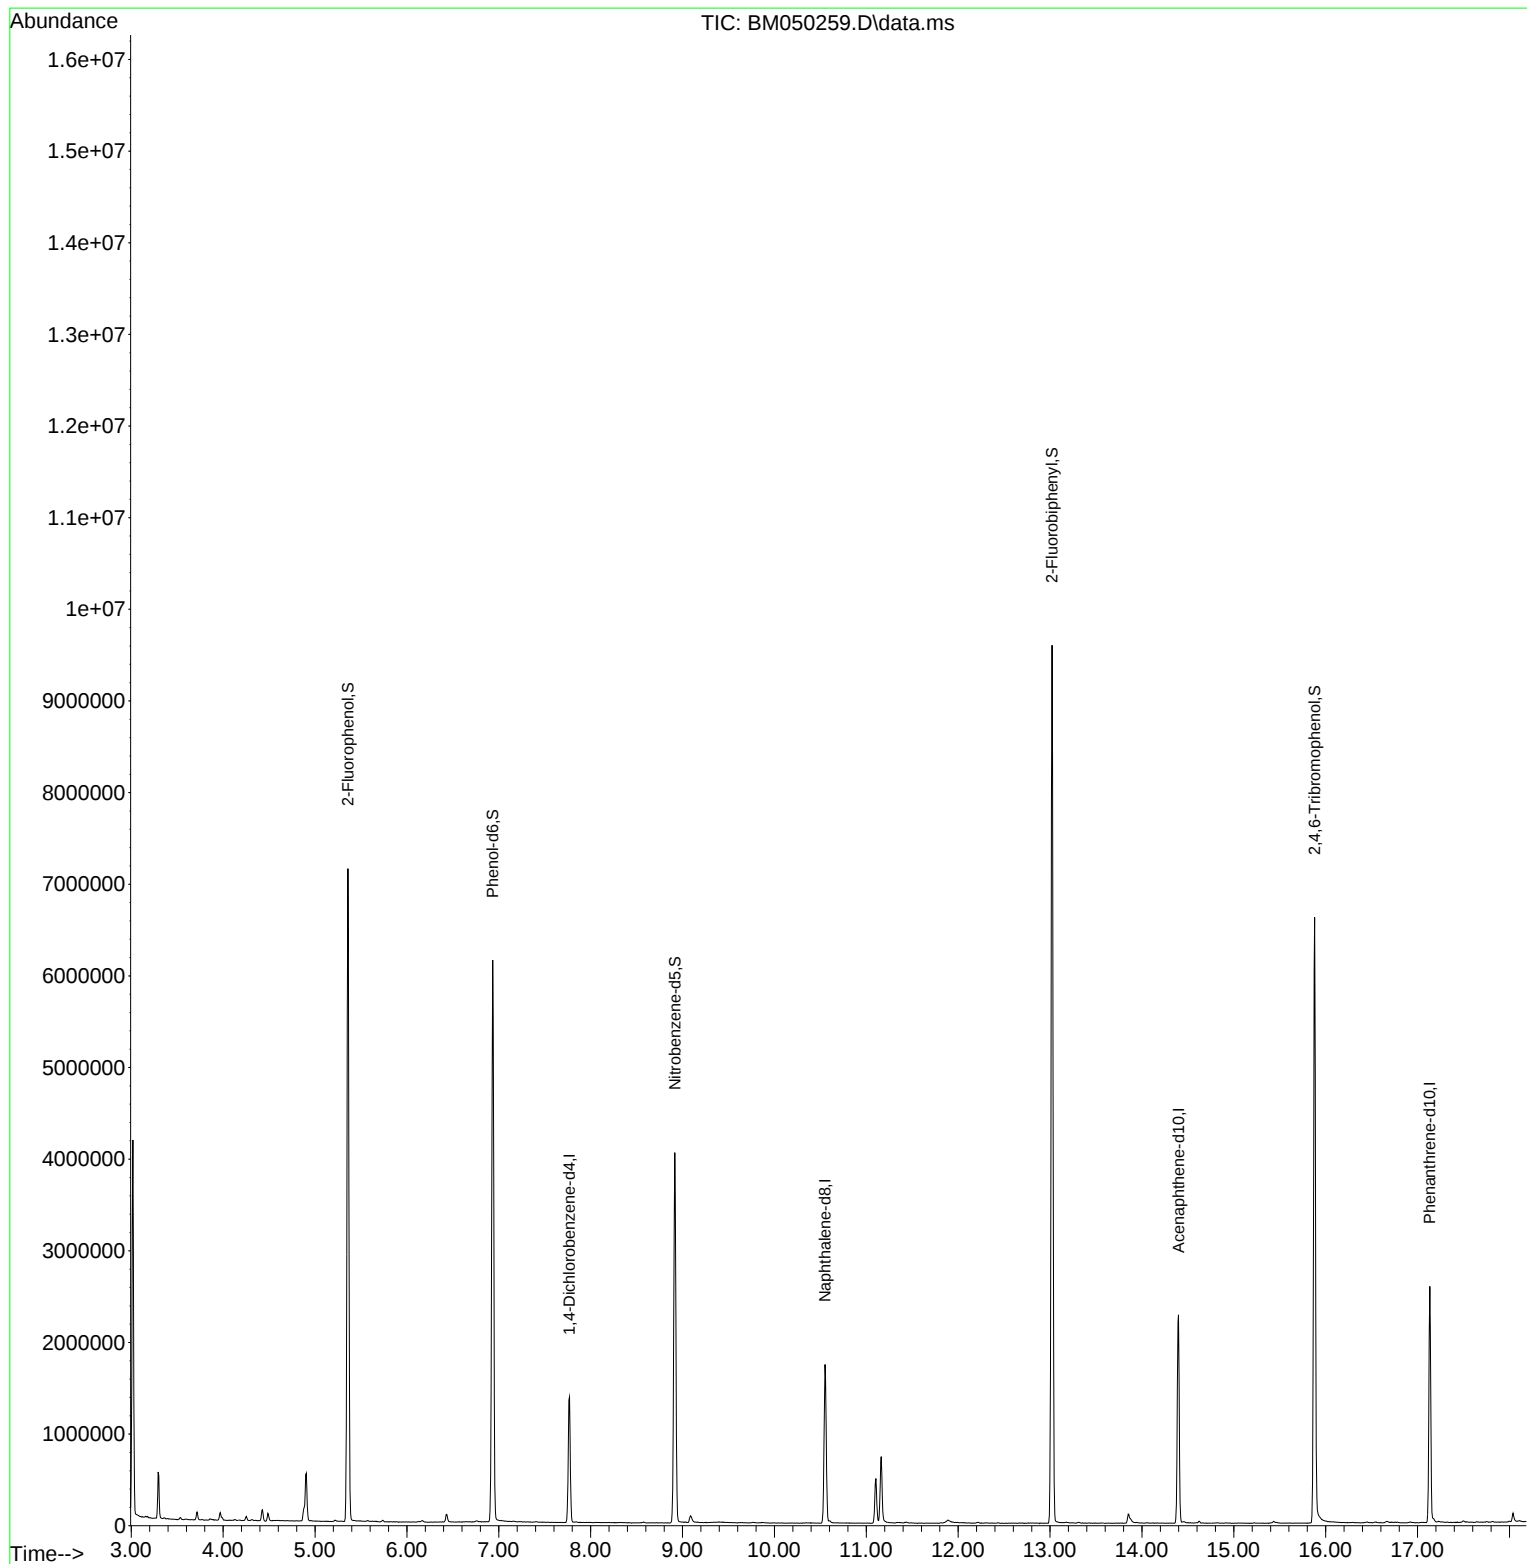


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050259.D
Acq On : 10 Jun 2025 02:12
Operator : RC/JU
Sample : Q2260-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP10-MHG-WC

Quant Time: Jun 10 02:46:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration




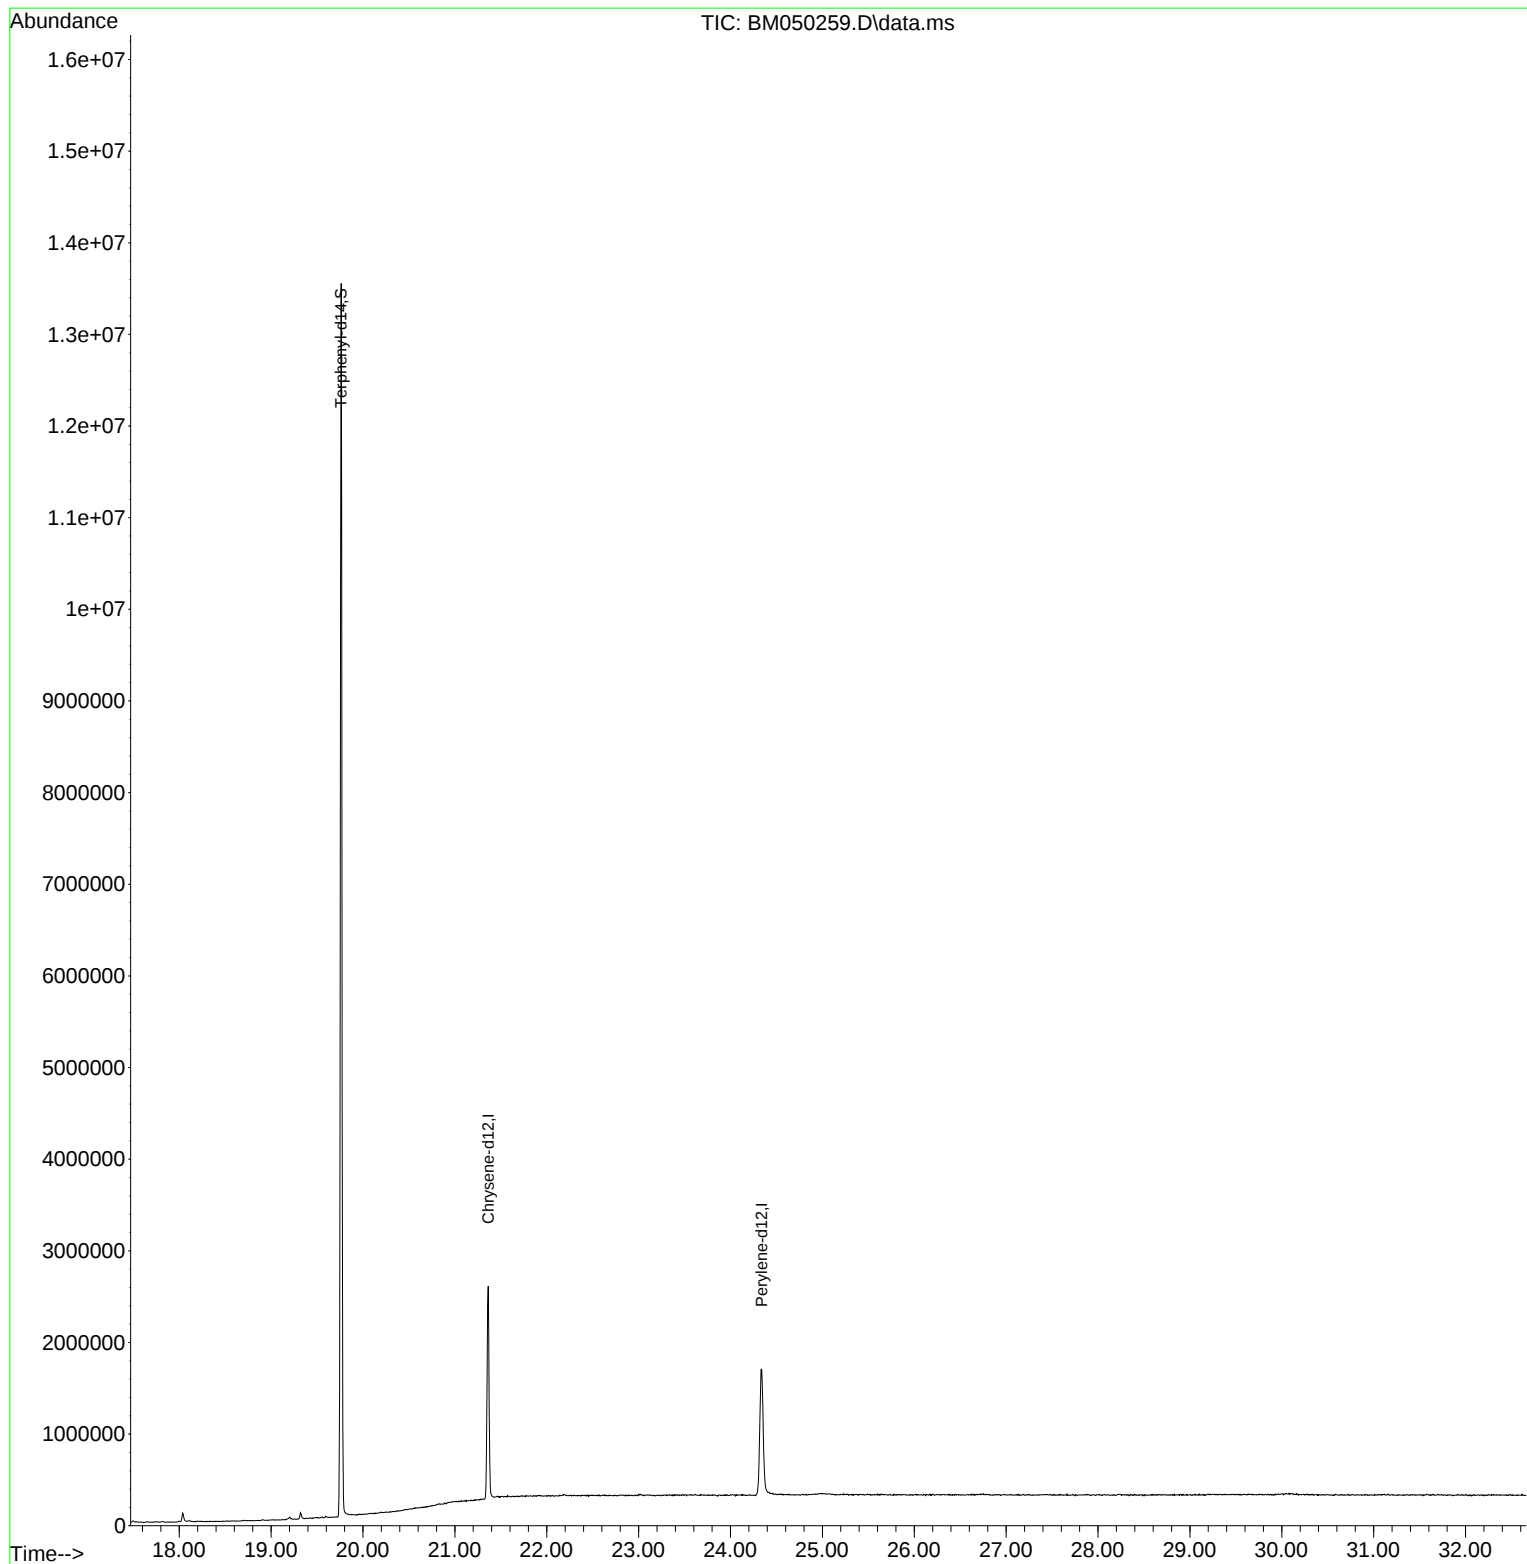


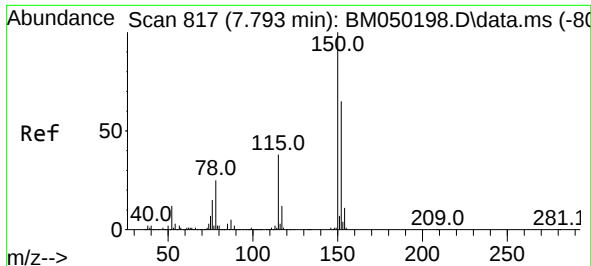

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.769 min Scan# 817
Delta R.T. -0.000 min
Lab File: BM050259.D
Acq: 10 Jun 2025 02:12




Instrument :
BNA_M
ClientSampleId :
TP10-MHG-WC


Tgt Ion:152 Resp: 381618
Ion Ratio Lower Upper
152 100
150 157.5 122.2 183.4
115 60.4 46.3 69.5

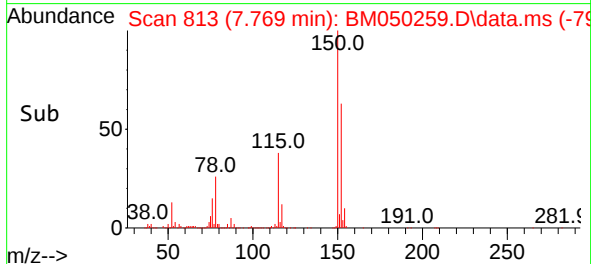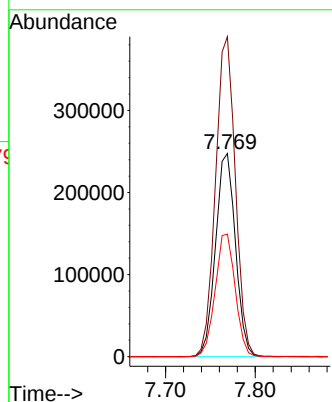

#5
2-Fluorophenol
Concen: 146.008 ng
RT: 5.357 min Scan# 403
Delta R.T. 0.000 min
Lab File: BM050259.D
Acq: 10 Jun 2025 02:12

Tgt Ion:112 Resp: 3340207
Ion Ratio Lower Upper
112 100
64 50.9 39.8 59.6
63 25.7 19.8 29.8


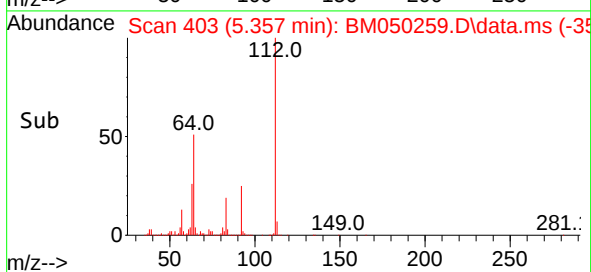
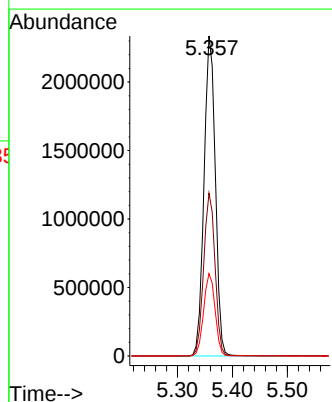
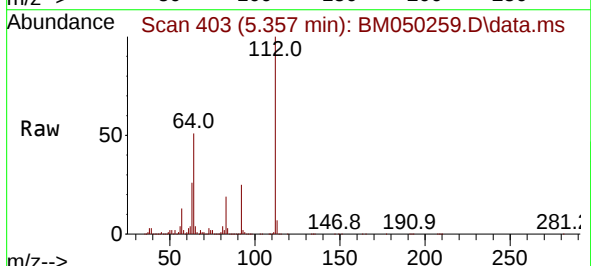


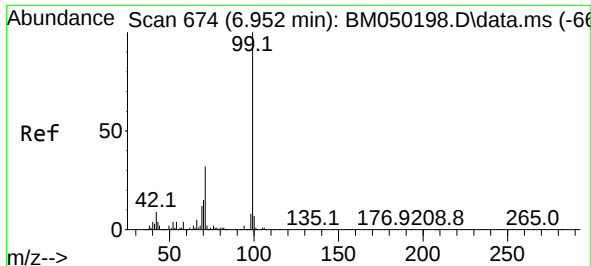

#7
Phenol-d6
Concen: 132.401 ng
RT: 6.934 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM050259.D
Acq: 10 Jun 2025 02:12




Instrument :
BNA_M
ClientSampleId :
TP10-MHG-WC


Tgt Ion: 99 Resp: 3987283
Ion Ratio Lower Upper
99 100
42 8.9 6.9 10.3
71 32.8 25.3 37.9

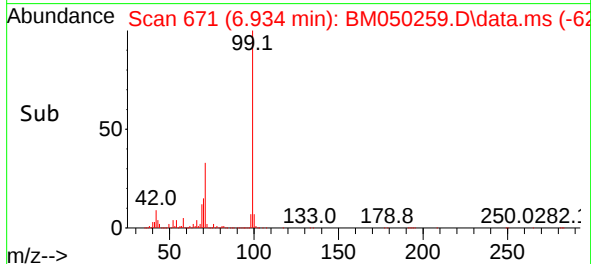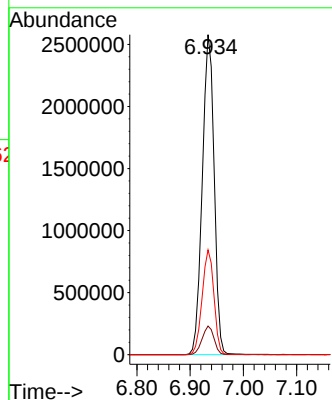

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.551 min Scan# 1286
Delta R.T. -0.006 min
Lab File: BM050259.D
Acq: 10 Jun 2025 02:12

Tgt Ion: 136 Resp: 1435649
Ion Ratio Lower Upper
136 100
137 11.1 8.6 13.0
54 5.6 3.8 5.8
68 6.6 4.9 7.3


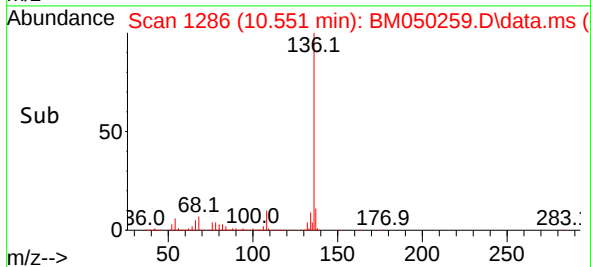
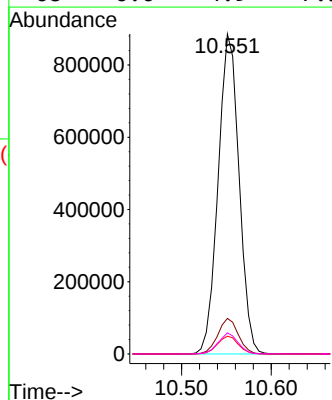
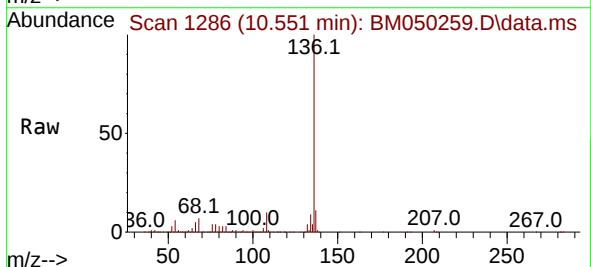


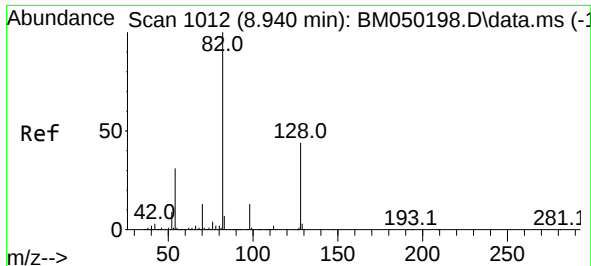

#23
Nitrobenzene-d5
Concen: 93.148 ng
RT: 8.916 min Scan# 1012
Delta R.T. 0.000 min
Lab File: BM050259.D
Acq: 10 Jun 2025 02:12




Instrument :
BNA_M
ClientSampleId :
TP10-MHG-WC


Tgt Ion: 82 Resp: 2571284
Ion Ratio Lower Upper
82 100
128 42.5 35.2 52.8
54 31.6 24.5 36.7

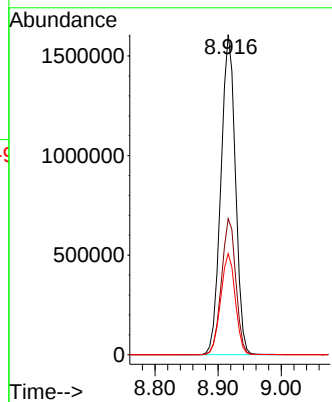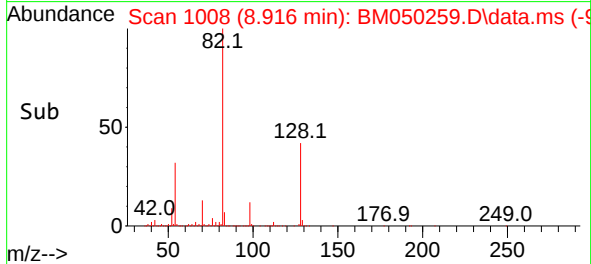

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.398 min Scan# 1940
Delta R.T. 0.000 min
Lab File: BM050259.D
Acq: 10 Jun 2025 02:12

Tgt Ion:164 Resp: 781255
Ion Ratio Lower Upper
164 100
162 99.5 80.2 120.4
160 45.4 35.7 53.5


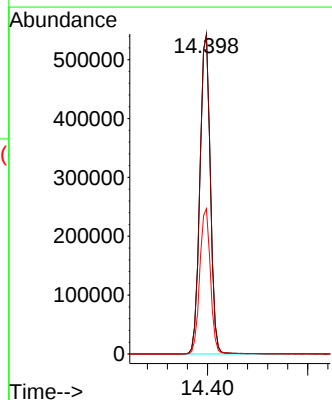
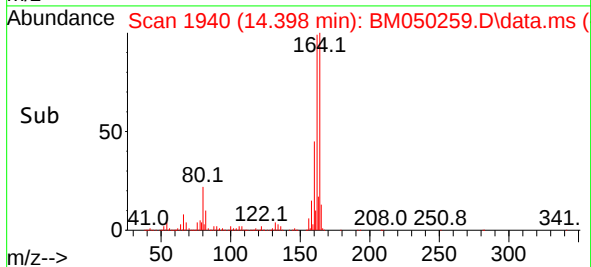
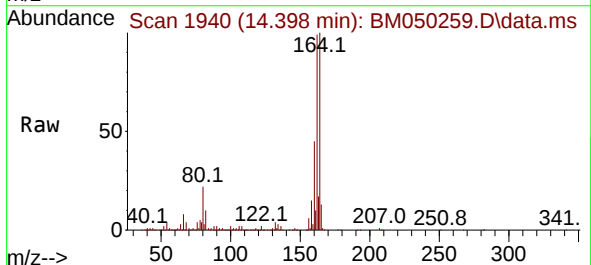


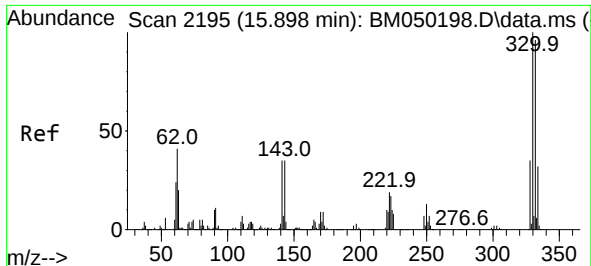

#42
2,4,6-Tribromophenol
Concen: 138.293 ng
RT: 15.880 min Scan# 2195
Delta R.T. 0.000 min
Lab File: BM050259.D
Acq: 10 Jun 2025 02:12




Instrument :
BNA_M
ClientSampleId :
TP10-MHG-WC


Tgt Ion:330 Resp: 1228902
Ion Ratio Lower Upper
330 100
332 97.3 77.5 116.3
141 38.4 28.8 43.2

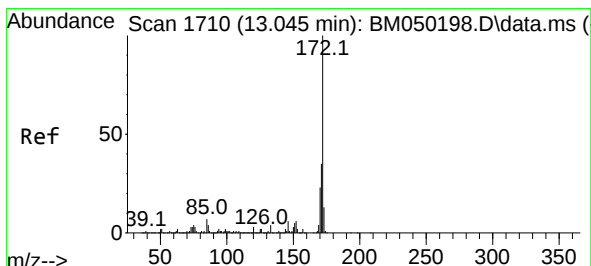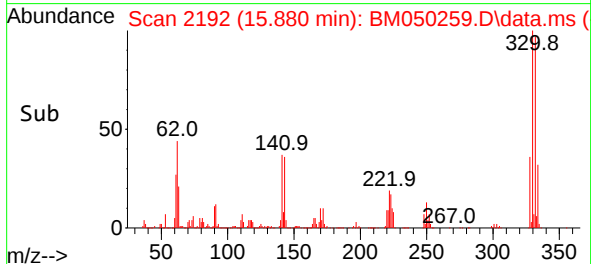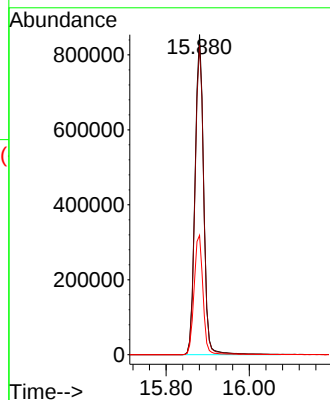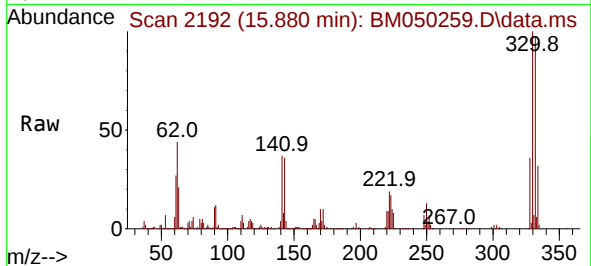

#45
2-Fluorobiphenyl
Concen: 84.446 ng
RT: 13.022 min Scan# 1706
Delta R.T. -0.006 min
Lab File: BM050259.D
Acq: 10 Jun 2025 02:12

Tgt Ion:172 Resp: 4873058
Ion Ratio Lower Upper
172 100
171 35.1 27.8 41.6
170 23.4 18.6 27.8

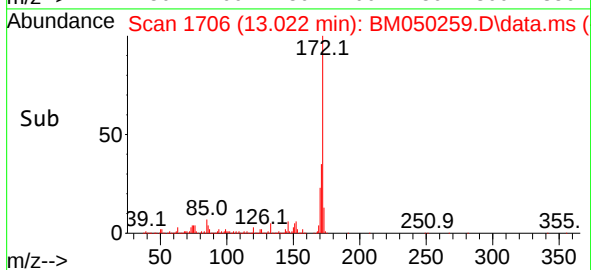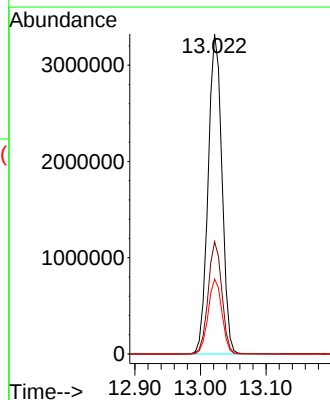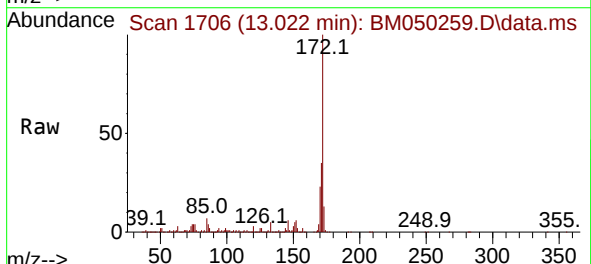



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.133 min Scan# 2405

Delta R.T. -0.006 min

Lab File: BM050259.D

Acq: 10 Jun 2025 02:12

Instrument :

BNA_M

ClientSampleId :

TP10-MHG-WC





Tgt Ion:188 Resp: 1399416

Ion Ratio Lower Upper

188 100

94 10.3 8.1 12.1

80 11.4 8.6 13.0

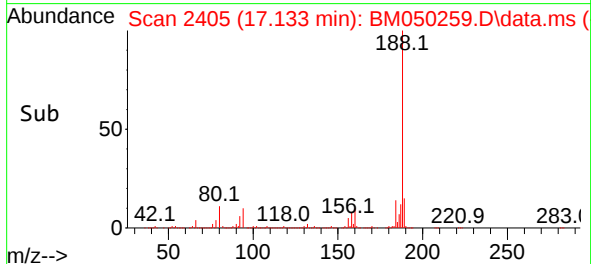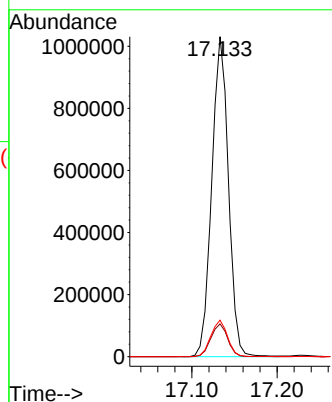

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.362 min Scan# 3124

Delta R.T. -0.012 min

Lab File: BM050259.D

Acq: 10 Jun 2025 02:12




Tgt Ion:240 Resp: 1250695


Ion Ratio Lower Upper

240 100

120 12.5 9.0 13.4

236 24.7 20.7 31.1


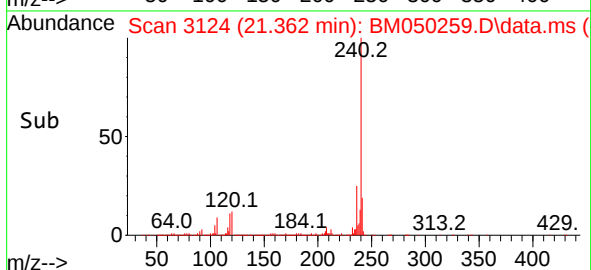
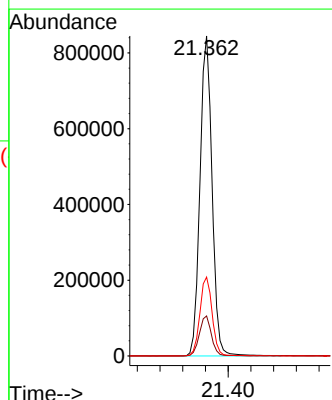
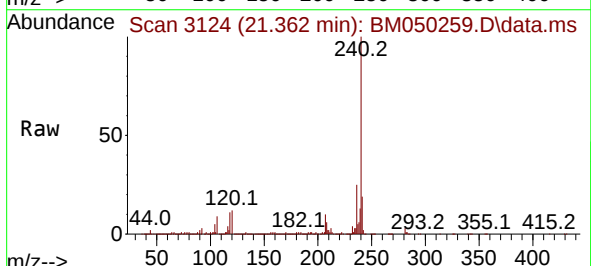


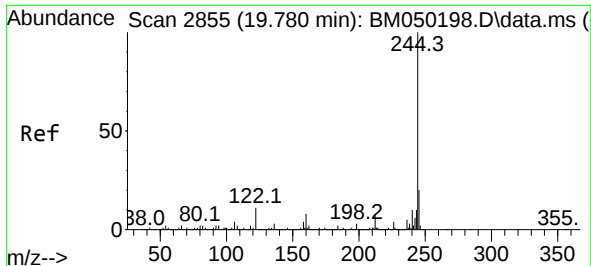

#79
 Terphenyl-d14
 Concen: 90.737 ng
 RT: 19.762 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BM050259.D
 Acq: 10 Jun 2025 02:12

Instrument :
 BNA_M
 ClientSampleId :
 TP10-MHG-WC

Tgt Ion:244 Resp: 5988537
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.0 9.0
 122 11.2 8.6 12.8

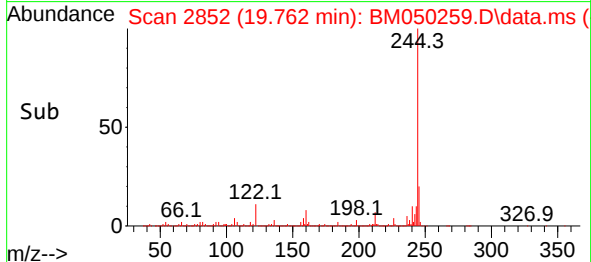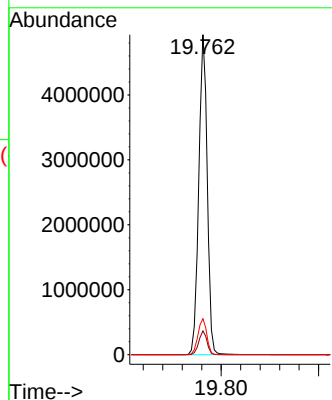

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.338 min Scan# 3630
 Delta R.T. -0.006 min
 Lab File: BM050259.D
 Acq: 10 Jun 2025 02:12

Tgt Ion:264 Resp: 1291609
 Ion Ratio Lower Upper
 264 100
 260 22.9 18.6 28.0
 265 22.8 16.8 25.2

