

Data Path : S:\HPCHEM1\BNA_M\DATA\BM061015\
 Data File : BM001630.D
 Acq On : 10 Jun 2015 13:03
 Operator : TP/IZ
 Sample : PB83814BL
 Misc : SBLK69
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK69

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM061015.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.840	20	26	34	rBV	63800	128303	7.52%	0.767%
2	2.916	34	39	52	rVB	188862	248936	14.60%	1.487%
3	3.410	121	123	128	rBV3	1609	1713	0.10%	0.010%
4	3.722	172	176	180	rVB	16801	20082	1.18%	0.120%
5	5.916	546	549	554	rVB	1504	2343	0.14%	0.014%
6	6.675	674	678	682	rVB2	1843	2424	0.14%	0.014%
7	6.851	702	708	719	rVB	303458	457361	26.82%	2.733%
8	7.028	732	738	746	rBV	201355	310522	18.21%	1.855%
9	7.216	764	770	779	rVB	305855	470797	27.61%	2.813%
10	7.298	783	784	788	rVV2	1405	1816	0.11%	0.011%
11	7.687	843	850	858	rBV	306261	463432	27.18%	2.769%
12	7.904	884	887	892	rVB	2981	3828	0.22%	0.023%
13	8.216	936	940	943	rVV	1674	1842	0.11%	0.011%
14	8.387	963	969	976	rVB	347557	545029	31.96%	3.257%
15	8.845	1039	1047	1055	rVB	267221	412885	24.21%	2.467%
16	9.563	1163	1169	1177	rVB	214908	345650	20.27%	2.065%
17	9.957	1232	1236	1239	rBV2	1677	2053	0.12%	0.012%
18	10.092	1253	1259	1268	rBV	346891	559735	32.83%	3.344%
19	10.475	1318	1324	1331	rBV	341905	575448	33.75%	3.438%
20	10.616	1340	1348	1359	rBV	332594	537769	31.54%	3.213%
21	13.751	1875	1881	1888	rBV	546251	742793	43.56%	4.438%
22	14.033	1922	1929	1936	rBV	623607	892314	52.33%	5.332%
23	14.339	1975	1981	1988	rVB2	477759	712208	41.77%	4.255%
24	14.533	2009	2014	2027	rBV	236695	362953	21.29%	2.169%
25	15.333	2144	2150	2156	rBV	825498	1125887	66.03%	6.727%
26	15.451	2165	2170	2176	rBV	220971	292445	17.15%	1.747%
27	15.574	2187	2191	2193	rVB2	1794	1869	0.11%	0.011%
28	16.874	2409	2412	2416	rVB2	1537	2086	0.12%	0.012%
29	17.086	2442	2448	2454	rBV	614808	835705	49.01%	4.993%
30	17.186	2459	2465	2474	rVB	932553	1325151	77.71%	7.918%
31	19.339	2828	2831	2832	rVV	2260	2304	0.14%	0.014%
32	19.368	2833	2836	2840	rVB2	6048	8702	0.51%	0.052%
33	19.486	2849	2856	2864	rBV	1177247	1570836	92.12%	9.386%
34	19.721	2893	2896	2899	rVB4	1447	2146	0.13%	0.013%

Data Path : S:\HPCHEM1\BNA_M\DATA\BM061015\
Data File : BM001630.D
Acq On : 10 Jun 2015 13:03
Operator : TP/IZ
Sample : PB83814BL
Misc : SBLK69
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK69

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM061015.M
Title : SVOA CALIBRATION

35	19.874	2920	2922	2925	rBV2	2091	2286	0.13%	0.014%
36	20.703	3061	3063	3065	rBV2	1855	1840	0.11%	0.011%
37	21.074	3123	3126	3128	rBV4	7316	7114	0.42%	0.043%
38	21.274	3155	3160	3166	rBV	828719	1052065	61.70%	6.286%
39	23.374	3509	3517	3529	rVV2	921737	1705150	100.00%	10.188%
40	23.515	3533	3541	3552	rVB	527257	998693	58.57%	5.967%


Sum of corrected areas: 16736515

Data Path : S:\HPCHEM1\BNA_M\DATA\BM061015\
Data File : BM001630.D
Acq On : 10 Jun 2015 13:03
Operator : TP/IZ
Sample : PB83814BL
Misc : SBLK69
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK69

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM061015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

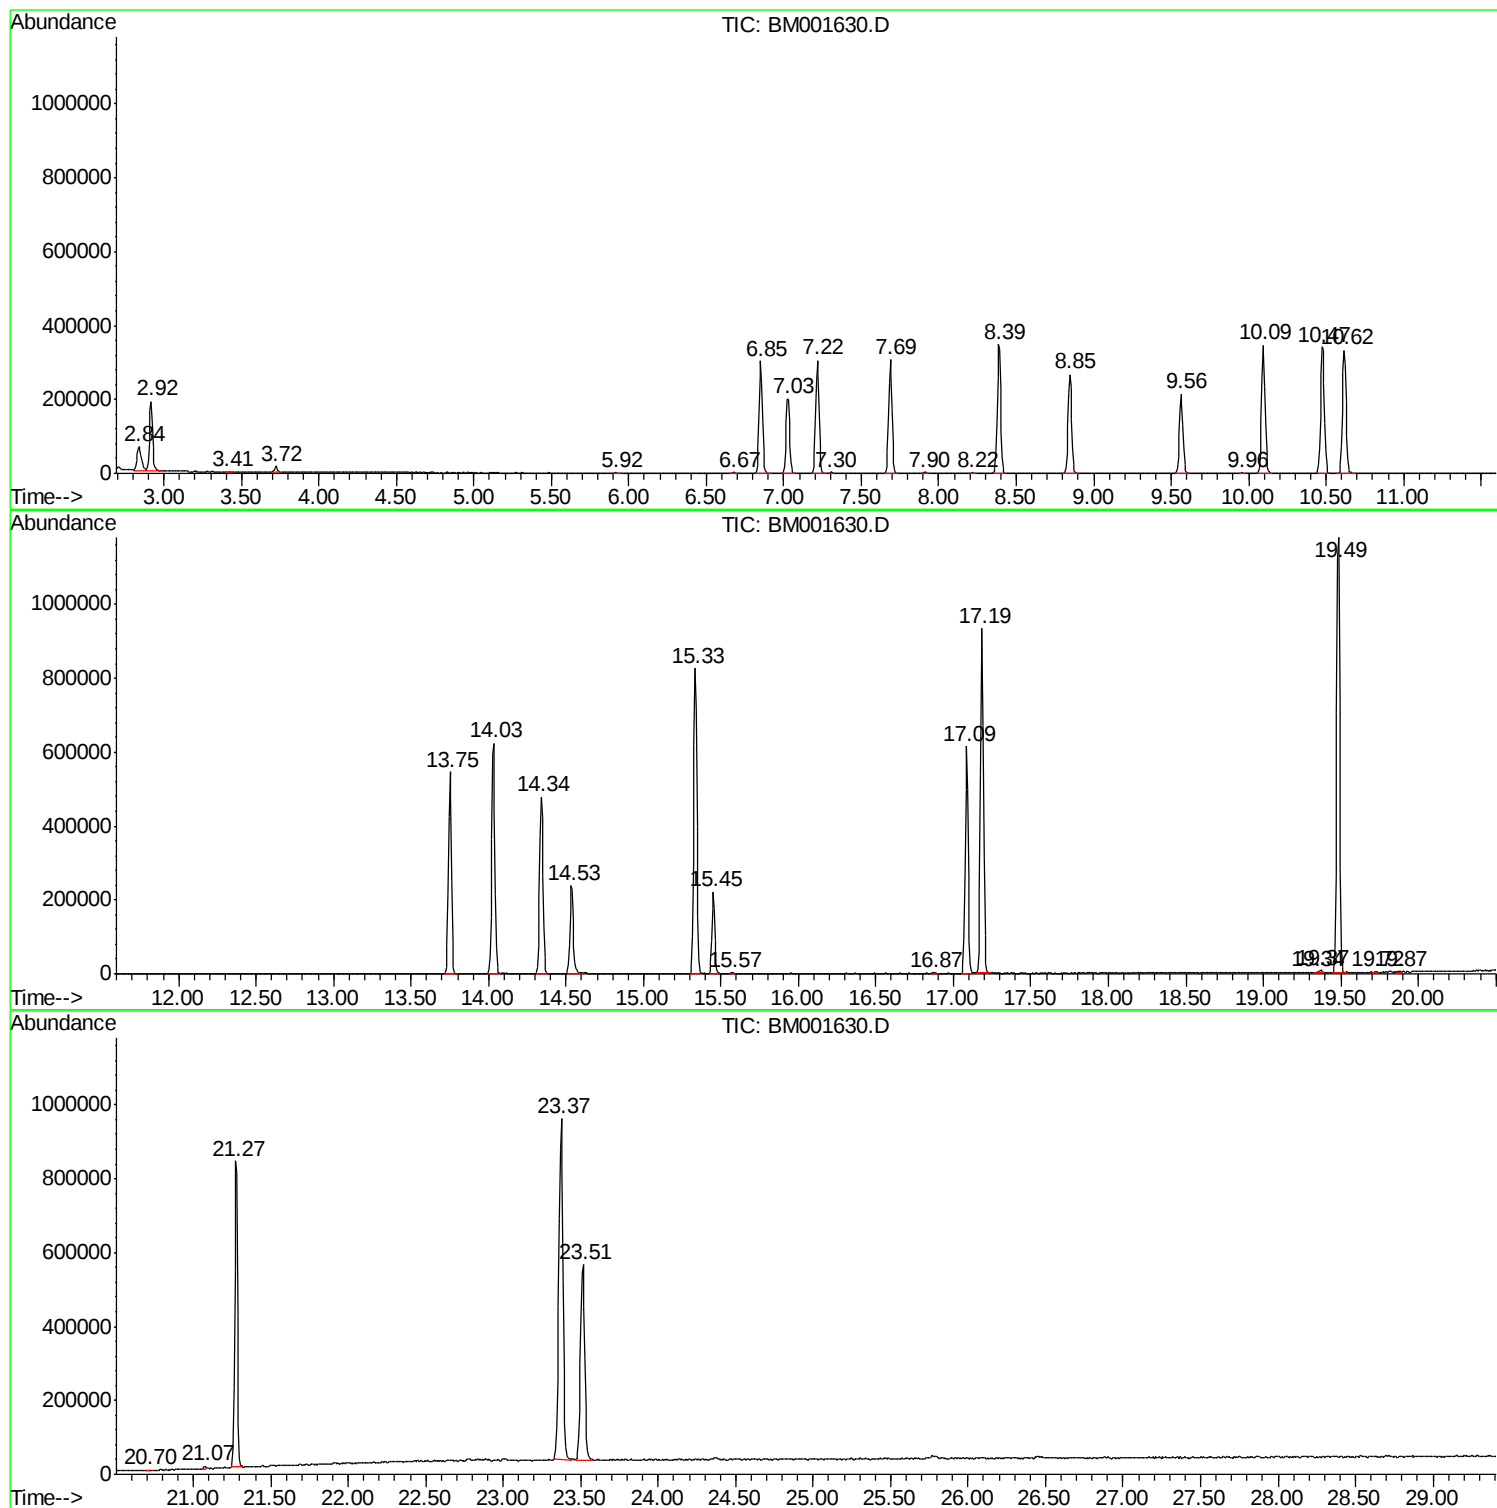

Data Path : S:\HPCHEM1\BNA_M\DATA\BM061015\
Data File : BM001630.D
Acq On : 10 Jun 2015 13:03
Operator : TP/IZ
Sample : PB83814BL
Misc : SBLK69
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK69










Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM061015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.92	10.74 ng/ul	248936	1,4-Dichlorobenzene-d4	7.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
3		Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	33
4		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5		Boronic acid, ethyl-, dimethyl e...	102	C4H11B02	007318-82-3	10

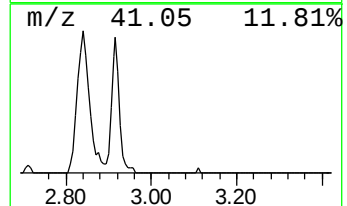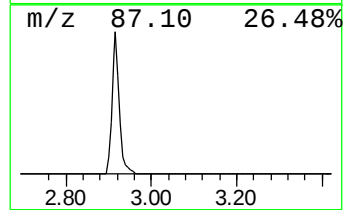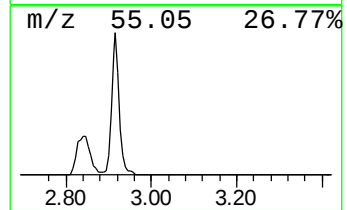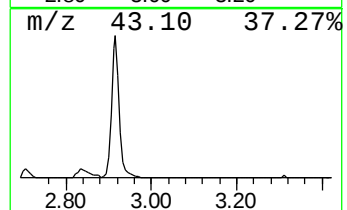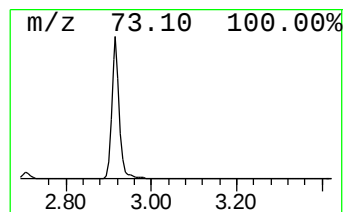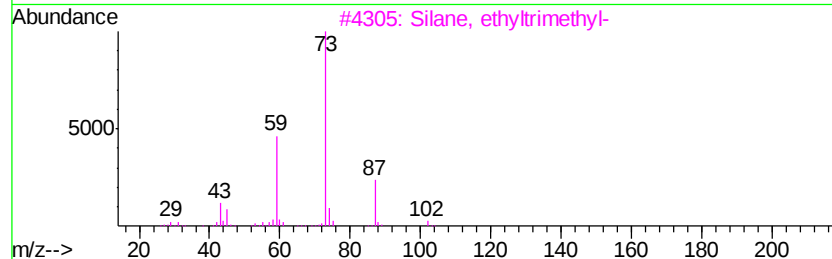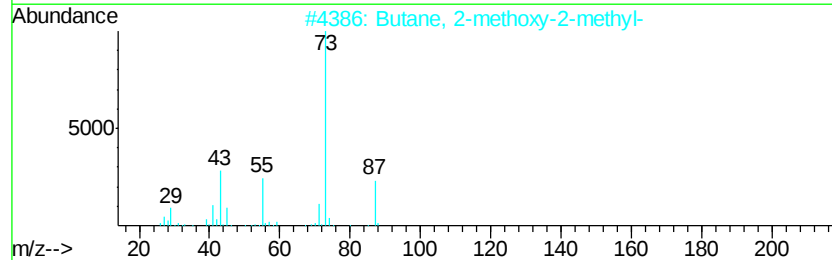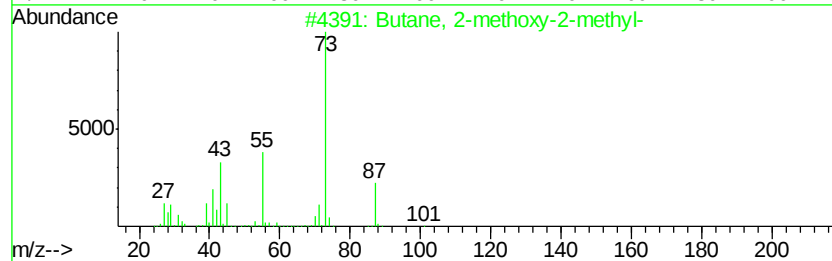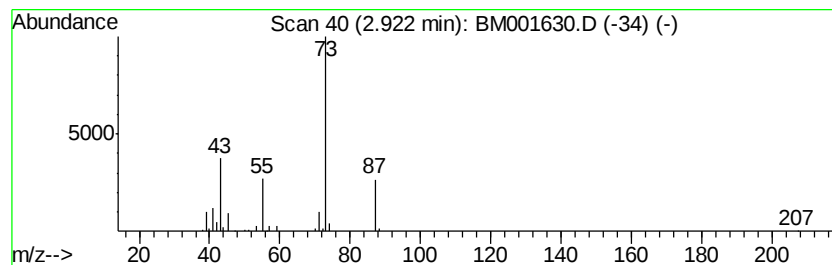

Data Path : S:\HPCHEM1\BNA_M\DATA\BM061015\
Data File : BM001630.D
Acq On : 10 Jun 2015 13:03
Operator : TP/IZ
Sample : PB83814BL
Misc : SBLK69
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK69

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM061015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	2.92	10.7	ng/ul	248936	1	7.69	463432	20.0