


Data Path : S:\HPCHEM1\BNA_M\DATA\BM061015\
Data File : BM001624.D
Acq On : 10 Jun 2015 08:45
Operator : TP/IZ
Sample : DFTPP56
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP56

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM061015.M
Title : SVOA CALIBRATION
Last Update : Wed Jun 10 13:11:01 2015

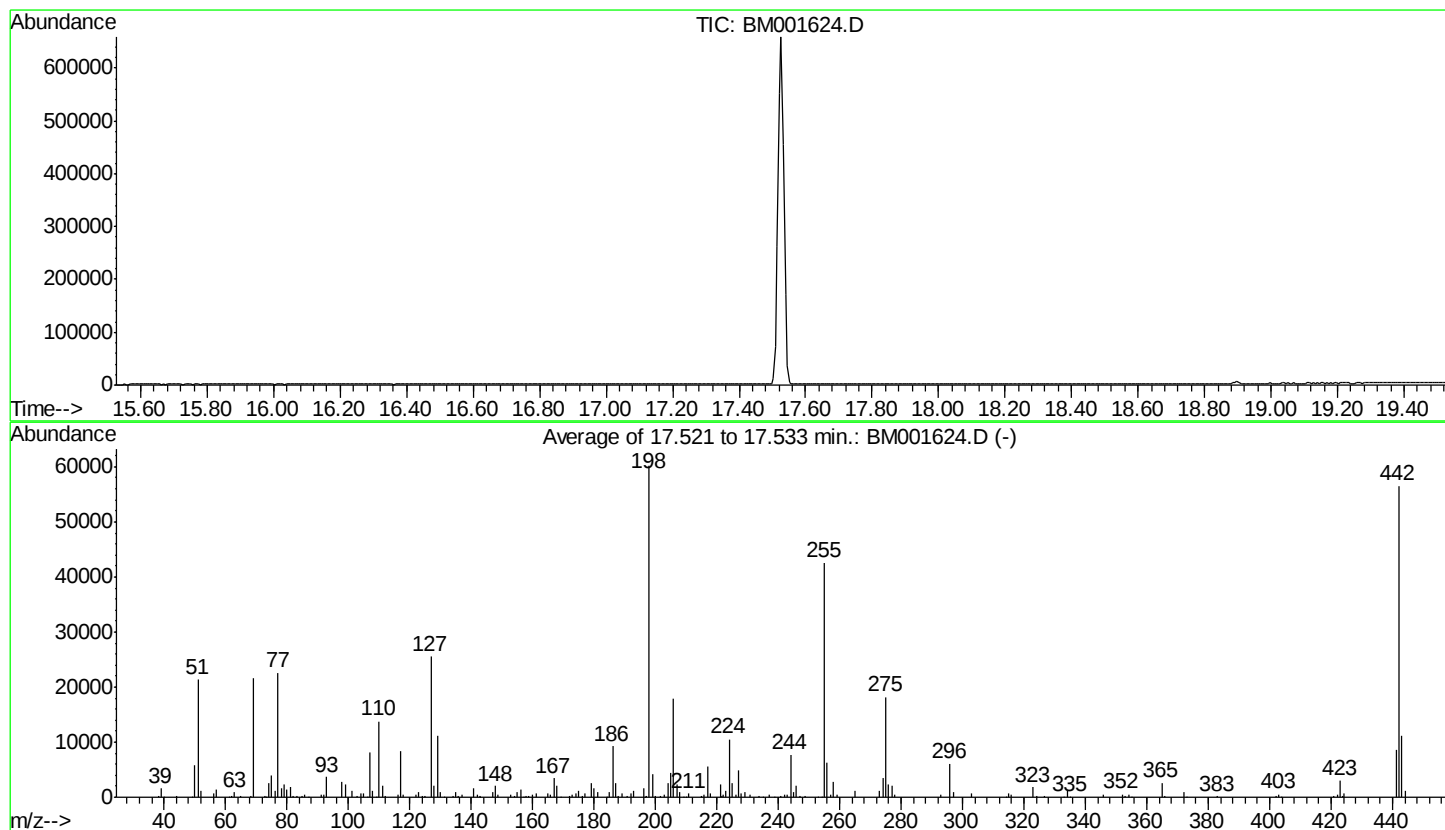

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	21319	PASS
68	69	0.00	2	1.4	301	PASS
69	198	0.00	100	35.8	21575	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.4	25525	PASS
197	198	0.00	2	0.5	276	PASS
198	198	100	100	100.0	60208	PASS
199	198	5	9	6.9	4147	PASS
275	198	10	60	30.3	18237	PASS
365	198	1	100	4.3	2601	PASS
441	443	0.01	100	78.2	8682	PASS
442	198	50	100	94.0	56600	PASS
443	442	15	24	19.6	11096	PASS

m/z	Abundance
38.00	393.0
39.00	1699.0
40.00	697.0
44.00	1340.0
49.00	305.0
50.10	6604.0
51.10	24720.0
52.10	1383.0
56.00	913.0
57.00	1638.0
61.00	321.0
61.90	372.0
63.00	993.0
65.00	555.0
68.00	386.0
69.00	23984.0
74.00	2506.0
75.00	4238.0
76.10	1385.0
77.10	24744.0
78.10	1773.0
79.00	2646.0
80.00	1588.0
81.00	2104.0
82.00	524.0
83.00	341.0
85.00	494.0
85.90	726.0
91.00	553.0
92.00	566.0
93.00	4408.0
98.00	2834.0
99.00	2688.0
101.00	1200.0
103.10	384.0
103.90	868.0
105.00	917.0
106.00	309.0
107.00	9541.0
108.00	1271.0
108.90	360.0
110.00	14642.0
111.00	2072.0
116.00	759.0
117.00	8544.0
118.00	540.0
122.00	493.0
123.00	875.0
124.00	388.0
124.90	420.0
127.00	26696.0
128.00	2267.0
129.00	11619.0
130.00	1135.0
131.00	351.0
134.00	433.0
135.00	924.0
135.90	495.0
137.00	698.0
140.90	1750.0
141.90	517.0
143.00	415.0
147.10	732.0
147.90	2207.0
148.90	399.0
153.00	424.0
154.00	456.0
155.00	836.0
156.00	1419.0
157.90	340.0
159.90	643.0
161.00	691.0
165.00	710.0
166.00	509.0
167.00	3628.0
168.00	2228.0
172.00	308.0
172.90	488.0
174.00	740.0
174.90	1204.0
176.10	362.0
176.90	613.0
178.90	2447.0
179.90	1876.0
181.00	903.0
184.10	346.0
185.00	1011.0
186.00	9274.0
187.00	2397.0
188.10	306.0
189.00	742.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56

190.90	343.0
191.90	800.0
193.00	1212.0
196.00	1857.0
197.10	300.0
198.00	61312.0
198.90	4108.0
199.90	318.0
202.90	558.0
204.00	2745.0
205.00	4420.0
206.00	18240.0
207.00	2770.0
208.00	926.0
210.90	683.0
215.10	308.0
216.00	485.0
217.00	5447.0
217.90	603.0
221.00	2308.0
222.00	660.0
222.90	944.0
224.00	10036.0
225.00	2490.0
226.10	326.0
227.00	4996.0
228.00	655.0
229.00	875.0
231.00	335.0
237.00	523.0
242.10	409.0
243.10	417.0
244.00	7202.0
245.00	1021.0
246.00	2082.0
247.00	310.0
254.10	364.0
255.00	40088.0
256.00	5793.0
257.00	622.0
258.00	2800.0
258.90	550.0
265.00	906.0
273.00	1106.0
274.00	3084.0
275.00	17024.0
276.00	2224.0
277.00	1805.0
278.00	372.0
292.90	343.0
296.00	5109.0
296.90	938.0
302.90	715.0
314.90	726.0
316.00	391.0
323.00	1376.0
324.00	343.0
334.00	1236.0
335.10	306.0
345.90	356.0
352.00	486.0
352.90	379.0
354.00	479.0
365.00	2086.0
366.00	311.0
372.00	703.0
383.00	348.0
403.00	566.0
422.10	474.0
423.00	2707.0
423.90	980.0
441.10	6832.0
442.10	44984.0
443.10	9014.0
444.10	806.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56

m/z	Abundance
38.10	330.0
39.10	1752.0
40.00	489.0
43.90	1175.0
50.10	6838.0
51.10	24712.0
52.00	1176.0
56.00	792.0
57.00	1568.0
62.00	358.0
63.00	1155.0
65.00	470.0
68.10	519.0
69.00	25760.0
72.90	398.0
74.00	3098.0
75.00	4669.0
76.10	1425.0
77.10	27160.0
78.00	1801.0
79.00	2594.0
79.90	1710.0
81.00	2217.0
82.00	490.0
83.10	562.0
86.00	566.0
87.00	345.0
91.00	562.0
92.00	569.0
93.00	3801.0
98.00	3287.0
99.00	2726.0
101.00	1249.0
102.90	414.0
103.90	749.0
105.00	966.0
107.00	9022.0
107.90	1440.0
110.00	16744.0
111.00	2548.0
112.00	381.0
116.00	646.0
117.00	10056.0
118.00	783.0
122.00	835.0
123.00	976.0
123.90	494.0
124.90	441.0
127.00	30504.0
128.00	2513.0
129.00	13081.0
129.90	998.0
133.90	401.0
135.00	1181.0
135.90	349.0
137.00	593.0
141.00	2065.0
142.00	377.0
143.10	387.0
147.00	1106.0
148.00	2374.0
148.90	461.0
152.90	734.0
153.90	350.0
155.00	1019.0
156.00	1710.0
157.20	358.0
157.80	467.0
158.90	376.0
160.00	643.0
161.00	746.0
164.90	788.0
165.90	456.0
167.00	3844.0
168.00	2364.0
169.00	308.0
171.90	304.0
173.00	467.0
174.10	714.0
175.00	1514.0
176.00	375.0
177.00	781.0
179.00	3031.0
180.00	1859.0
181.00	935.0
185.00	1415.0
186.00	11260.0
187.00	3256.0
188.00	402.0
188.90	872.0
191.00	354.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56

192.00	947.0
193.10	1339.0
196.00	1728.0
197.10	529.0
198.00	72216.0
198.90	4980.0
199.90	336.0
201.50	450.0
203.00	750.0
204.00	3155.0
205.00	4768.0
206.00	20168.0
207.10	3021.0
208.00	1256.0
209.00	308.0
210.10	363.0
210.90	803.0
214.80	378.0
216.00	624.0
217.00	6466.0
217.90	710.0
221.00	2578.0
221.90	899.0
223.00	1563.0
224.00	12267.0
225.00	2782.0
226.00	404.0
227.00	5463.0
227.90	749.0
229.00	1116.0
231.00	460.0
233.90	453.0
234.90	361.0
237.00	656.0
238.90	342.0
241.00	359.0
242.10	555.0
243.10	724.0
244.00	9278.0
245.10	1304.0
246.00	2337.0
247.00	422.0
248.90	373.0
253.00	343.0
255.00	50400.0
256.00	7480.0
257.00	487.0
258.00	3169.0
259.00	799.0
265.00	1587.0
273.00	1207.0
274.00	4000.0
275.00	21848.0
276.00	2569.0
277.00	2484.0
278.00	494.0
293.00	463.0
296.00	7399.0
297.00	944.0
302.90	546.0
314.90	843.0
316.00	421.0
323.10	2379.0
324.10	450.0
326.80	447.0
332.90	371.0
334.00	1306.0
346.00	481.0
351.90	602.0
353.00	405.0
354.10	633.0
355.00	303.0
365.00	3173.0
366.00	344.0
372.10	1094.0
373.10	307.0
382.90	316.0
402.00	370.0
403.00	563.0
403.90	306.0
420.90	331.0
421.90	473.0
423.10	3406.0
424.10	1244.0
441.10	10131.0
442.10	65664.0
443.10	13425.0
444.10	1226.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56

m/z	Abundance
39.10	1210.0
40.00	467.0
44.00	1268.0
50.00	3856.0
51.10	14525.0
52.00	702.0
56.10	431.0
57.00	792.0
63.00	576.0
69.00	14981.0
73.10	345.0
74.00	1840.0
75.00	2845.0
76.00	951.0
77.10	16068.0
78.10	1298.0
79.00	1524.0
80.00	1043.0
81.00	1626.0
86.00	406.0
91.00	388.0
91.90	419.0
93.00	2768.0
98.00	2140.0
99.00	1675.0
101.00	765.0
103.90	530.0
104.90	557.0
107.00	6065.0
107.90	960.0
110.00	9833.0
111.00	1627.0
117.00	6211.0
118.10	364.0
123.00	645.0
127.00	19376.0
128.00	1709.0
129.00	8466.0
129.90	694.0
134.90	762.0
136.90	365.0
140.90	1292.0
142.00	490.0
142.80	316.0
146.90	777.0
148.00	1640.0
148.90	364.0
153.00	534.0
155.10	636.0
156.00	1167.0
159.90	386.0
161.00	772.0
165.00	590.0
166.00	358.0
167.00	2970.0
167.90	1537.0
171.90	322.0
172.90	405.0
173.90	545.0
175.10	964.0
177.10	423.0
179.00	1904.0
180.00	1203.0
181.00	722.0
184.90	725.0
186.00	7055.0
186.90	2108.0
189.10	604.0
190.90	360.0
191.80	537.0
193.10	841.0
196.00	1220.0
196.80	308.0
198.00	47096.0
199.00	3355.0
201.40	308.0
202.90	461.0
204.00	2063.0
205.00	4045.0
206.00	15599.0
207.10	2635.0
207.90	751.0
211.00	580.0
217.00	4644.0
217.90	576.0
221.10	1834.0
221.70	544.0
223.00	963.0
224.00	9193.0
225.00	2148.0
226.00	370.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56

227.00	4025.0
227.90	379.0
229.00	1036.0
231.00	367.0
236.90	475.0
240.90	352.0
241.90	440.0
242.90	357.0
244.00	6616.0
245.10	768.0
246.00	1590.0
255.00	37144.0
256.00	5462.0
257.00	376.0
258.00	2386.0
258.90	412.0
265.00	1303.0
272.90	985.0
274.00	3070.0
275.00	15841.0
276.00	2304.0
277.00	1892.0
278.10	352.0
292.90	373.0
296.00	5711.0
297.00	734.0
303.00	682.0
314.10	371.0
315.00	635.0
316.00	347.0
323.00	1752.0
326.90	305.0
334.00	1125.0
346.00	406.0
352.10	534.0
353.90	324.0
365.00	2545.0
365.90	406.0
372.00	1019.0
402.00	603.0
403.00	489.0
421.00	558.0
421.90	375.0
423.00	2858.0
424.00	641.0
441.10	9085.0
442.10	59152.0
443.10	10850.0
444.00	1130.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56

Scan 2517 (17.492 min): BM001624.D
DFTPP56

m/z	Abundance
39.90	473.0
44.00	1096.0
206.90	481.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56