


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061016\
Data File : BM005717.D
Acq On : 10 Jun 2016 23:28
Operator : UM/SJ
Sample : DFTPP52
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP52

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Title : SVOA CALIBRATION
Last Update : Sat Apr 23 01:00:10 2016

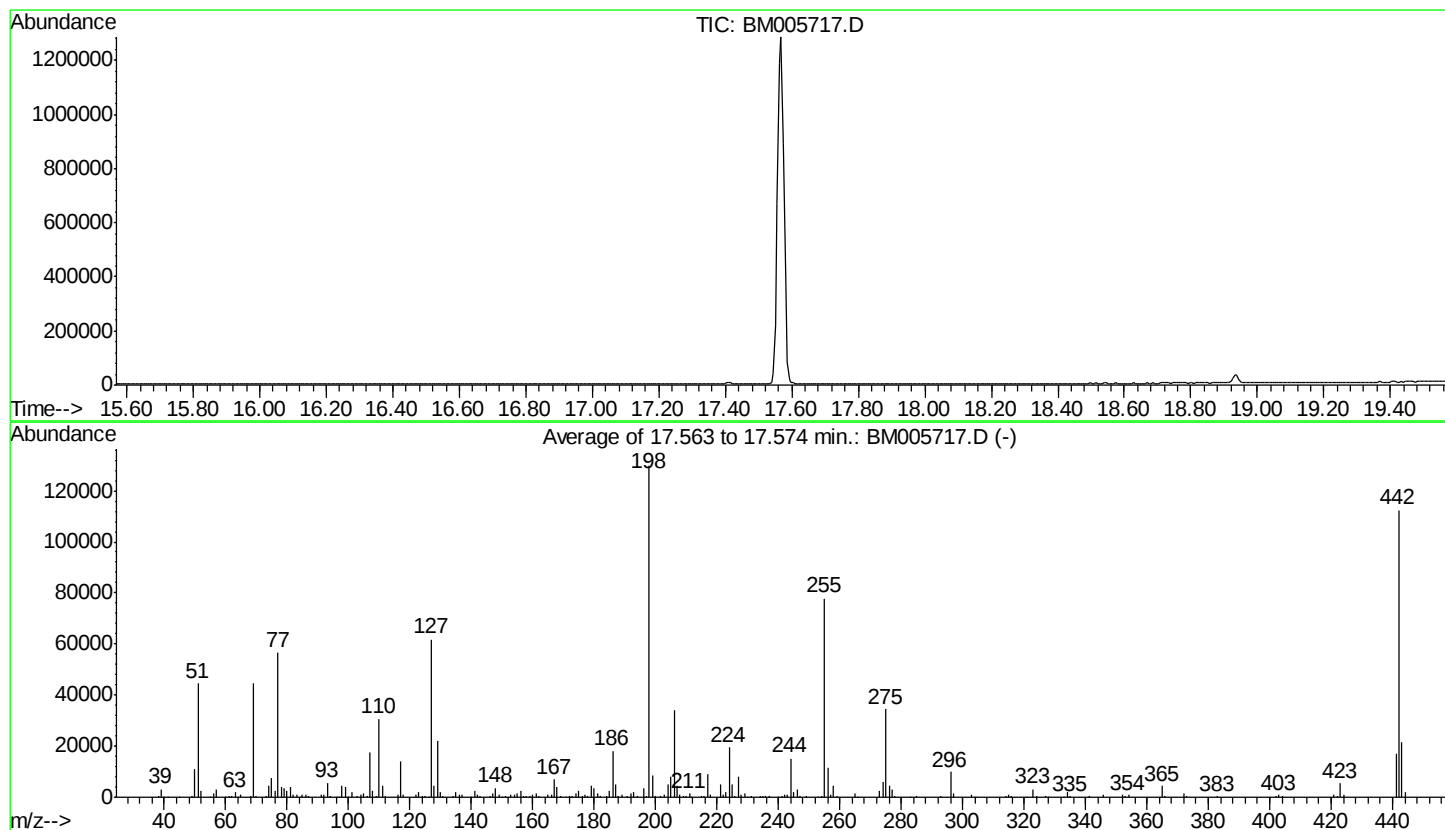

AutoFind: Scans 2546, 2547, 2548; Background Corrected with Scan 2540

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	44504	PASS
68	69	0.00	2	1.7	744	PASS
69	198	0.00	100	34.5	44773	PASS
70	69	0.00	2	0.6	275	PASS
127	198	10	80	47.5	61696	PASS
197	198	0.00	2	0.5	694	PASS
198	198	100	100	100.0	129842	PASS
199	198	5	9	6.7	8749	PASS
275	198	10	60	26.6	34520	PASS
365	198	1	100	3.4	4465	PASS
441	443	0.01	100	78.1	16874	PASS
442	198	50	100	86.5	112314	PASS
443	442	15	24	19.2	21618	PASS

m/z	Abundance
38.00	631.0
39.10	3871.0
40.00	544.0
41.00	654.0
43.00	773.0
44.00	633.0
49.00	515.0
50.00	12911.0
51.00	52400.0
52.00	2986.0
55.00	723.0
56.00	1498.0
57.00	4017.0
59.90	324.0
61.00	685.0
62.00	825.0
63.00	2001.0
64.00	322.0
65.00	1059.0
68.00	872.0
69.00	52856.0
70.00	417.0
73.00	664.0
74.00	5308.0
75.00	8691.0
76.00	2888.0
77.00	64840.0
78.00	4672.0
79.00	3729.0
80.00	2905.0
81.00	4278.0
82.00	1093.0
83.00	1237.0
85.00	1044.0
86.00	1170.0
87.00	594.0
91.00	1071.0
92.00	1100.0
93.00	6801.0
93.90	541.0
96.00	360.0
97.10	314.0
98.00	5365.0
99.00	4585.0
99.90	400.0
101.00	2568.0
103.00	806.0
104.00	1287.0
105.00	1531.0
106.00	567.0
107.00	20592.0
108.00	3243.0
109.00	545.0
110.00	34480.0
111.00	5421.0
111.90	631.0
116.00	1014.0
117.00	15986.0
118.00	1219.0
122.00	1248.0
123.00	2215.0
124.00	919.0
125.00	809.0
126.10	402.0
127.00	69144.0
128.00	4960.0
129.00	24992.0
130.00	2173.0
130.90	426.0
134.00	615.0
135.00	2151.0
136.00	828.0
137.00	1113.0
140.00	305.0
141.00	3226.0
142.00	1083.0
142.90	707.0
145.90	641.0
147.00	1598.0
147.90	4005.0
149.00	979.0
151.00	454.0
153.00	1058.0
154.00	886.0
155.00	1994.0
156.00	2870.0
157.10	606.0
157.90	644.0
159.00	562.0
160.00	928.0
161.00	1531.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

162.00	557.0
165.00	1166.0
165.90	805.0
167.00	7909.0
168.00	4002.0
168.90	692.0
171.90	664.0
173.00	813.0
174.00	1411.0
175.00	2850.0
176.00	901.0
177.00	1260.0
177.90	464.0
179.00	4458.0
180.00	3545.0
181.00	1657.0
182.00	387.0
184.00	366.0
185.00	2653.0
186.00	19592.0
187.00	5481.0
188.00	622.0
188.90	1118.0
190.90	555.0
192.00	1759.0
193.00	2013.0
194.00	378.0
196.00	4007.0
197.00	681.0
198.00	140224.0
199.00	9883.0
200.00	776.0
201.40	593.0
202.90	897.0
204.00	5276.0
205.00	8471.0
206.00	36496.0
207.00	5205.0
208.00	1288.0
209.00	418.0
210.00	555.0
211.00	1438.0
211.70	306.0
214.90	462.0
215.90	714.0
217.00	9494.0
218.00	1309.0
221.00	4898.0
221.80	1221.0
223.00	2309.0
224.00	19784.0
225.00	5226.0
226.00	601.0
227.00	8386.0
228.00	1158.0
229.00	1921.0
231.00	709.0
234.00	499.0
235.00	590.0
235.90	531.0
237.00	801.0
241.00	447.0
242.00	1128.0
243.00	1129.0
244.00	15701.0
245.00	2066.0
246.00	3227.0
247.00	639.0
249.00	464.0
254.10	604.0
255.00	78480.0
256.00	11905.0
257.00	1053.0
258.00	4363.0
259.00	723.0
265.00	1890.0
265.90	322.0
273.00	2552.0
274.00	6031.0
275.00	33800.0
276.00	4720.0
277.00	3105.0
278.00	611.0
283.00	373.0
285.00	623.0
293.00	594.0
296.00	9455.0
297.00	1444.0
303.00	1140.0
304.00	360.0
314.00	463.0
315.00	1099.0
315.90	573.0
323.00	3043.0
324.00	510.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

327.00	601.0
333.00	319.0
334.00	1884.0
335.00	422.0
346.00	696.0
352.00	932.0
353.00	584.0
354.00	986.0
365.00	4097.0
365.90	635.0
372.10	1471.0
373.00	324.0
382.90	448.0
402.00	613.0
403.00	577.0
404.00	335.0
421.00	711.0
422.00	694.0
423.00	4637.0
424.00	1138.0
441.10	14406.0
442.00	97432.0
443.00	19152.0
444.00	1818.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

m/z	Abundance
38.00	662.0
39.00	3642.0
40.00	448.0
41.00	569.0
41.90	354.0
43.00	729.0
44.00	776.0
45.00	332.0
49.00	437.0
50.00	12567.0
51.00	50032.0
52.00	2702.0
55.00	666.0
56.00	1671.0
57.00	3800.0
61.00	560.0
62.00	794.0
63.00	2024.0
64.00	327.0
65.00	1128.0
68.00	781.0
69.00	49792.0
70.00	409.0
73.00	686.0
74.00	5194.0
75.00	8440.0
76.00	2735.0
77.00	63856.0
78.00	4609.0
79.00	3977.0
80.00	2833.0
81.00	4482.0
82.00	1233.0
83.00	1069.0
83.90	366.0
85.00	955.0
86.00	1221.0
87.00	571.0
91.00	1097.0
92.00	1038.0
93.00	6444.0
93.90	442.0
96.00	345.0
98.00	4871.0
99.00	4133.0
100.00	365.0
101.00	2425.0
102.90	700.0
103.90	1438.0
105.00	1666.0
106.00	417.0
107.00	20056.0
108.00	3072.0
109.10	475.0
110.00	34272.0
111.00	5196.0
112.00	693.0
116.00	1074.0
117.00	15858.0
118.00	1253.0
122.00	1178.0
123.00	2128.0
124.00	874.0
125.00	835.0
126.00	370.0
127.00	69760.0
128.00	5226.0
129.00	25112.0
130.00	2185.0
131.00	494.0
134.00	689.0
135.00	2092.0
136.00	936.0
137.00	1137.0
139.90	335.0
141.00	3090.0
142.00	1082.0
142.90	763.0
146.00	570.0
147.00	1800.0
148.00	3990.0
149.00	788.0
150.00	332.0
151.10	440.0
152.90	1119.0
154.00	895.0
155.00	1872.0
156.00	2934.0
157.00	573.0
157.90	523.0
158.90	400.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

159.90	1038.0
161.00	1816.0
161.90	458.0
165.00	1279.0
166.00	1058.0
167.00	7638.0
168.00	4337.0
169.00	862.0
170.90	411.0
171.90	636.0
173.00	856.0
174.00	1506.0
175.00	2886.0
176.00	741.0
177.00	1301.0
178.00	464.0
179.00	5317.0
180.00	3739.0
181.00	2029.0
182.00	366.0
184.00	457.0
185.00	2696.0
186.00	20824.0
187.00	6169.0
188.00	638.0
189.00	1271.0
190.90	686.0
192.00	1795.0
193.00	2155.0
194.00	468.0
196.00	3964.0
197.00	728.0
198.00	148480.0
199.00	9880.0
200.00	911.0
201.50	584.0
203.00	1056.0
204.00	5499.0
205.00	8984.0
206.00	39184.0
207.00	5214.0
208.00	1287.0
209.00	486.0
210.00	467.0
211.00	1557.0
215.00	469.0
216.00	933.0
217.00	10611.0
217.90	1397.0
221.10	5546.0
221.80	1356.0
223.00	2158.0
224.00	22320.0
225.00	5656.0
226.00	506.0
227.00	9071.0
228.00	1440.0
229.00	1970.0
229.90	329.0
231.00	925.0
233.90	588.0
235.00	752.0
236.00	460.0
237.00	696.0
239.90	345.0
241.00	437.0
241.90	1161.0
243.00	1240.0
244.00	17568.0
245.00	2403.0
246.00	3705.0
247.00	772.0
248.90	575.0
253.00	432.0
254.10	736.0
255.00	91632.0
256.00	13736.0
257.00	994.0
258.00	5255.0
259.00	845.0
265.00	1995.0
266.00	300.0
273.00	2651.0
274.00	7416.0
275.00	40144.0
276.00	4967.0
277.00	3472.0
278.00	501.0
283.00	343.0
285.00	673.0
293.00	791.0
296.00	11363.0
297.00	1557.0
303.00	1336.0
304.00	389.0

Instrument :

BNA_M

ClientSampleId :

DFTPP52

314.00	573.0
315.00	1241.0
316.00	640.0
320.90	368.0
323.00	3948.0
324.00	617.0
327.00	643.0
327.90	317.0
333.00	335.0
334.00	2468.0
335.00	589.0
341.00	468.0
346.00	943.0
352.00	924.0
353.00	671.0
354.00	1203.0
365.00	5255.0
366.00	795.0
372.00	1891.0
373.00	466.0
383.00	499.0
402.00	685.0
403.00	1110.0
403.90	307.0
421.00	896.0
422.00	837.0
423.00	6612.0
424.00	1271.0
441.00	19784.0
442.10	132032.0
443.00	25408.0
444.00	2310.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

m/z	Abundance
38.00	396.0
39.00	2670.0
40.00	465.0
41.00	732.0
42.00	301.0
43.00	764.0
44.00	894.0
50.00	7474.0
51.00	31080.0
52.00	1751.0
55.00	628.0
56.00	1096.0
57.00	2639.0
60.00	340.0
60.90	452.0
62.00	453.0
63.00	1329.0
65.00	708.0
68.00	581.0
69.00	31672.0
73.00	639.0
74.00	3297.0
75.00	5456.0
76.00	2019.0
77.00	41136.0
78.00	2973.0
79.00	2407.0
80.00	1798.0
81.00	2689.0
82.00	748.0
83.00	864.0
85.00	736.0
85.90	864.0
87.00	412.0
91.00	838.0
92.00	666.0
93.00	3948.0
94.00	431.0
98.00	3146.0
99.00	2799.0
101.00	1658.0
103.00	554.0
103.90	844.0
104.90	954.0
106.00	355.0
107.00	12410.0
108.00	1915.0
109.00	428.0
110.00	23056.0
110.90	3349.0
112.00	437.0
115.90	686.0
117.00	10269.0
118.00	778.0
122.00	897.0
123.00	1389.0
123.90	497.0
124.90	581.0
127.00	46184.0
128.00	3262.0
129.00	16544.0
129.90	1383.0
130.80	309.0
133.90	481.0
135.00	1435.0
136.00	547.0
137.00	988.0
141.00	1841.0
142.00	715.0
142.90	528.0
146.00	414.0
146.90	1074.0
148.00	2618.0
149.00	686.0
151.10	302.0
153.00	636.0
154.00	634.0
155.00	1460.0
156.00	2158.0
156.90	303.0
158.00	324.0
158.90	351.0
160.00	591.0
161.00	1149.0
164.90	818.0
166.00	707.0
167.00	5438.0
168.00	2997.0
169.00	621.0
171.90	372.0
172.90	547.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

174.00	1068.0
175.00	2124.0
176.00	604.0
176.90	875.0
178.00	350.0
179.00	3409.0
180.00	2558.0
180.90	1204.0
182.00	307.0
184.00	314.0
185.00	1762.0
186.00	13901.0
187.00	4149.0
188.00	415.0
188.90	851.0
190.90	502.0
192.00	1219.0
192.90	1364.0
193.90	325.0
196.00	2561.0
197.00	675.0
198.00	100824.0
199.00	6486.0
199.90	504.0
201.50	348.0
203.00	702.0
204.00	3806.0
205.00	6559.0
206.00	27144.0
207.00	3767.0
208.00	963.0
208.90	421.0
210.00	435.0
211.00	1173.0
216.00	619.0
217.00	6885.0
218.00	867.0
221.00	4202.0
221.80	960.0
223.00	1563.0
224.00	15976.0
225.00	4203.0
225.90	393.0
227.00	6428.0
228.00	919.0
228.90	1306.0
231.00	601.0
234.00	390.0
235.00	494.0
235.90	329.0
237.00	556.0
241.00	309.0
242.00	789.0
243.00	953.0
244.00	12621.0
245.10	1446.0
246.00	2410.0
246.90	523.0
248.90	361.0
254.00	358.0
255.00	63608.0
256.00	9261.0
257.00	669.0
258.00	3675.0
258.90	568.0
265.00	1409.0
273.00	1972.0
274.00	5388.0
275.00	29616.0
276.00	3441.0
277.00	2561.0
278.00	330.0
285.00	464.0
293.00	581.0
296.00	8796.0
297.00	1225.0
303.00	1043.0
314.00	455.0
315.00	811.0
316.00	400.0
323.00	2545.0
324.00	511.0
327.00	565.0
328.00	325.0
334.00	1934.0
335.00	426.0
341.00	364.0
345.90	764.0
352.00	797.0
353.00	676.0
354.10	805.0
365.00	4044.0
366.00	581.0
372.00	1547.0
373.00	329.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

383.00	449.0
402.00	556.0
403.00	904.0
403.90	333.0
421.00	851.0
422.00	722.0
423.00	5278.0
424.00	1104.0
441.00	16432.0
442.00	107480.0
443.10	20296.0
444.00	1872.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52

Scan 2540 (17.527 min): BM005717.D
DFTPP52

m/z	Abundance
39.00	357.0
39.90	415.0
41.00	600.0
42.00	355.0
43.00	936.0
44.00	844.0
55.00	454.0
57.00	555.0
73.00	342.0
207.10	319.0

Instrument :
BNA_M
ClientSampleId :
DFTPP52