
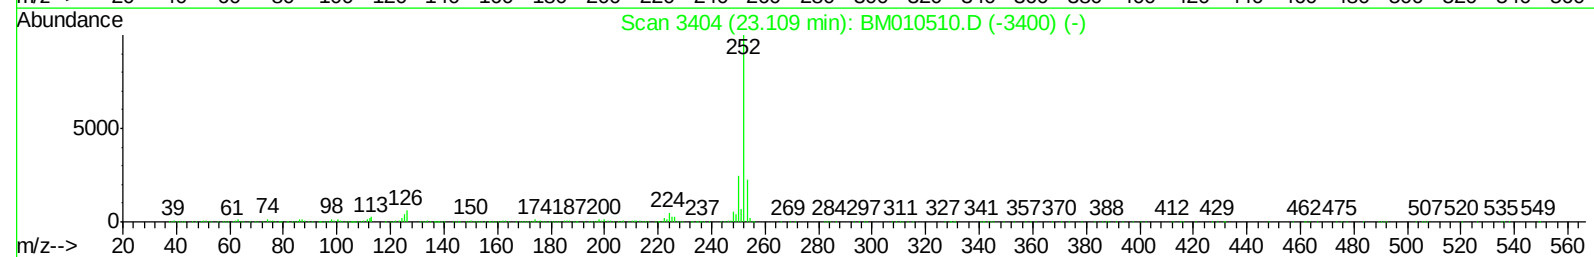
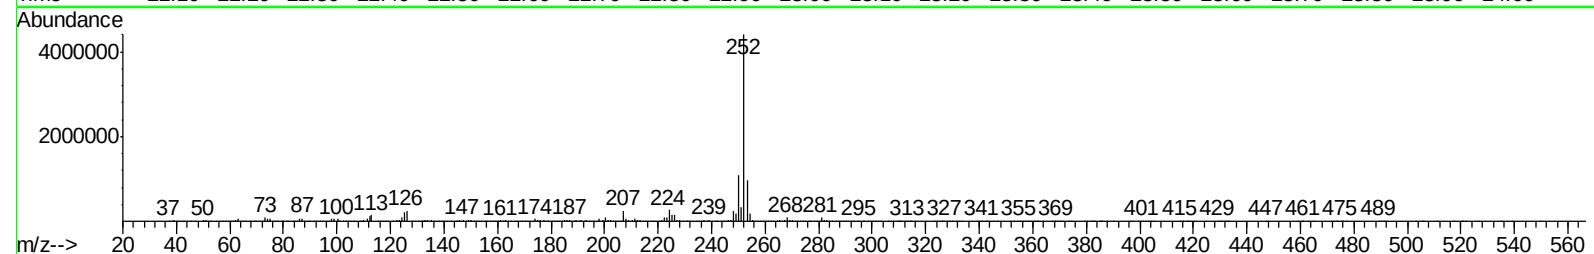


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010511.D
Acq On : 11 Jun 2017 06:34
Operator : SJ/MA
Sample : I3521-10
Misc :
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Jun 12 09:20:57 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:37 2017
Response via : Initial Calibration

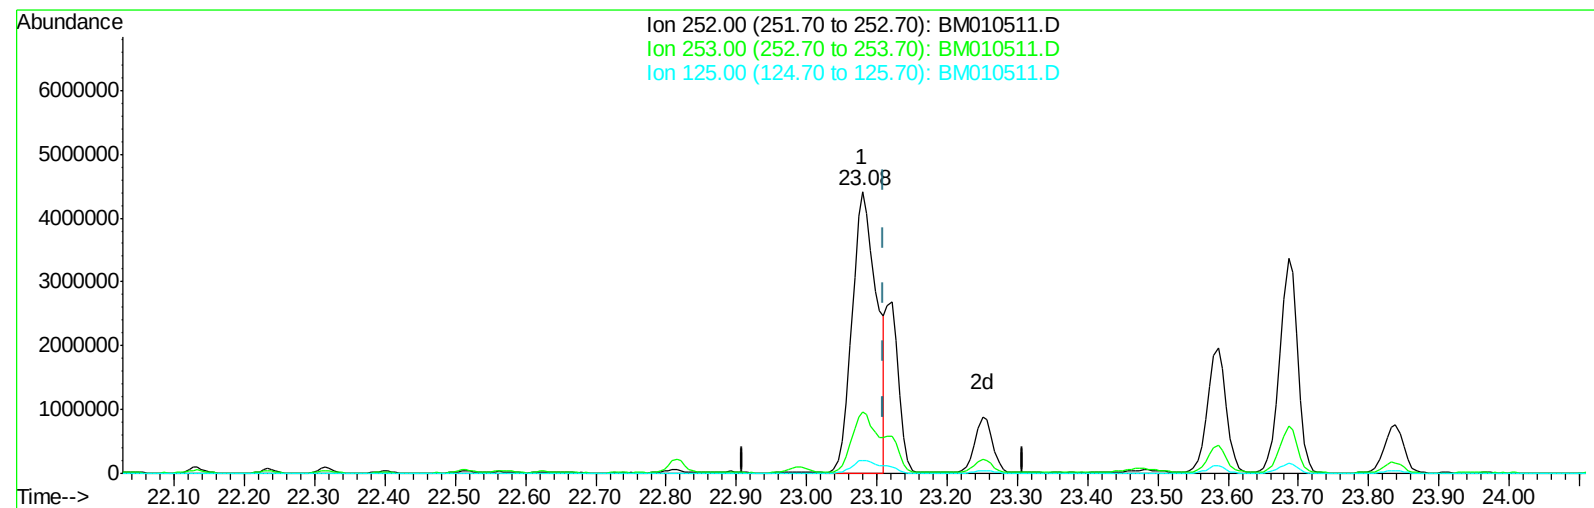

TIC: BM010511.D

(86) Benzo(k)fluoranthene

23.080min (-0.029) 106.84ng/ul

response 10850636

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	21.80
125.00	4.30	4.70
0.00	0.00	0.00