
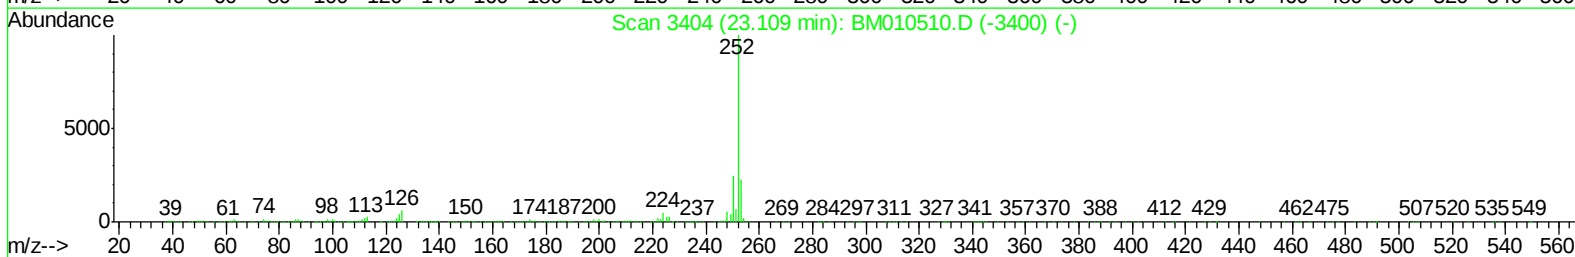
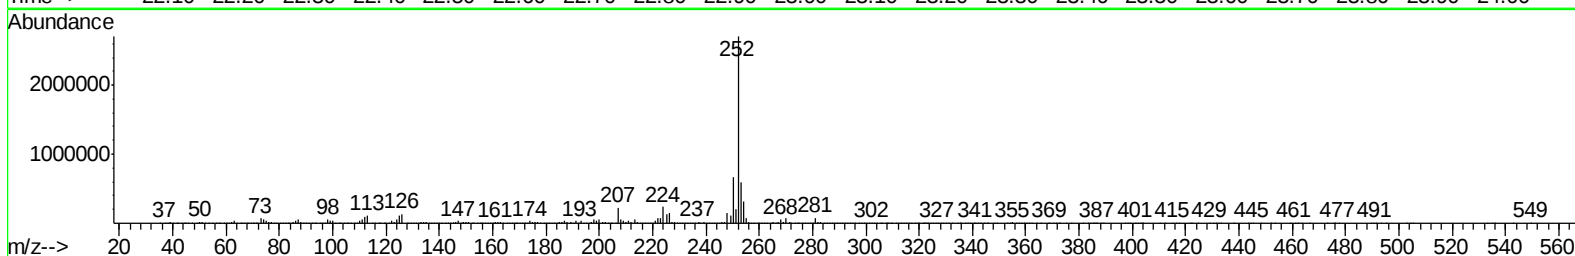


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010513.D
Acq On : 11 Jun 2017 07:46
Operator : SJ/MA
Sample : I3520-15
Misc :
ALS Vial : 38 Sample Multiplier: 1

Quant Time: Jun 12 09:07:32 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

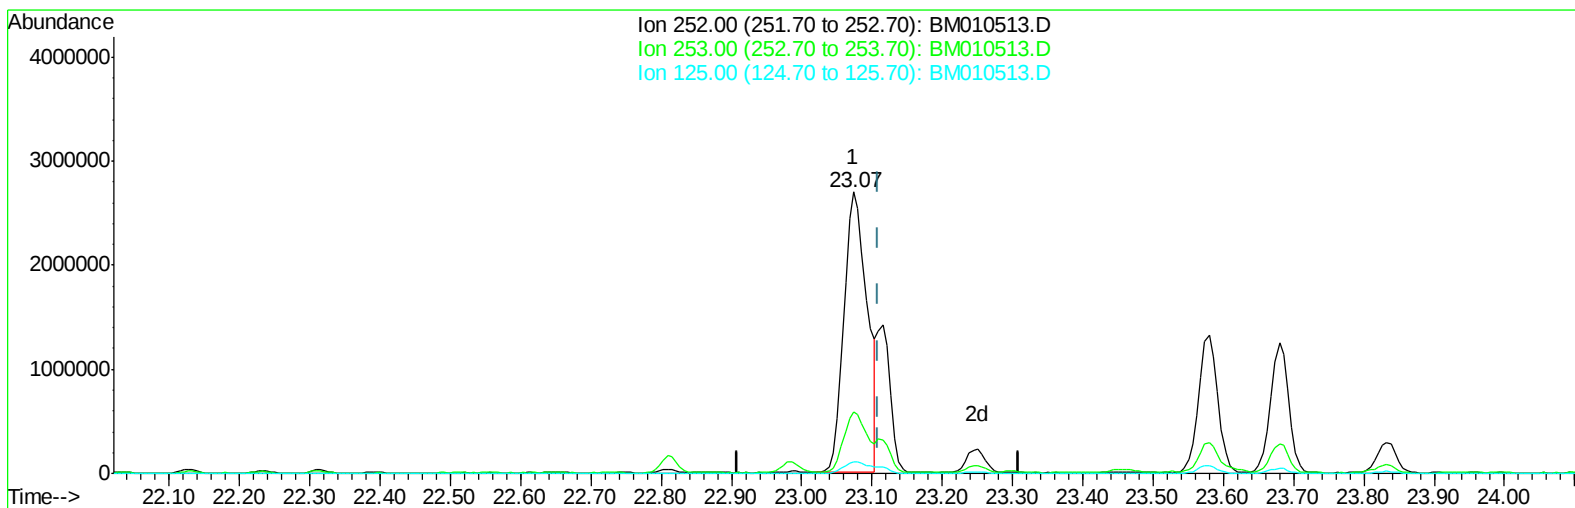

TIC: BM010513.D

(86) Benzo(k)fluoranthene

23.074min (-0.035) 77.29ng/ul

response 6280236

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	21.85
125.00	4.30	4.05
0.00	0.00	0.00