
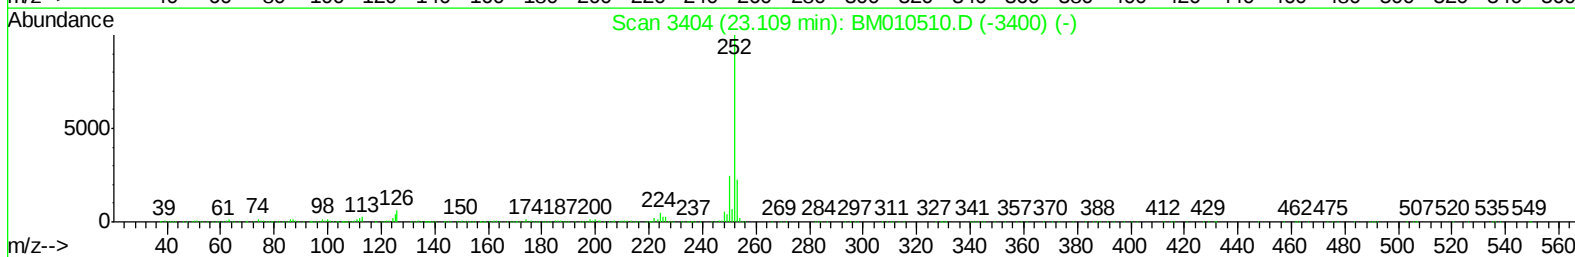
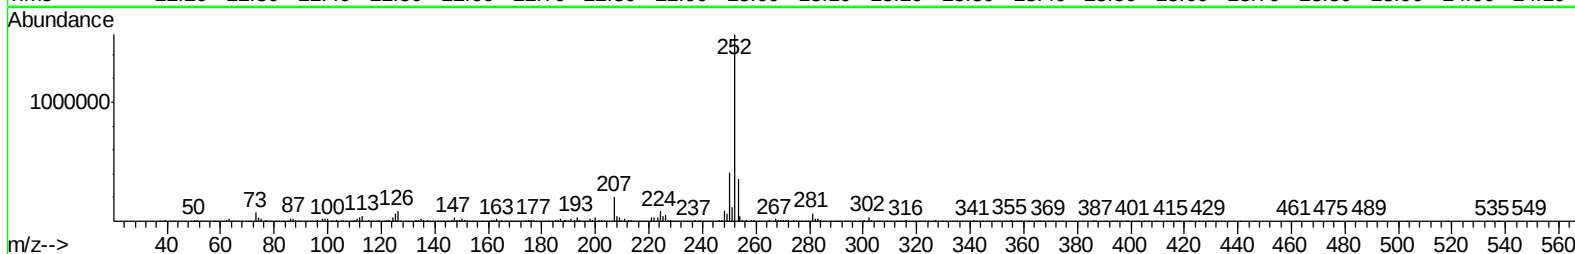


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010516.D
Acq On : 11 Jun 2017 09:34
Operator : SJ/MA
Sample : I3522-16
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Jun 12 09:08:23 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

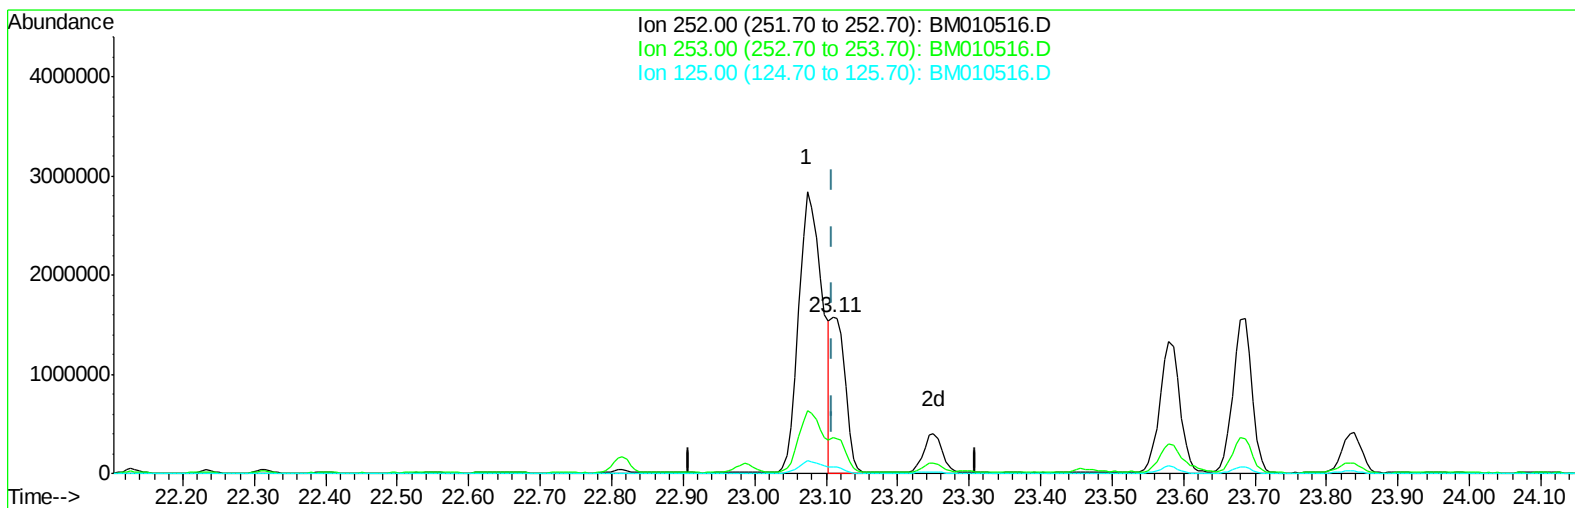

TIC: BM010516.D

(86) Benzo(k)fluoranthene

23.109min (+0.000) 17.47ng/ul m

response 2131942

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.93
125.00	4.30	3.98
0.00	0.00	0.00