
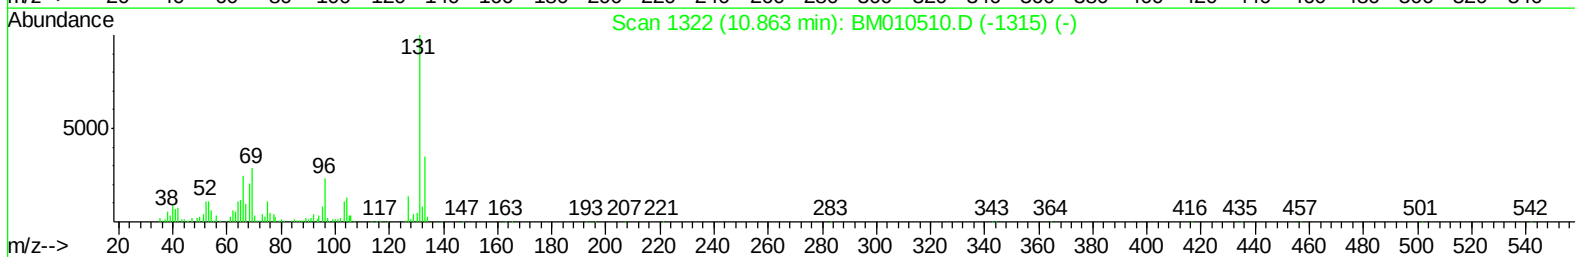
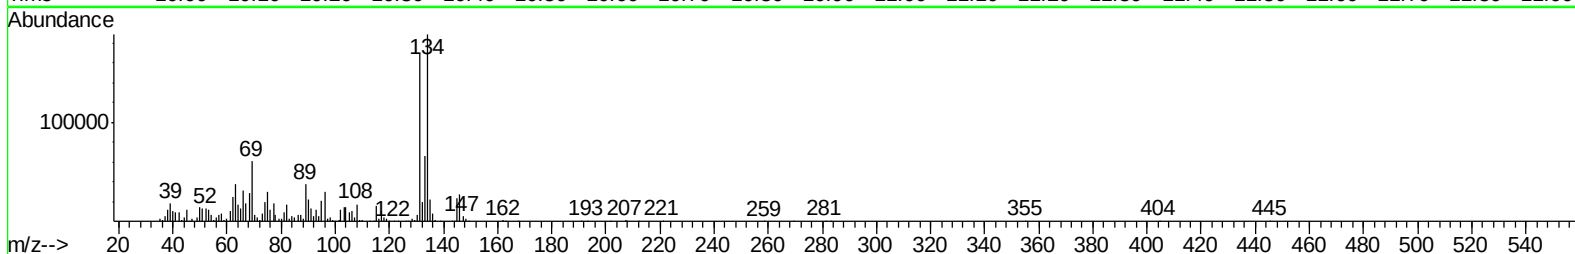


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Quant Time: Jun 12 09:08:39 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

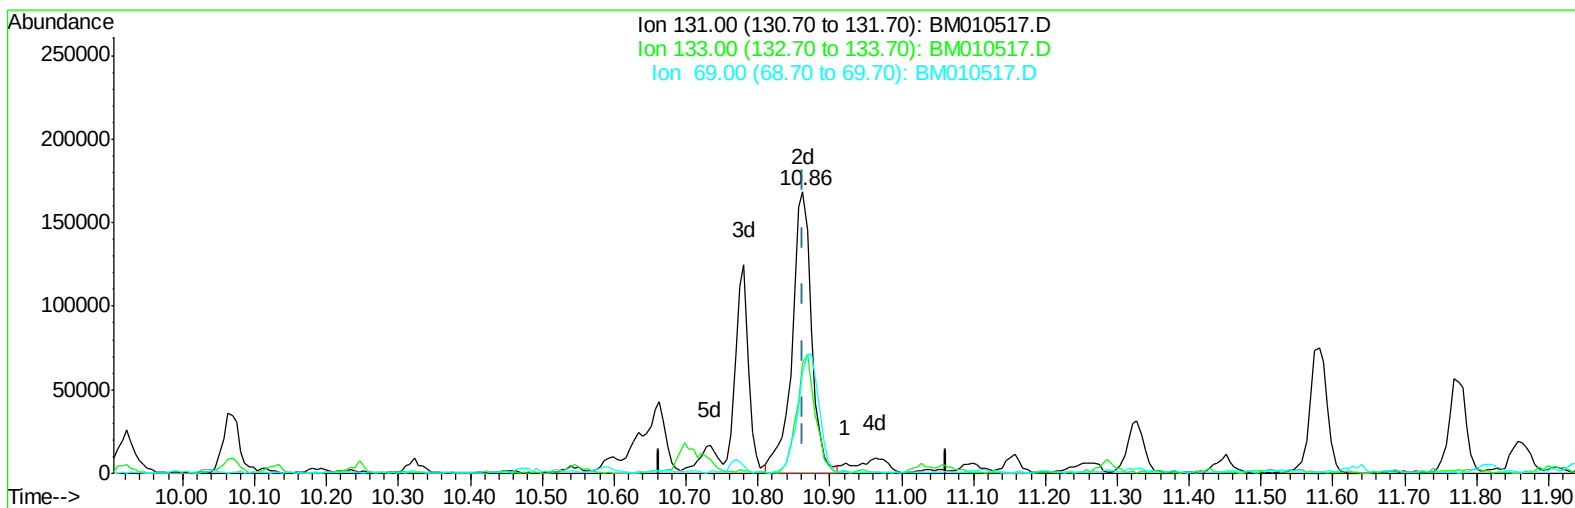

TIC: BM010517.D

(29) 4-Chloroaniline-d4 (S)

10.863min (+0.000) 30.90ng/ul m

response 320406

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	39.11#
69.00	24.30	36.10#
0.00	0.00	0.00