
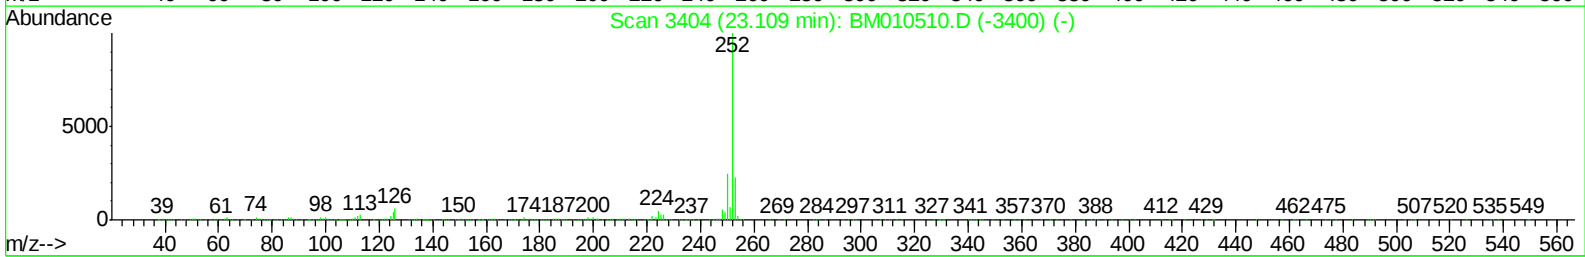
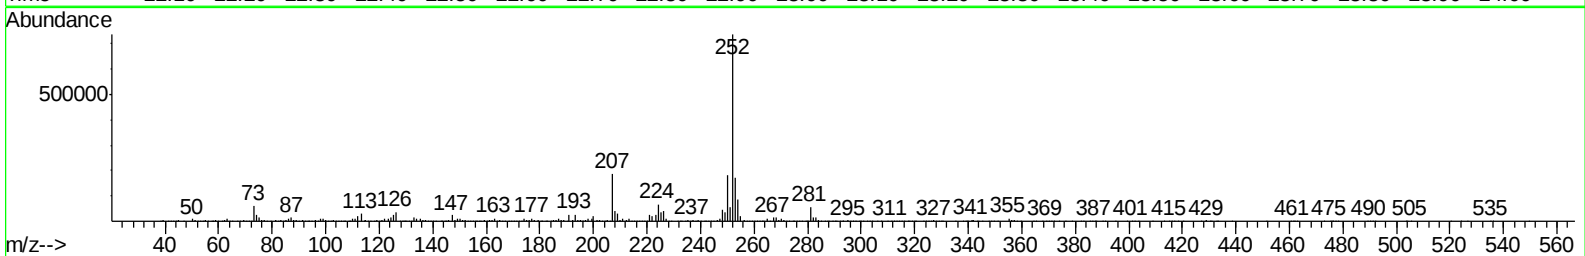


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010522.D
Acq On : 11 Jun 2017 13:10
Operator : SJ/MA
Sample : I3522-01
Misc :
ALS Vial : 47 Sample Multiplier: 1

Quant Time: Jun 12 10:06:43 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

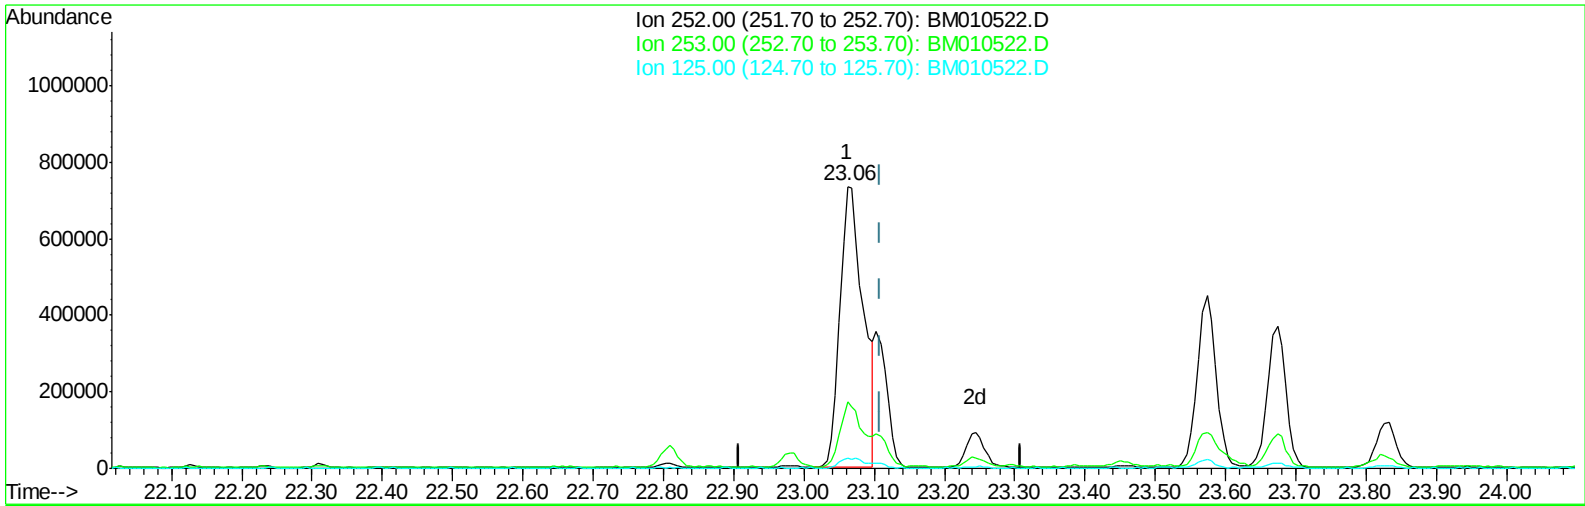

TIC: BM010522.D

(86) Benzo(k)fluoranthene

23.062min (-0.047) 23.65ng/ul

response 1717521

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	23.48
125.00	4.30	3.80
0.00	0.00	0.00