
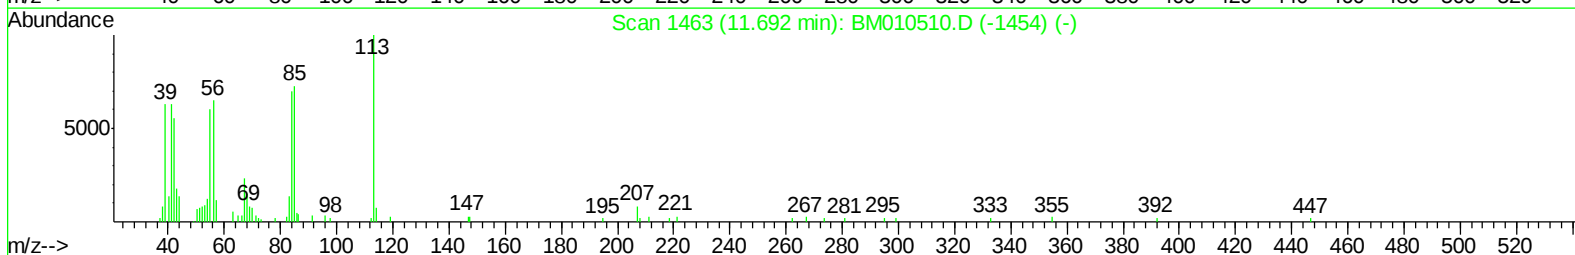
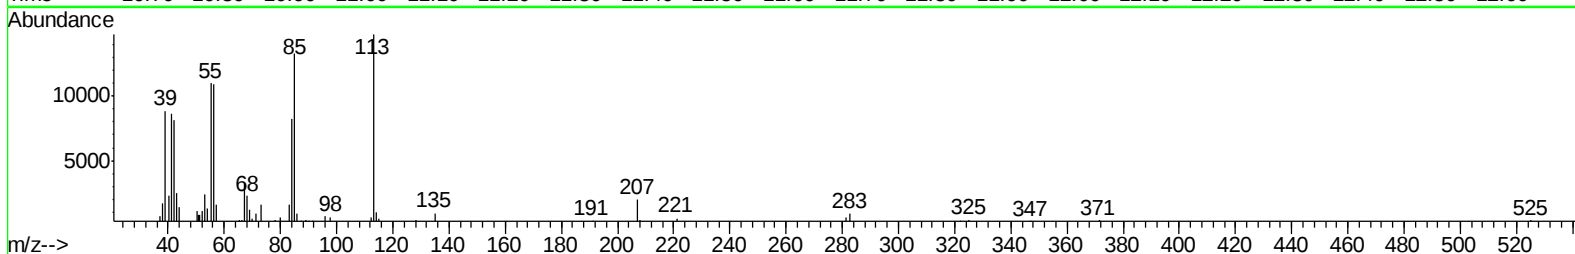


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010525.D
Acq On : 11 Jun 2017 14:58
Operator : SJ/MA
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jun 12 09:10:53 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

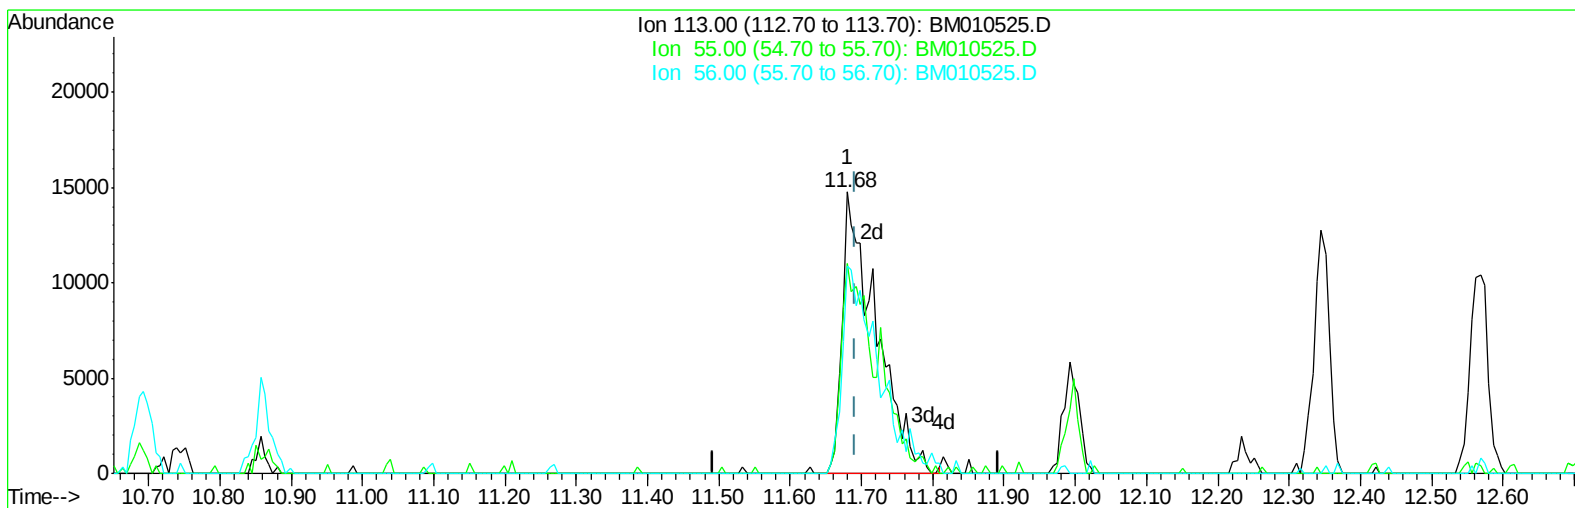

TIC: BM010525.D

(32) Caprolactam

11.680min (-0.012) 20.31ng/ul m

response 48673

Ion	Exp%	Act%
113.00	100	100
55.00	118.50	74.47#
56.00	107.50	73.65#
0.00	0.00	0.00