

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
 Data File : BM010486.D
 Acq On : 10 Jun 2017 15:34
 Operator : SJ/MA
 Sample : PB99638BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK38

Quant Time: Jun 12 04:17:35 2017
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 12 04:15:09 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	171973	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	637805	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.53	164	423023	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.28	188	1061733	20.00	ng/ul	0.00
75) Chrysene-d12	21.44	240	1337766	20.00	ng/ul	0.00
83) Perylene-d12	23.79	264	1413809	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.36	96	22121	5.28	ng/uL	0.00
5) Phenol-d5	7.08	99	359770	27.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.23	67	206484	28.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.43	132	319192	30.73	ng/ul	0.00
13) 4-Methylphenol-d8	8.62	113	302004	28.72	ng/ul	0.00
19) Nitrobenzene-d5	9.08	128	148729	31.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.79	143	194377	35.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.32	165	381548	34.32	ng/ul	0.00
29) 4-Chloroaniline-d4	10.86	131	400867	37.37	ng/ul	0.00
43) Dimethylphthalate-d6	13.94	166	1381786	39.31	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	1420438	34.64	ng/ul	0.00
51) 4-Nitrophenol-d4	14.77	143	184627	35.11	ng/ul	0.00
57) Fluorene-d10	15.53	176	1122808	36.34	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.65	200	243600	32.39	ng/ul	0.00
70) Anthracene-d10	17.38	188	1921407	37.19	ng/ul	0.00
76) Pyrene-d10	19.67	212	2275980	41.14	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.63	264	2451741	37.25	ng/ul	0.00


Target Compounds					Qvalue
21) Isophorone	9.80	82	33037	1.609 ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010486.D
Acq On : 10 Jun 2017 15:34
Operator : SJ/MA
Sample : PB99638BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK38

Quant Time: Jun 12 04:17:35 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 04:15:09 2017
Response via : Initial Calibration

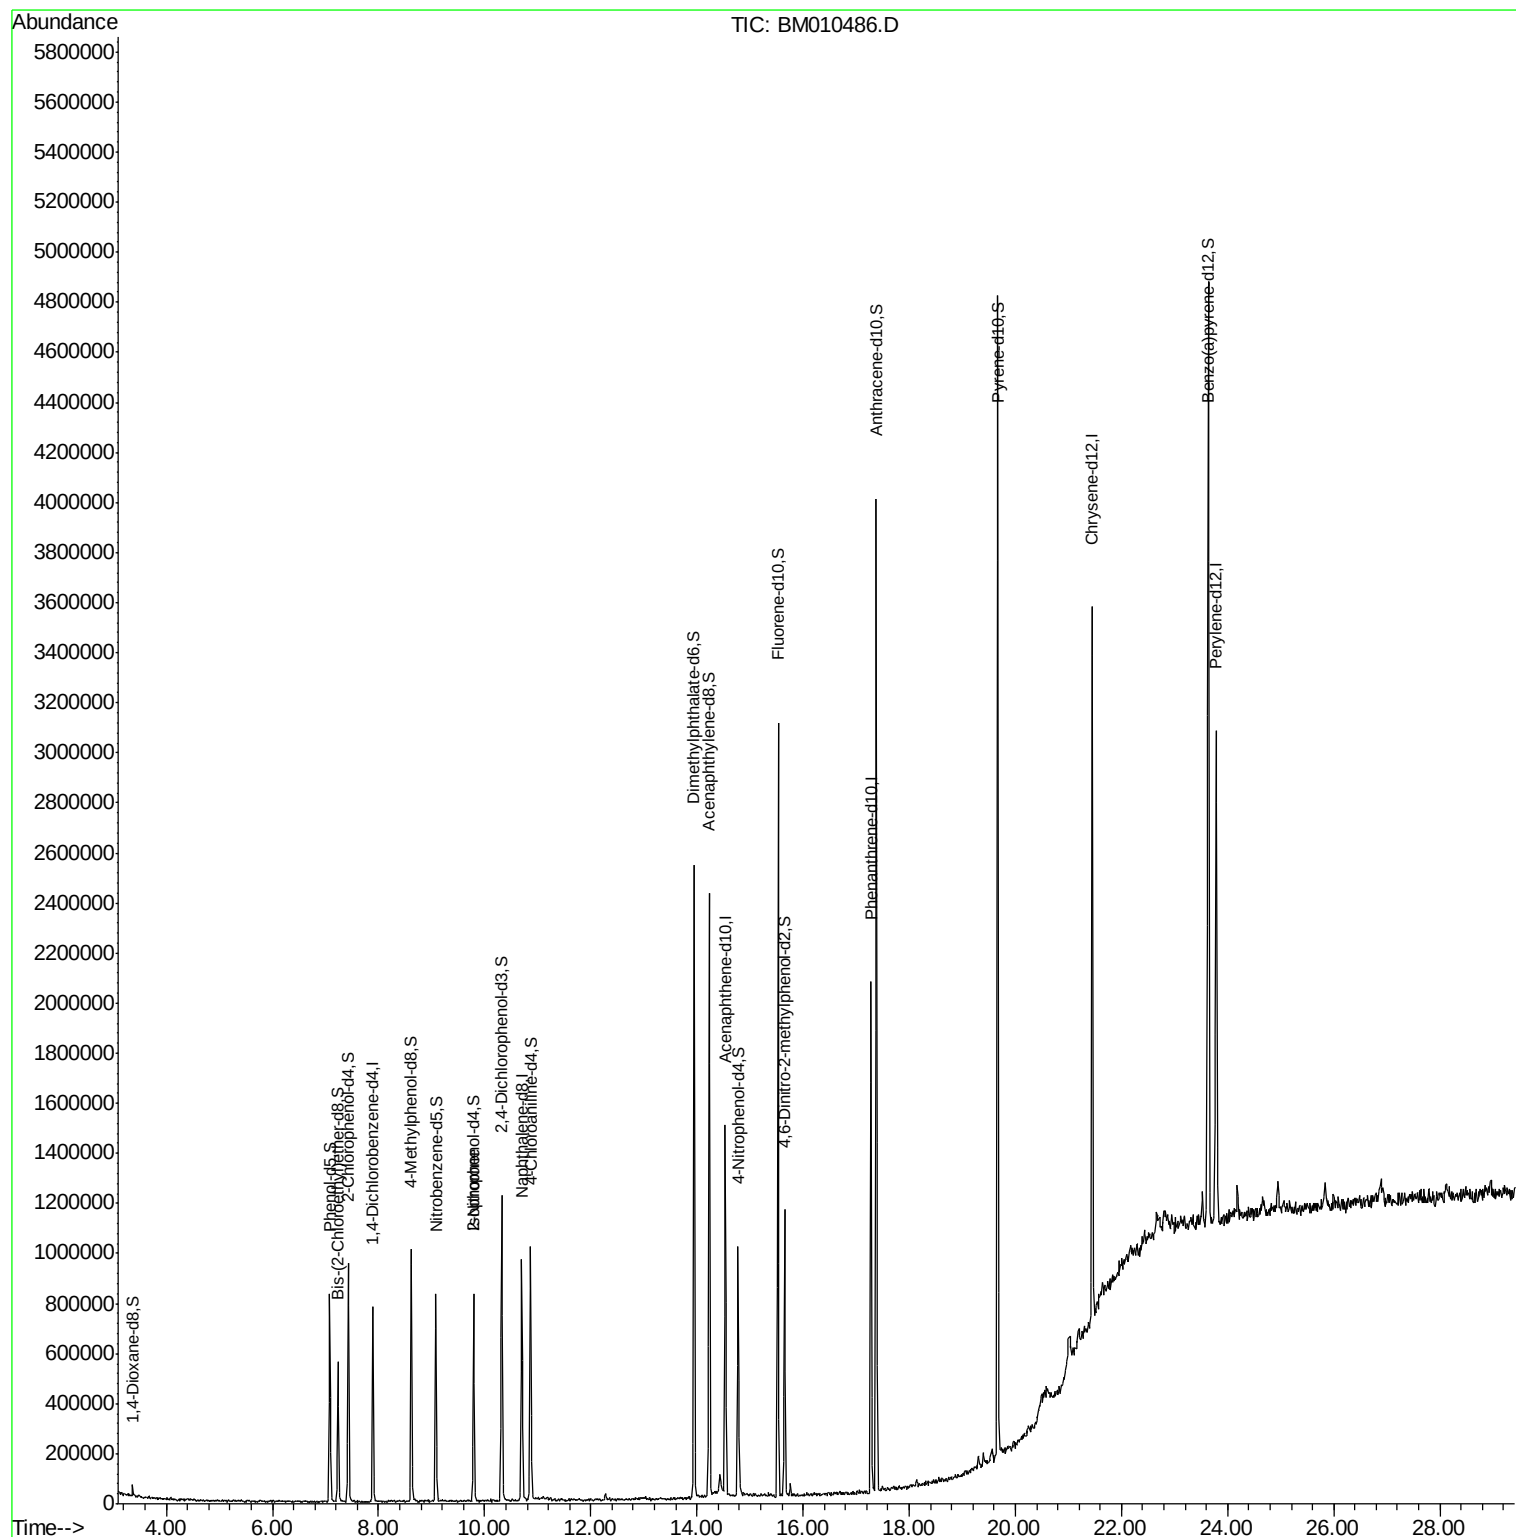

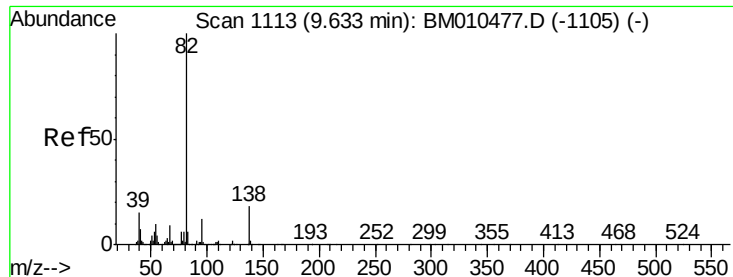

#21

Isophorone

Concen: 1.609 ng/ul

RT: 9.80 min Scan# 1141

Delta R.T. 0.16 min

Lab File: BM010486.D

Acq: 10 Jun 2017 15:34

Instrument :

BNA_M

ClientSampleId :

SBLK38

Tgt Ion: 82 Resp: 33037

Ion Ratio Lower Upper

82 100

95 6.9 7.8 11.8#

138 0.0 11.9 17.9#

