

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
 Data File : BM010487.D
 Acq On : 10 Jun 2017 16:10
 Operator : SJ/MA
 Sample : PB99646BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK46

Quant Time: Jun 12 04:17:45 2017
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 12 04:15:09 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	178537	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	666327	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.53	164	488695	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.28	188	1180510	20.00	ng/ul	0.00
75) Chrysene-d12	21.44	240	1322528	20.00	ng/ul	0.00
83) Perylene-d12	23.79	264	1315059	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.36	96	23137	5.32	ng/uL	0.00
5) Phenol-d5	7.08	99	395203	29.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.23	67	224498	29.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.43	132	345318	32.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.62	113	346457	31.74	ng/ul	0.00
19) Nitrobenzene-d5	9.08	128	169759	34.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.79	143	212227	37.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.32	165	422388	36.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.86	131	472240	42.14	ng/ul	0.00
43) Dimethylphthalate-d6	13.95	166	1693885	41.72	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	1752807	37.00	ng/ul	0.00
51) 4-Nitrophenol-d4	14.77	143	210952	34.73	ng/ul	0.00
57) Fluorene-d10	15.53	176	1378013	38.61	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.65	200	274669	32.85	ng/ul	0.00
70) Anthracene-d10	17.38	188	2338676	40.71	ng/ul	0.00
76) Pyrene-d10	19.67	212	2616879	47.85	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.63	264	2455235	40.10	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
21) Isophorone	9.79	82	36878	1.719	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010487.D
Acq On : 10 Jun 2017 16:10
Operator : SJ/MA
Sample : PB99646BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK46

Quant Time: Jun 12 04:17:45 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 04:15:09 2017
Response via : Initial Calibration

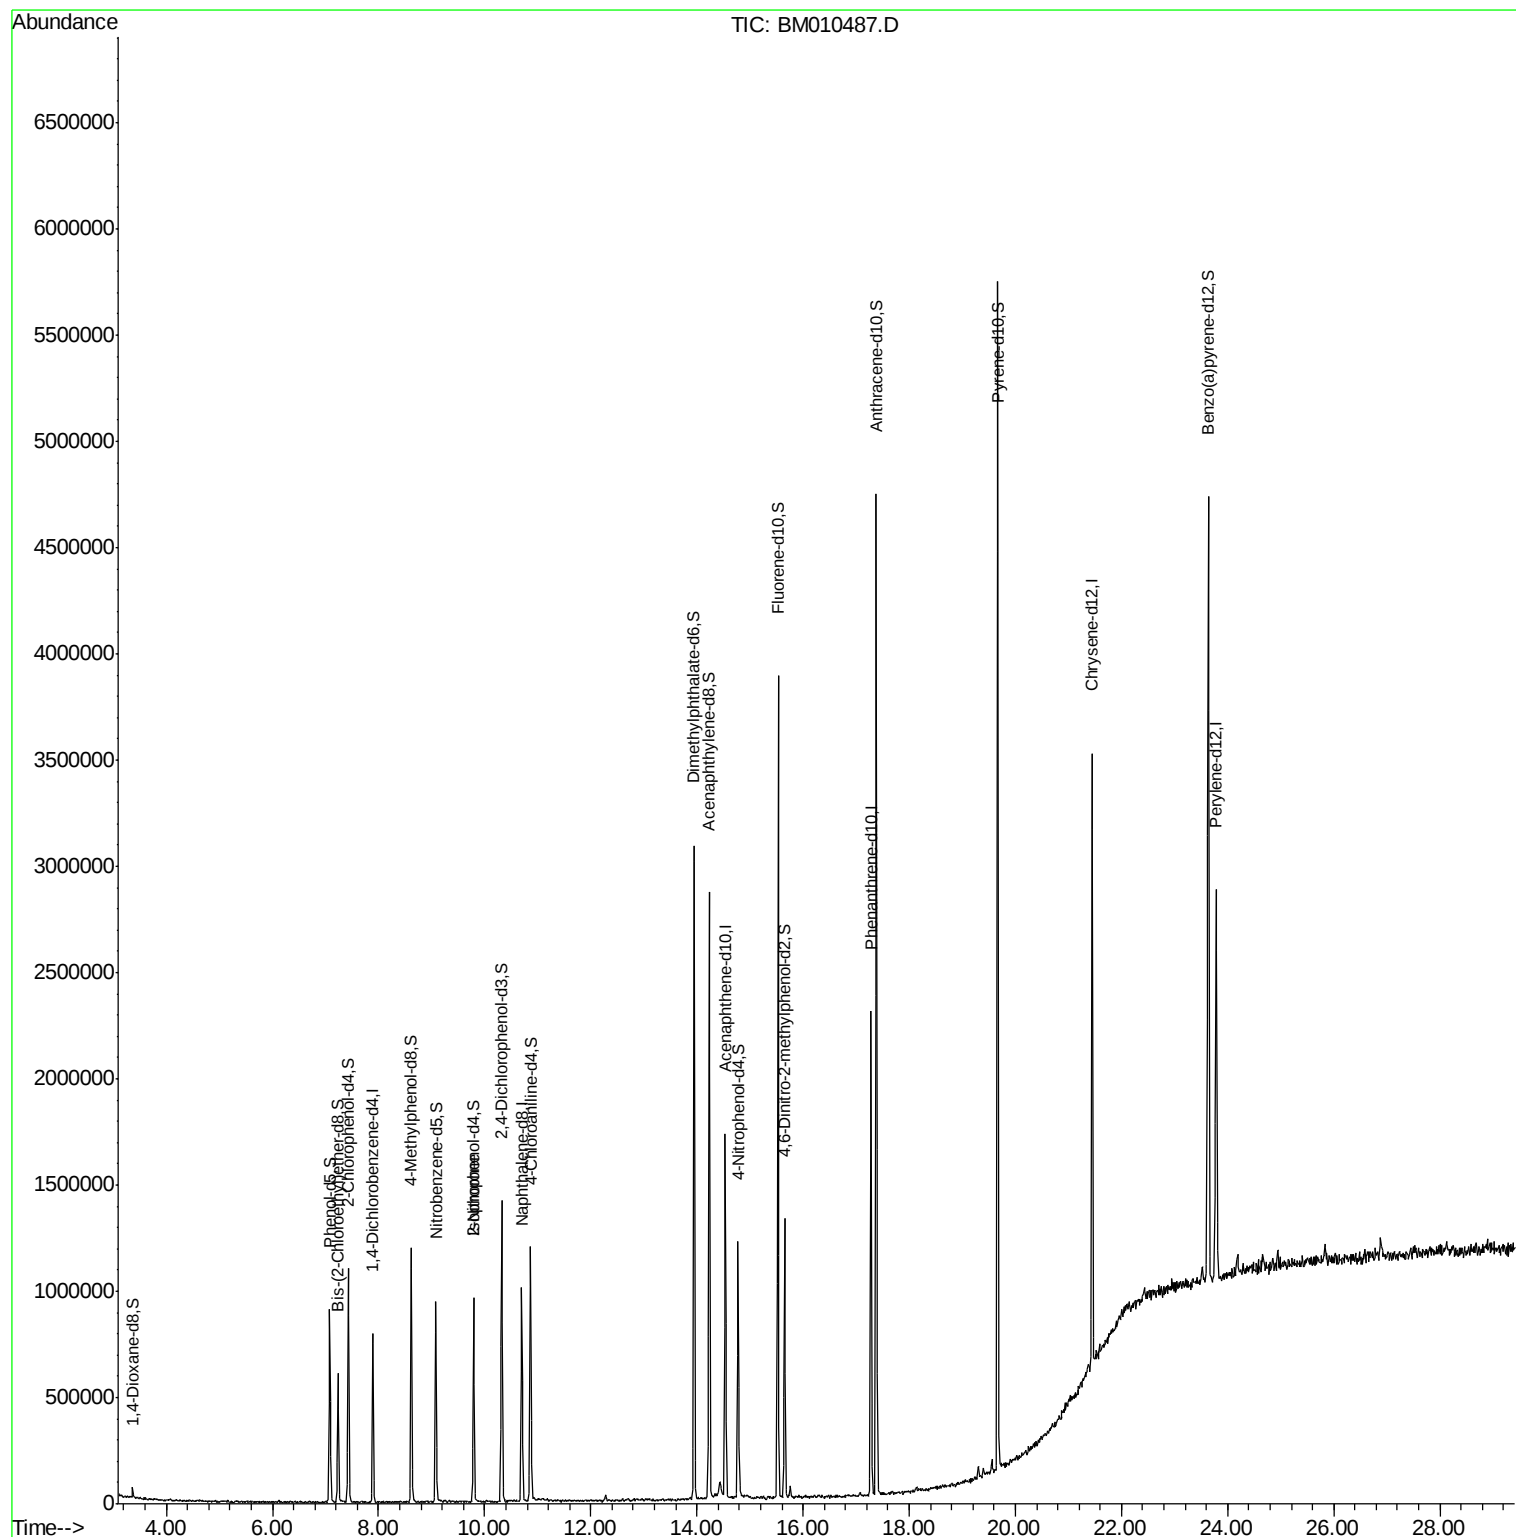

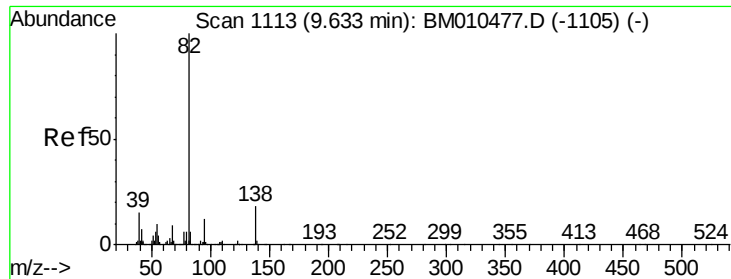

#21

Isophorone

Concen: 1.719 ng/ul

RT: 9.79 min Scan# 1140

Delta R.T. 0.16 min

Lab File: BM010487.D


Acq: 10 Jun 2017 16:10

Instrument :

BNA_M

ClientSampleId :

SBLK46

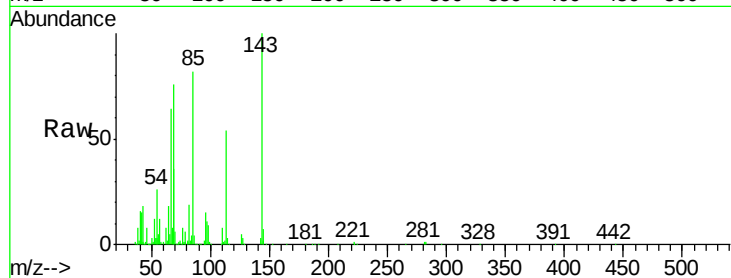

Tgt Ion:	82	Resp:	36878
Ion	Ratio	Lower	Upper
82	100		
95	7.9	7.8	11.8
138	0.0	11.9	17.9#

