

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
 Data File : BM010502.D
 Acq On : 11 Jun 2017 01:10
 Operator : SJ/MA
 Sample : I3558-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5A60

Quant Time: Jun 12 07:11:11 2017
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 12 07:08:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	152571	20.00	ng/ul	0.00
18) Naphthalene-d8	10.69	136	560829	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.53	164	383128	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.27	188	1038238	20.00	ng/ul	0.00
75) Chrysene-d12	21.44	240	1549388	20.00	ng/ul	0.00
83) Perylene-d12	23.78	264	1599112	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.36	96	13909	3.74	ng/uL	0.00
5) Phenol-d5	7.08	99	247729	21.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.23	67	138601	21.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.43	132	213758	23.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.62	113	207637	22.26	ng/ul	0.00
19) Nitrobenzene-d5	9.07	128	97695	23.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.79	143	120573	25.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.32	165	252931	25.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.86	131	246271	26.11	ng/ul	0.00
43) Dimethylphthalate-d6	13.95	166	868437	27.28	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	935804	25.20	ng/ul	0.00
51) 4-Nitrophenol-d4	14.77	143	114948	24.14	ng/ul	0.00
57) Fluorene-d10	15.52	176	764209	27.31	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.65	200	163527	22.24	ng/ul	0.00
70) Anthracene-d10	17.37	188	1304818	25.83	ng/ul	0.00
76) Pyrene-d10	19.66	212	1728511	26.98	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.63	264	1921096	25.80	ng/ul	0.00
Target Compounds						
6) Phenol	7.10	94	22479	1.896	ng/ul	96
44) Dimethylphthalate	13.99	163	263669	8.422	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010502.D
Acq On : 11 Jun 2017 01:10
Operator : SJ/MA
Sample : I3558-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5A60

Quant Time: Jun 12 07:11:11 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 07:08:51 2017
Response via : Initial Calibration

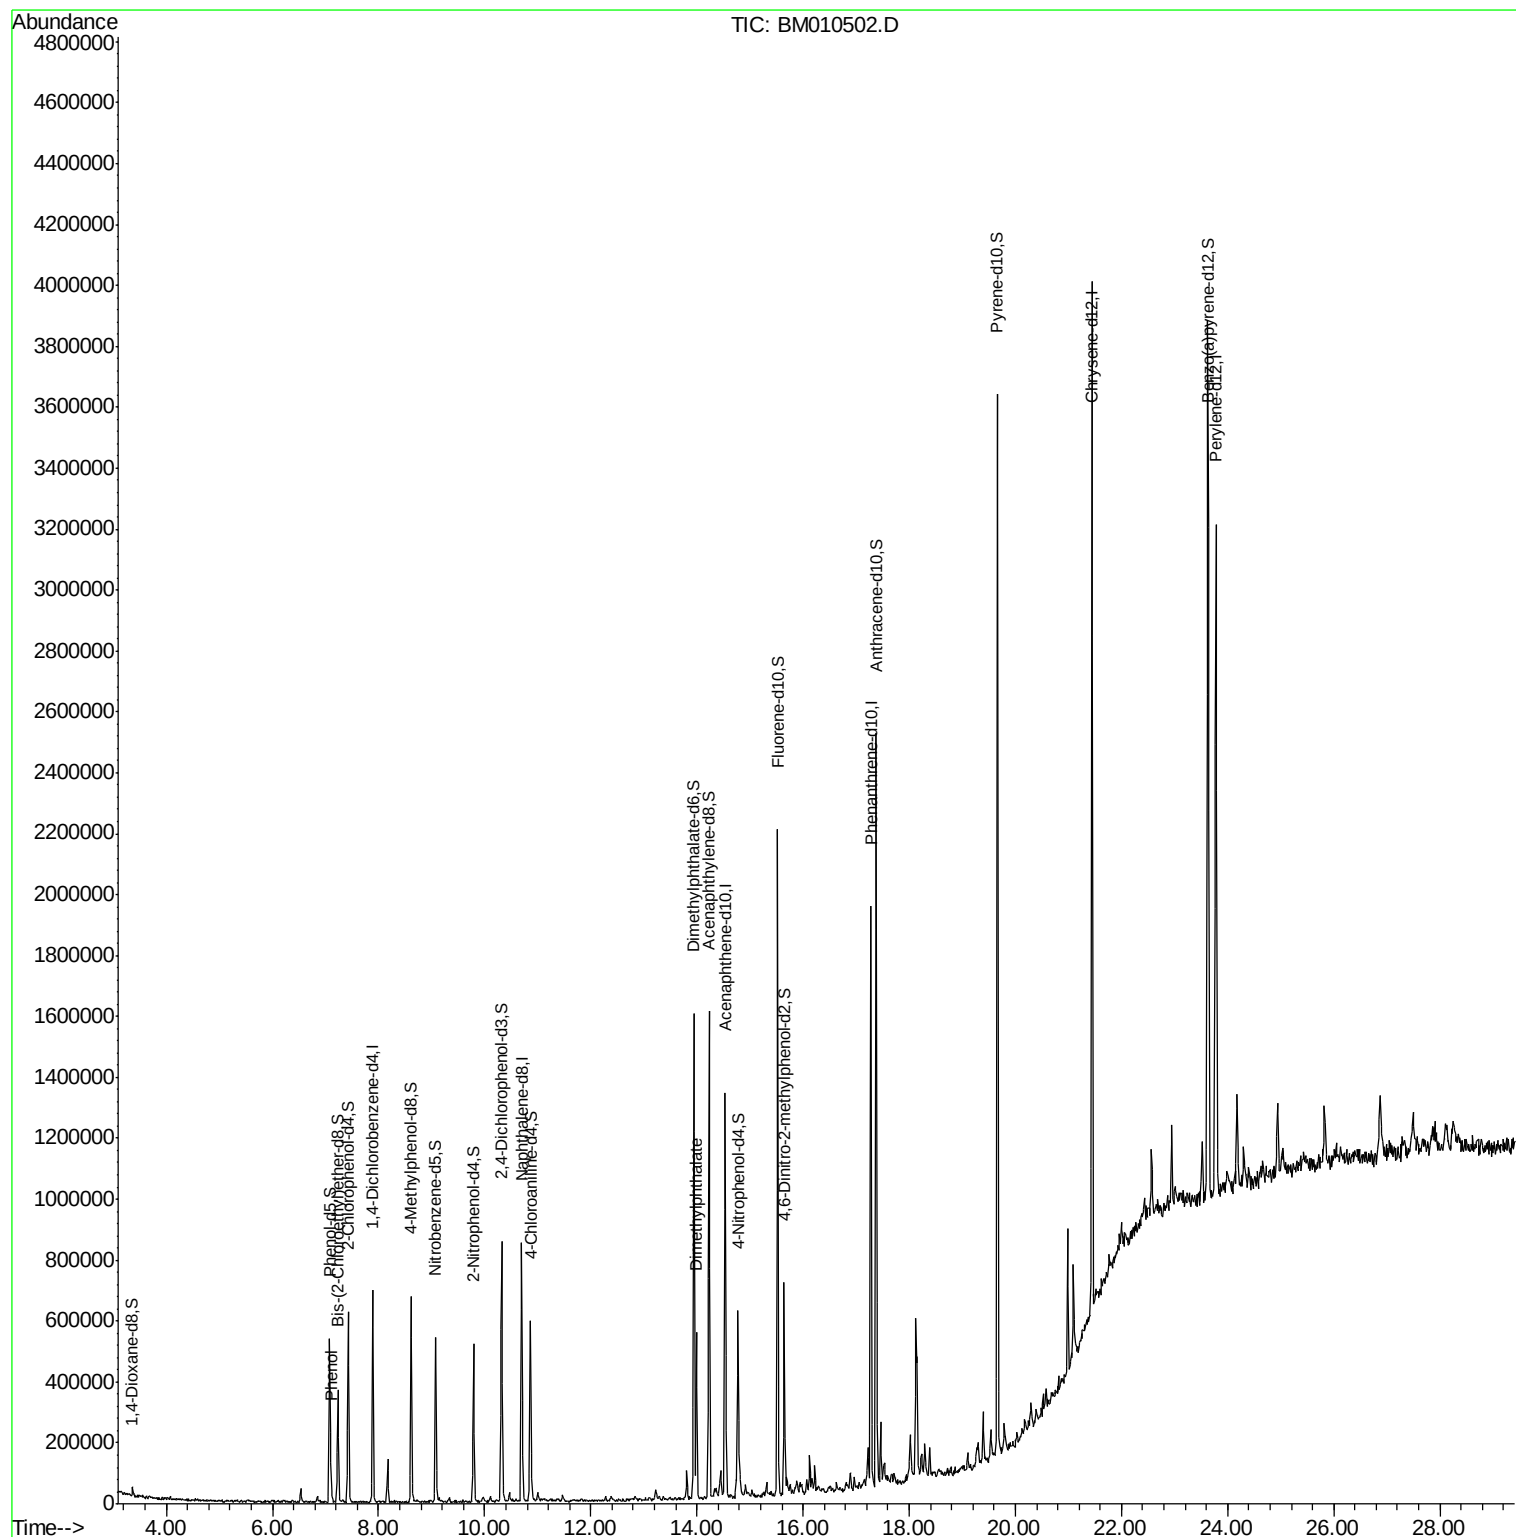

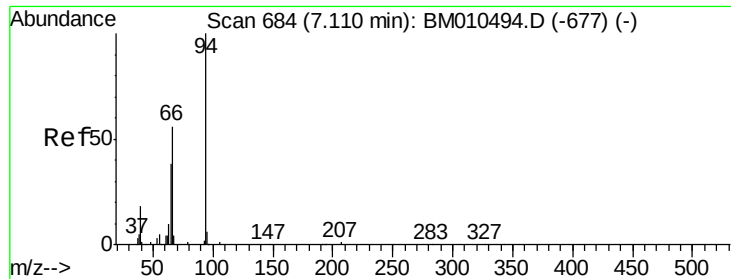

#6

Phenol

Concen: 1.896 ng/ul

RT: 7.10 min Scan# 683

Delta R.T. -0.01 min

Lab File: BM010502.D

Acq: 11 Jun 2017 01:10

Instrument :

BNA_M

ClientSampleId :

F5A60


Tgt Ion: 94 Resp: 22479

Ion Ratio Lower Upper

94 100

65 37.5 28.2 42.4




66 61.9 47.2 70.8

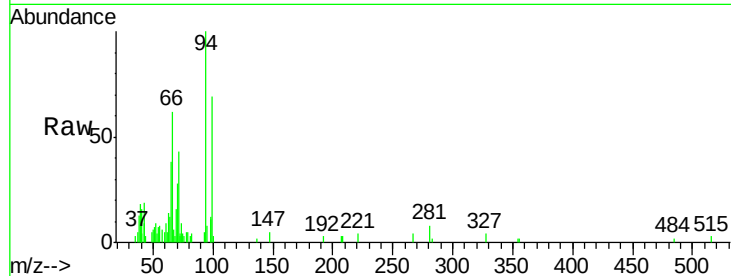

Abundance Ion 94.00 (93.70 to 94.70): BM010494.D (-677) (-)

Ion 65.00 (64.70 to 65.70): BM010494.D (-677) (-)

Ion 66.00 (65.70 to 66.70): BM010494.D (-677) (-)

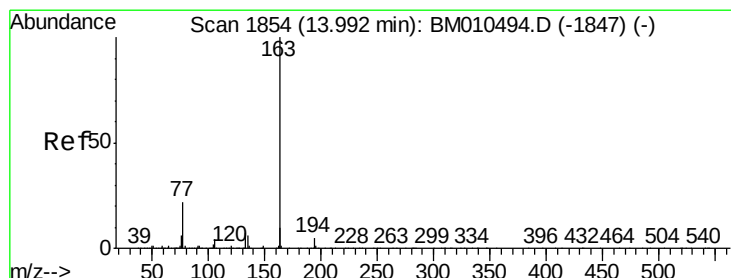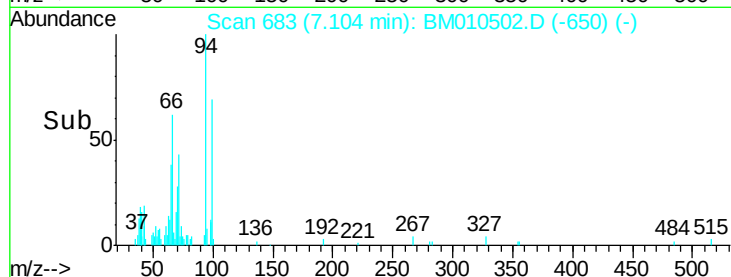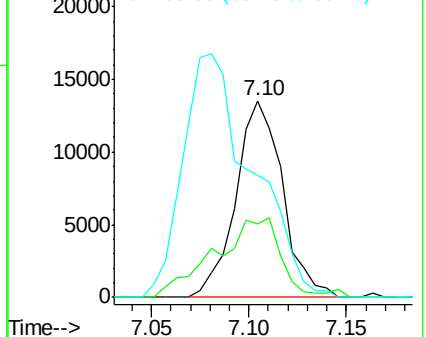

#44

Dimethylphthalate

Concen: 8.422 ng/ul

RT: 13.99 min Scan# 1854

Delta R.T. 0.00 min

Lab File: BM010502.D

Acq: 11 Jun 2017 01:10


Tgt Ion:163 Resp: 263669

Ion Ratio Lower Upper

163 100

194 5.4 3.5 5.3#

164 11.8 8.2 12.4

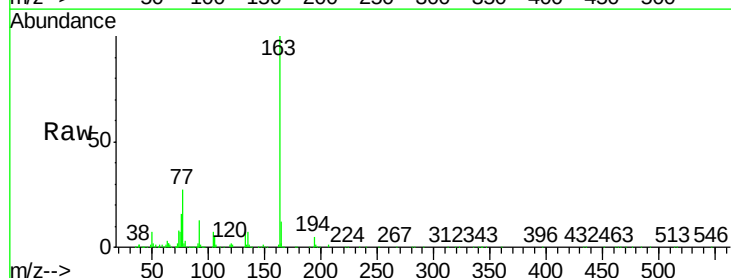

Abundance Ion 163.00 (162.70 to 163.70): BM010494.D (-1847) (-)

Ion 194.00 (193.70 to 194.70): BM010494.D (-1847) (-)

Ion 164.00 (163.70 to 164.70): BM010494.D (-1847) (-)

