


Data Path : Z:\HPCHEM1\BNA_M\Data\BM061017\
 Data File : BM010476.D
 Acq On : 10 Jun 2017 09:34
 Operator : SJ/MA
 Sample : DFTPP11
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP11

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION
 Last Update : Thu Jun 08 01:22:27 2017

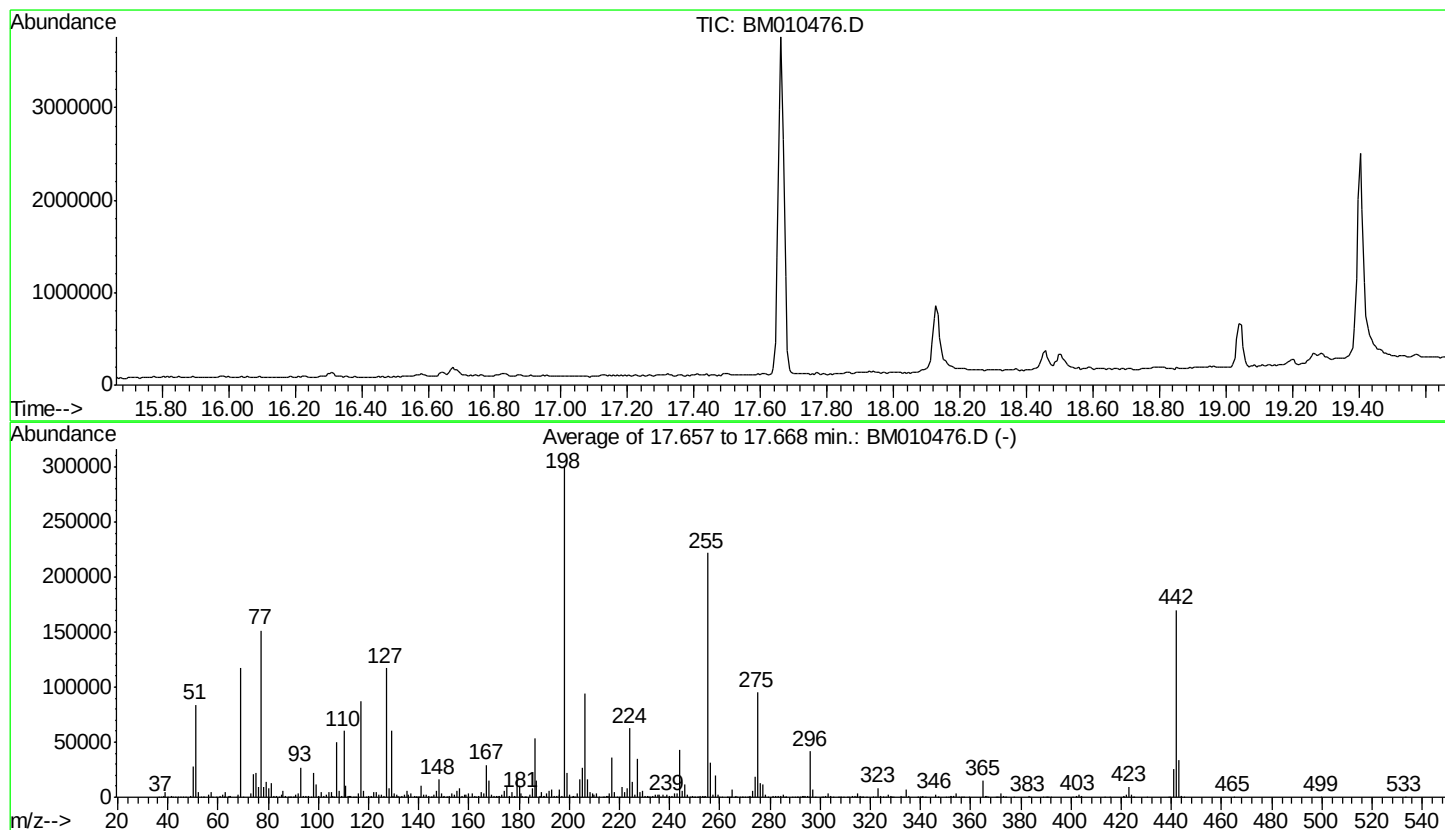

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	84054	PASS
68	69	0.00	2	1.9	2212	PASS
69	198	0.00	100	39.0	117442	PASS
70	69	0.00	2	0.3	300	PASS
127	198	10	80	38.8	116909	PASS
197	198	0.00	2	0.5	1649	PASS
198	198	100	100	100.0	301226	PASS
199	198	5	9	7.2	21576	PASS
275	198	10	60	31.5	94944	PASS
365	198	1	100	5.0	14923	PASS
441	443	0.01	100	76.3	25781	PASS
442	198	50	100	56.5	170309	PASS
443	442	15	24	19.9	33810	PASS