


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:49:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

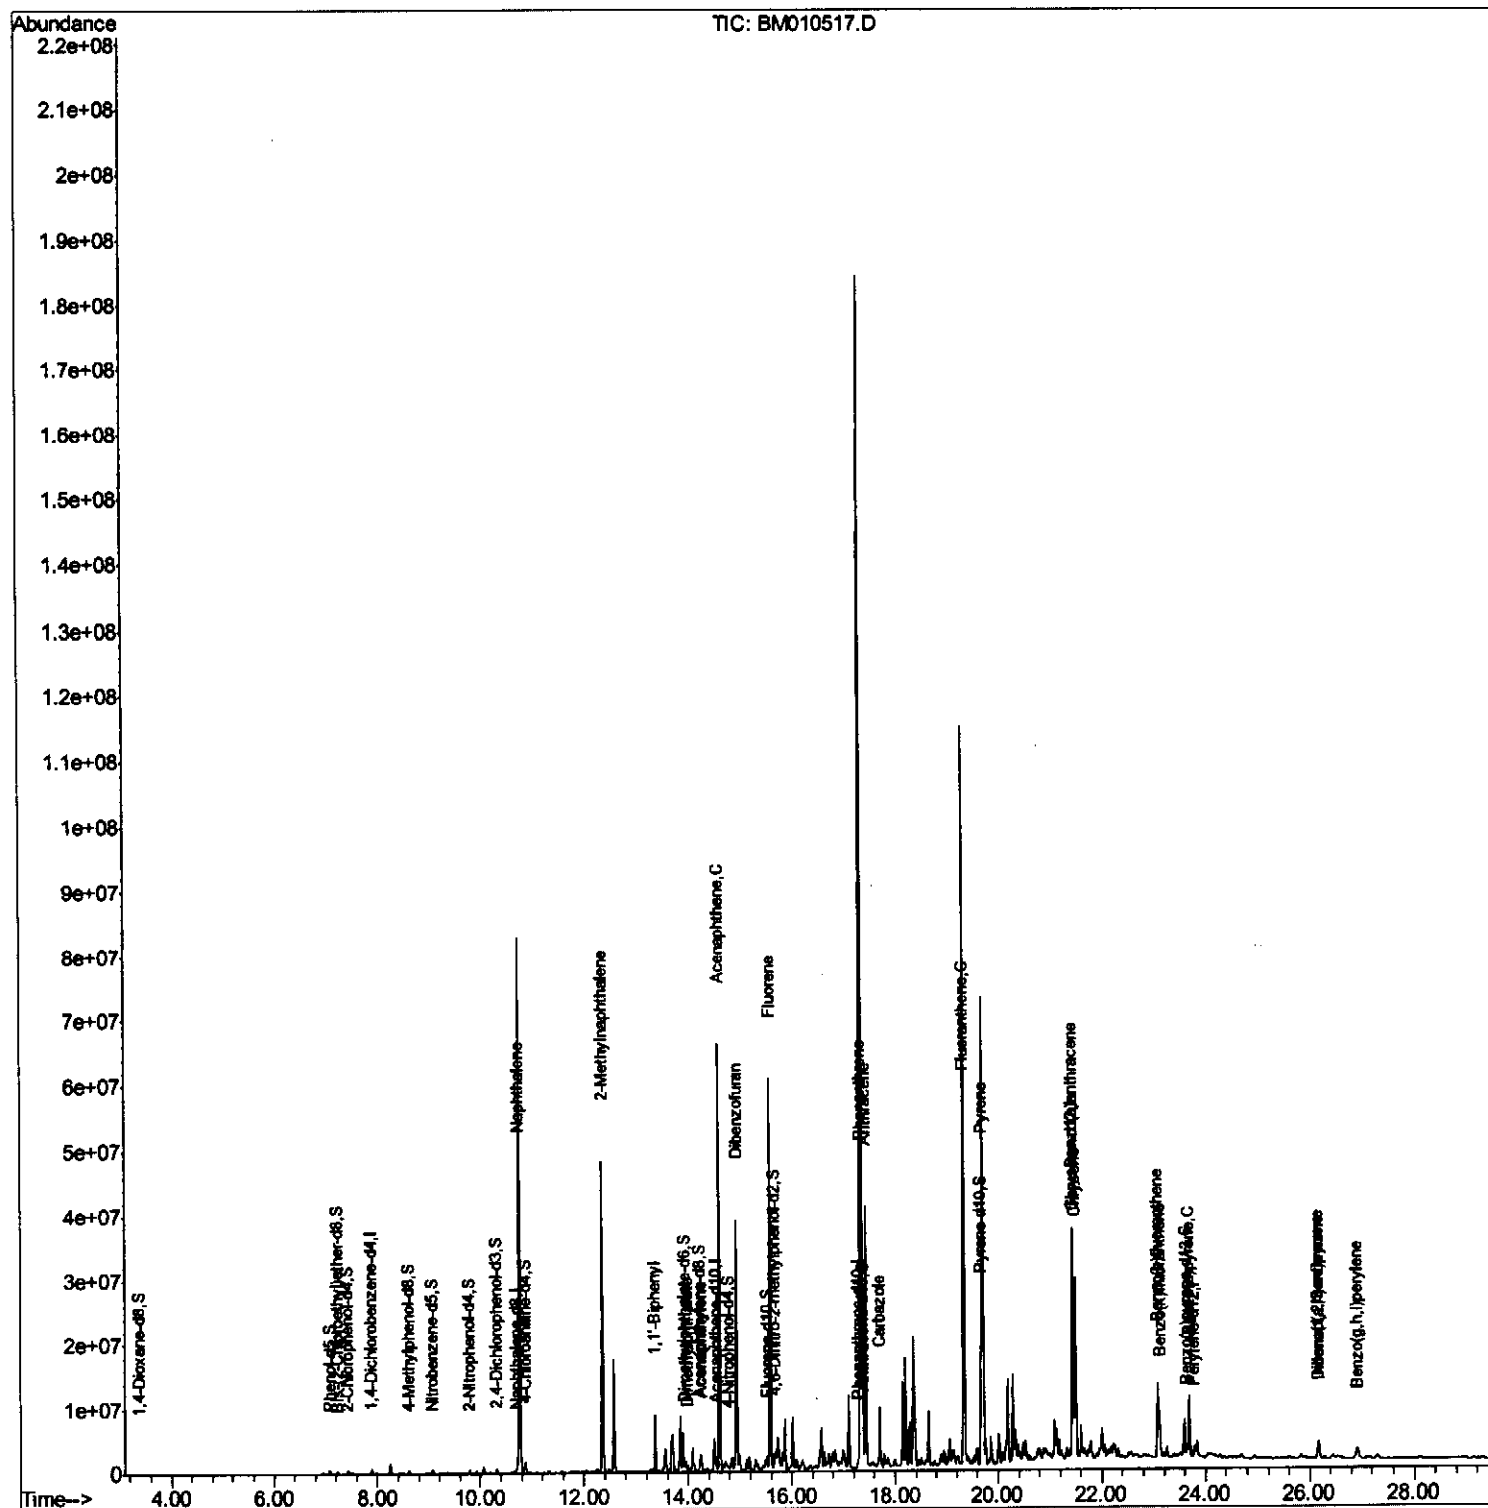




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:08:39 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

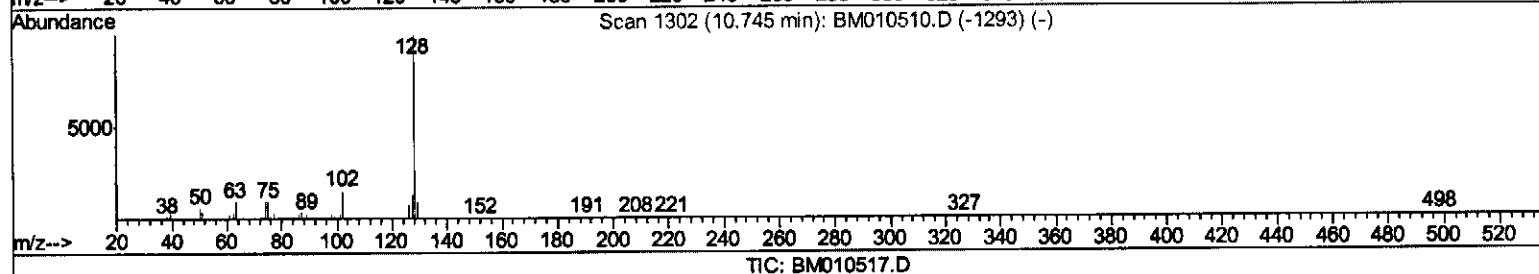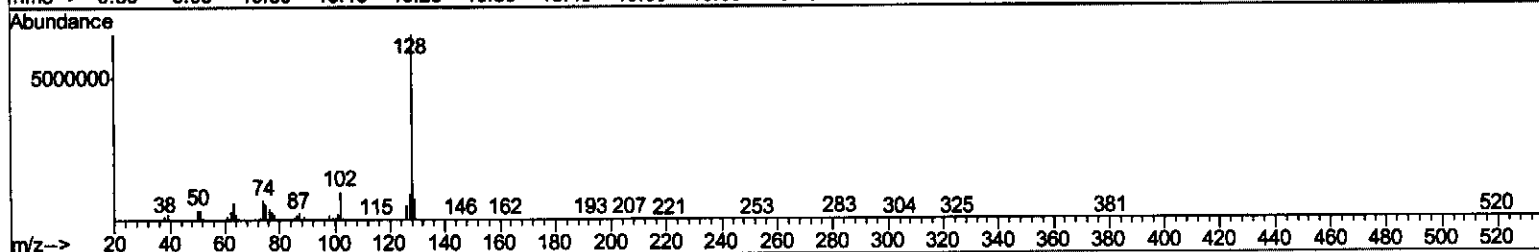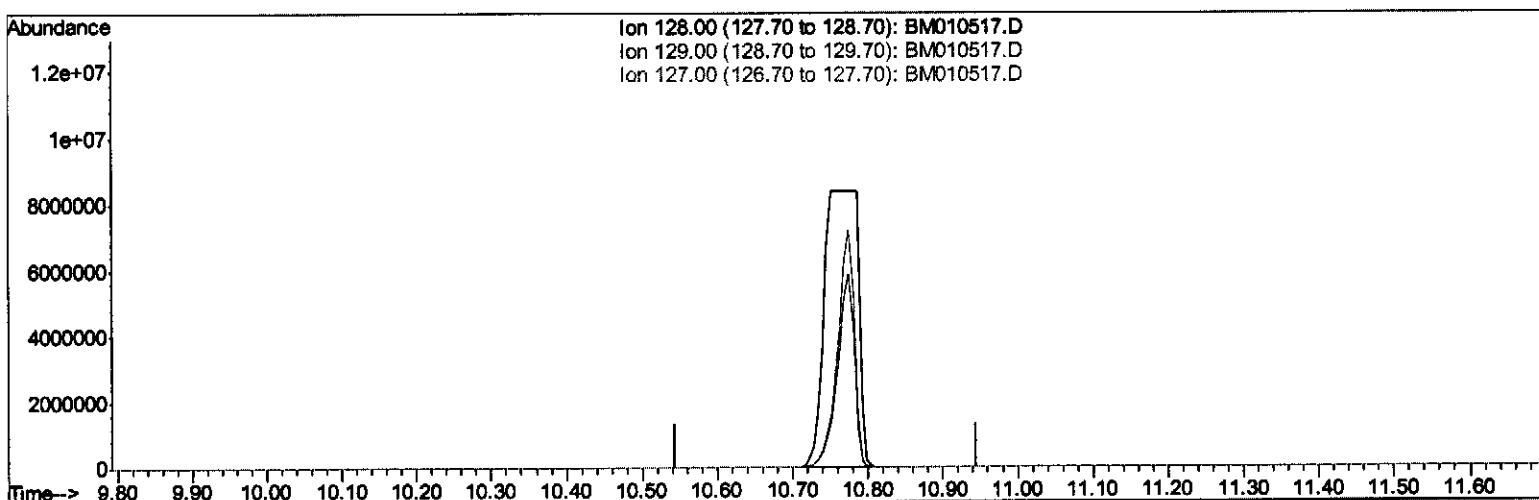

(28) Naphthalene

10.745min (-10.745) 0.00ng/ul

response 0

Ion	Exp%	Act%
128.00	100	0.00
129.00	11.00	0.00#
127.00	13.30	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:08:39 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

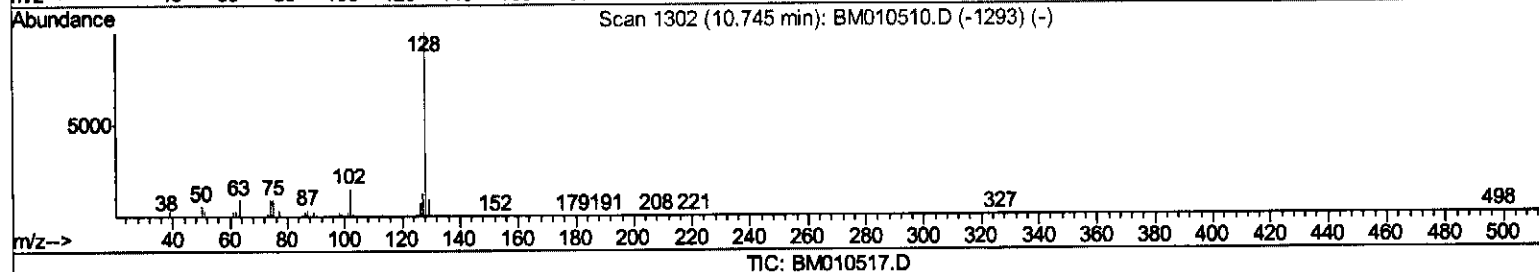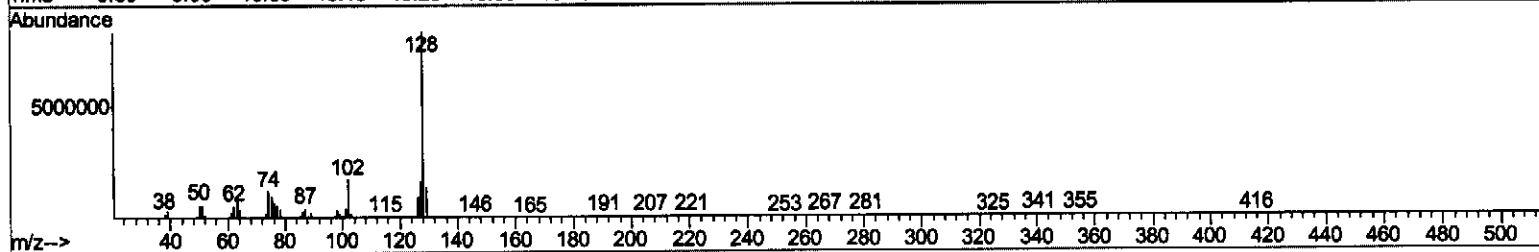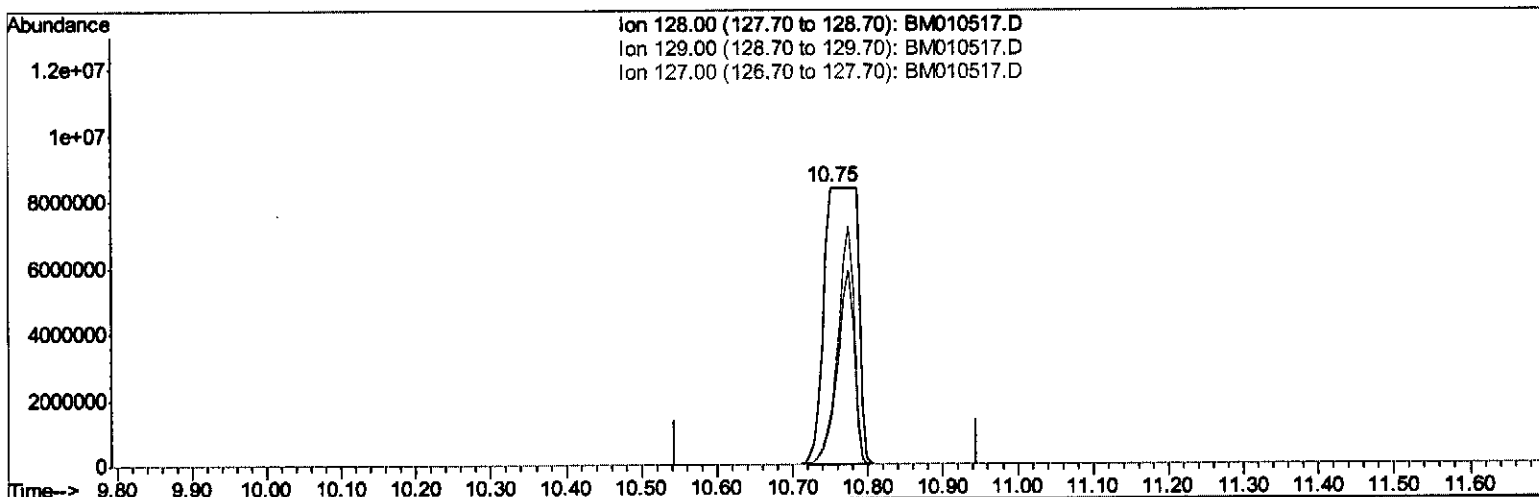

(28) Naphthalene

10.751min (+0.006) 838.88ng/ul m

response 25939201

Ion	Exp%	Act%
128.00	100	100
129.00	11.00	16.61#
127.00	13.30	19.46#
0.00	0.00	0.00

SJ
06/19/17




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:08:39 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

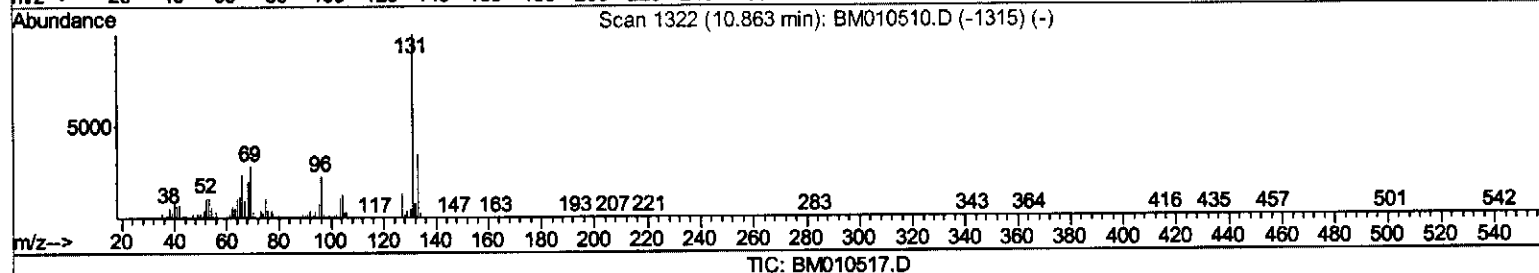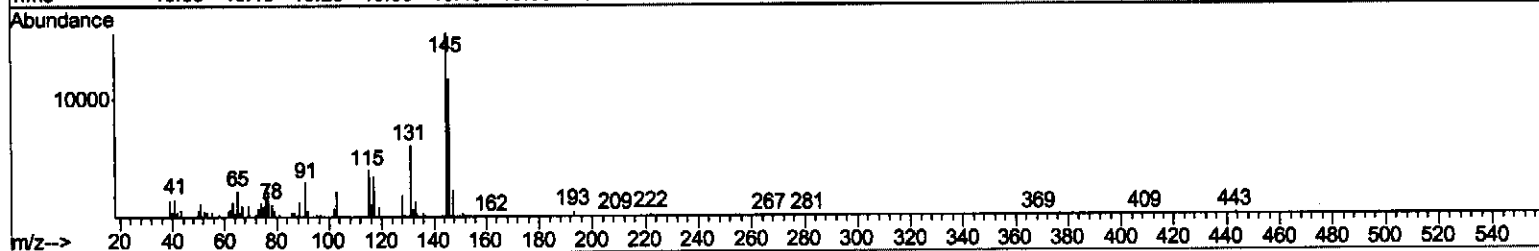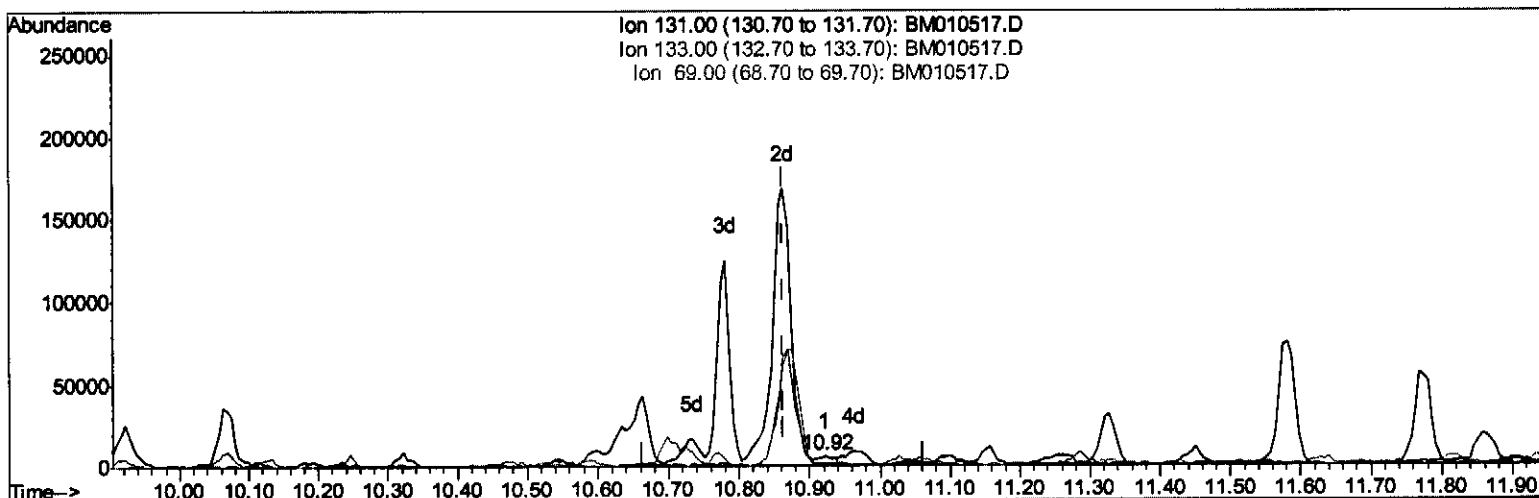

(29) 4-Chloroaniline-d4 (S)

10.922min (+0.059) 0.64ng/ui

response 6616

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	33.42
69.00	24.30	19.76
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:08:39 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

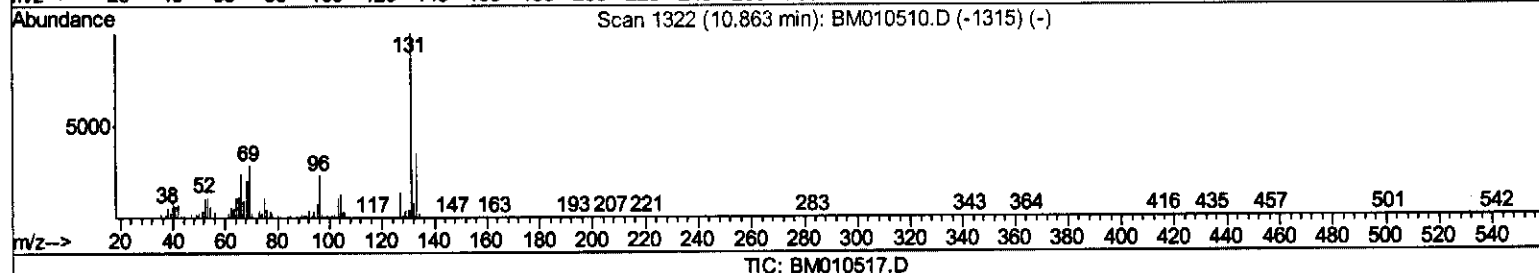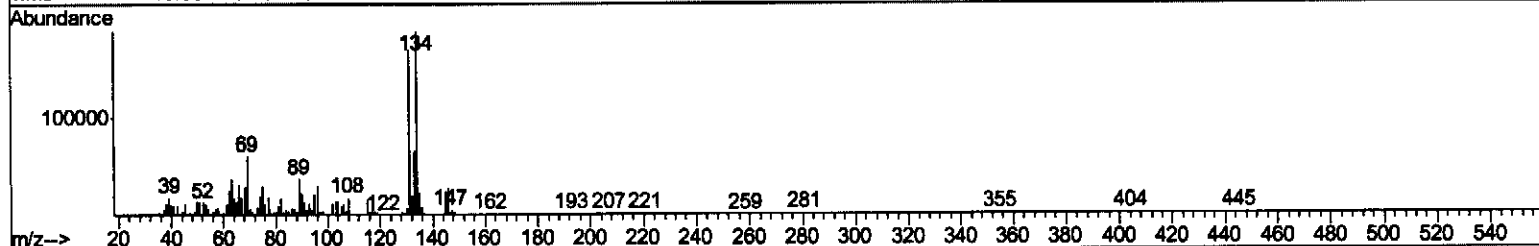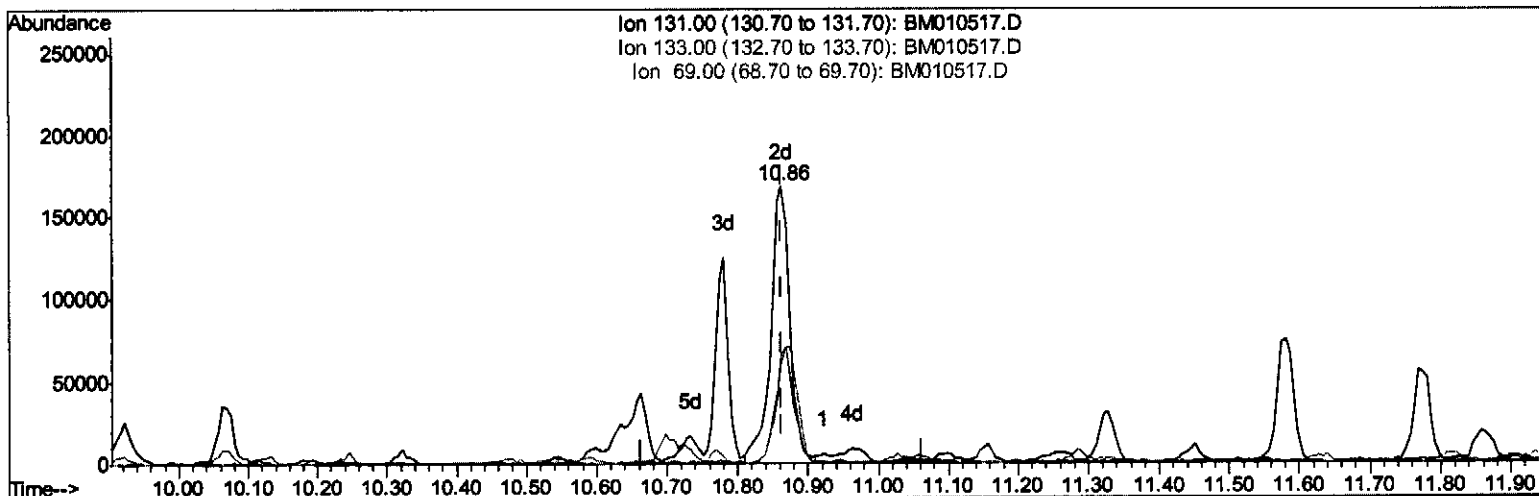

(29) 4-Chloroaniline-d4 (S)

10.863min (+0.000) 30.90ng/ul m

SS 06/19/17

response 320406

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	39.11#
69.00	24.30	36.10#
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

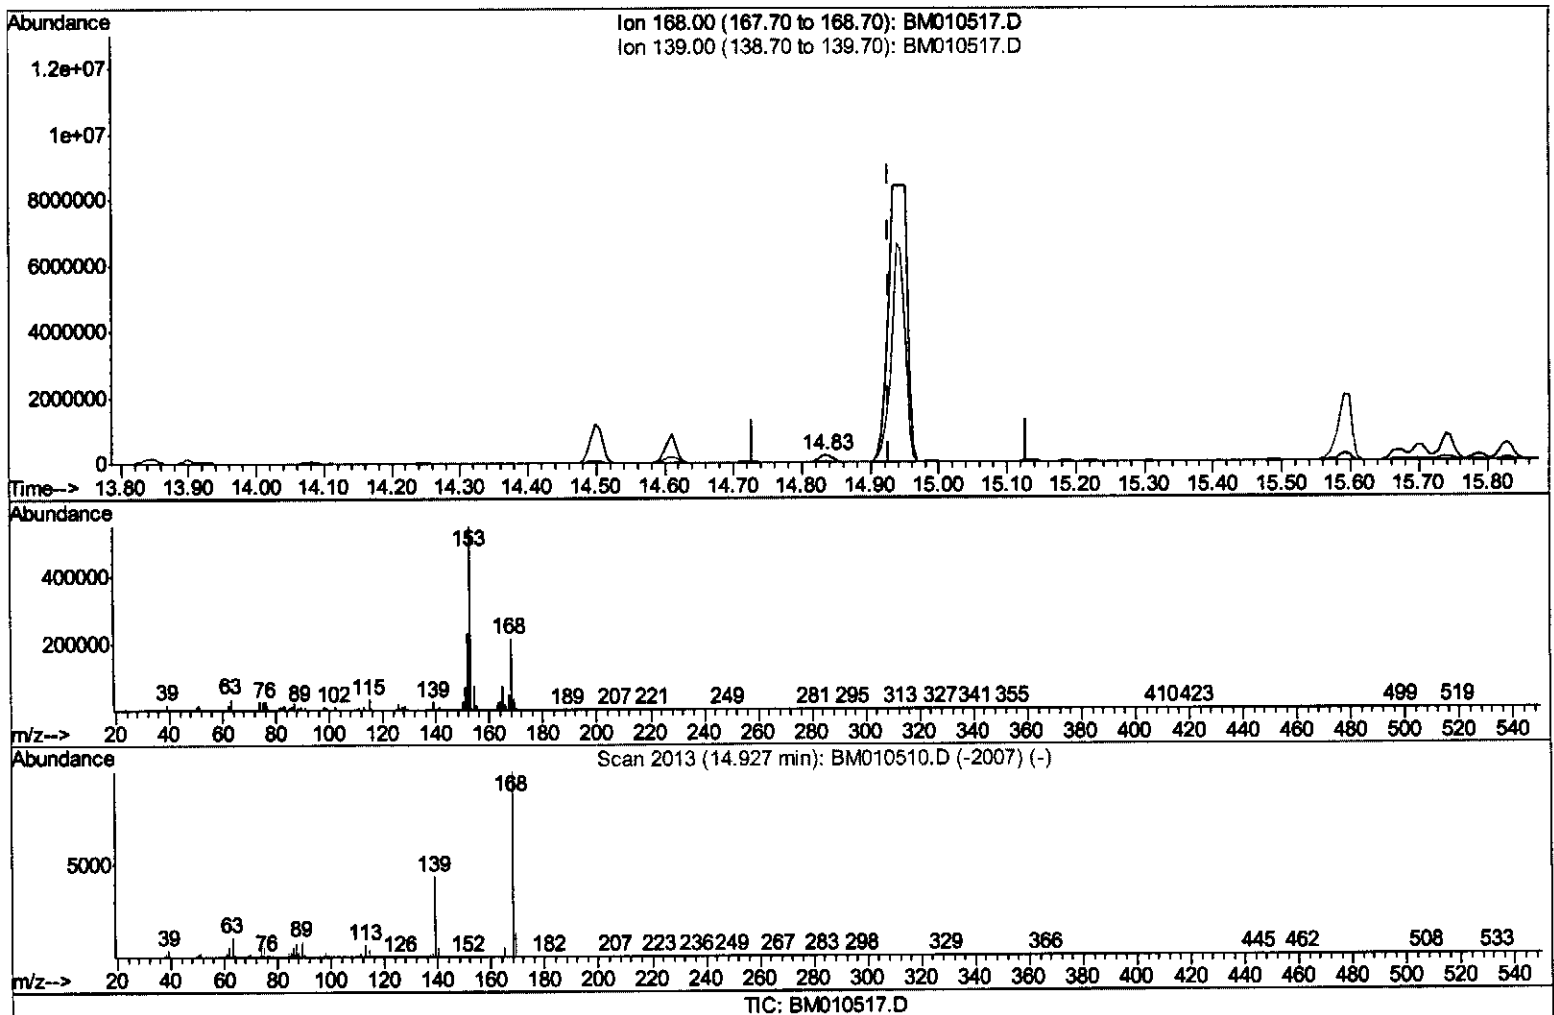

(53) Dibenzofuran

14.833min (-0.094) 7.37ng/ul

response 305656

Ion	Exp%	Act%
168.00	100	100
139.00	38.50	12.05#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

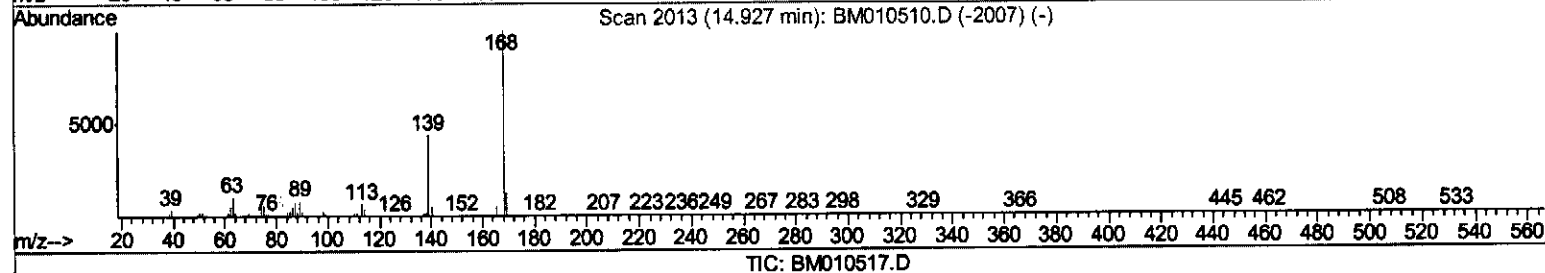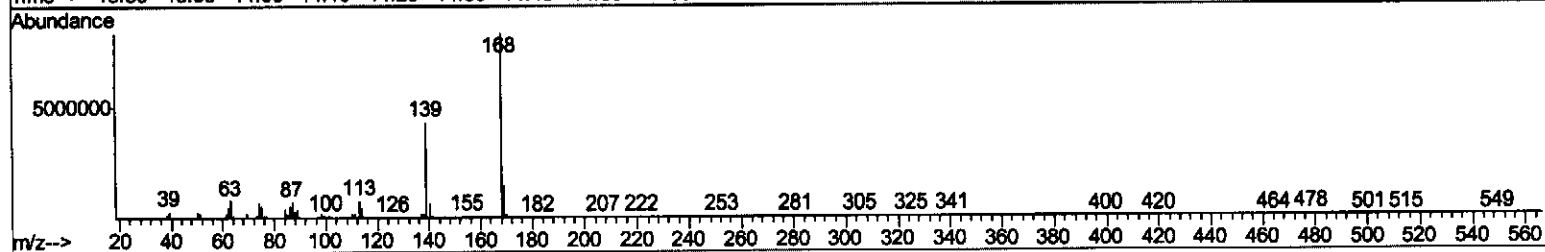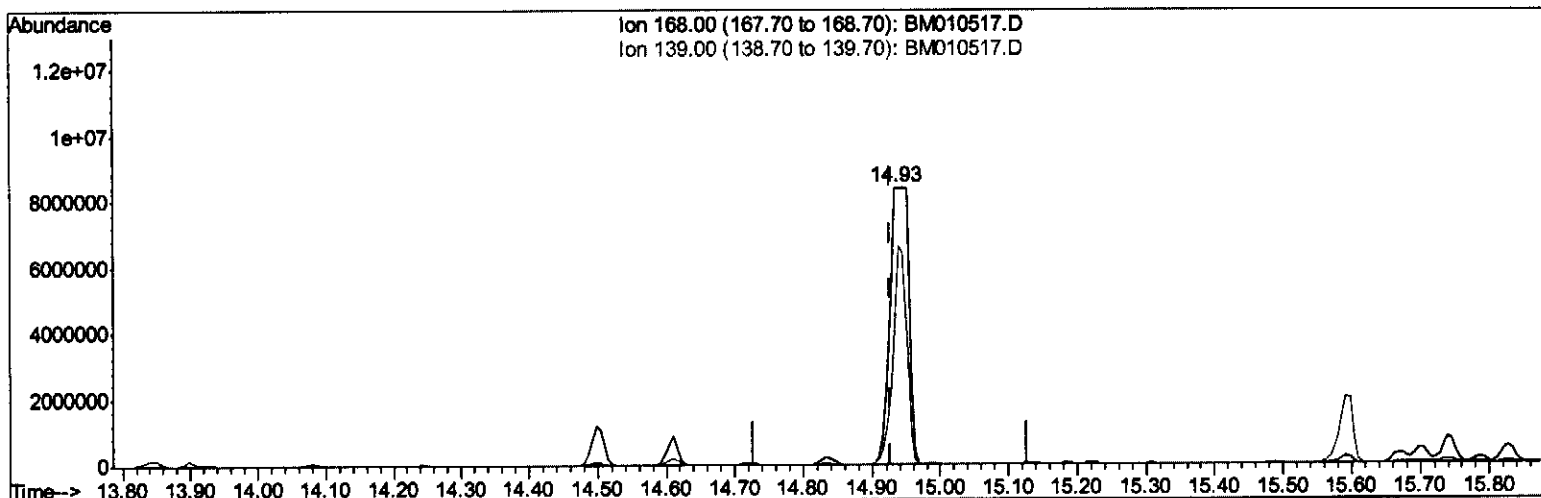

(53) Dibenzofuran

14.933min (+0.006) 384.47ng/ul m *JS 06/19/17*

response 15942700

Ion	Exp%	Act%
168.00	100	100
139.00	38.50	51.53#
0.00	0.00	0.00
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

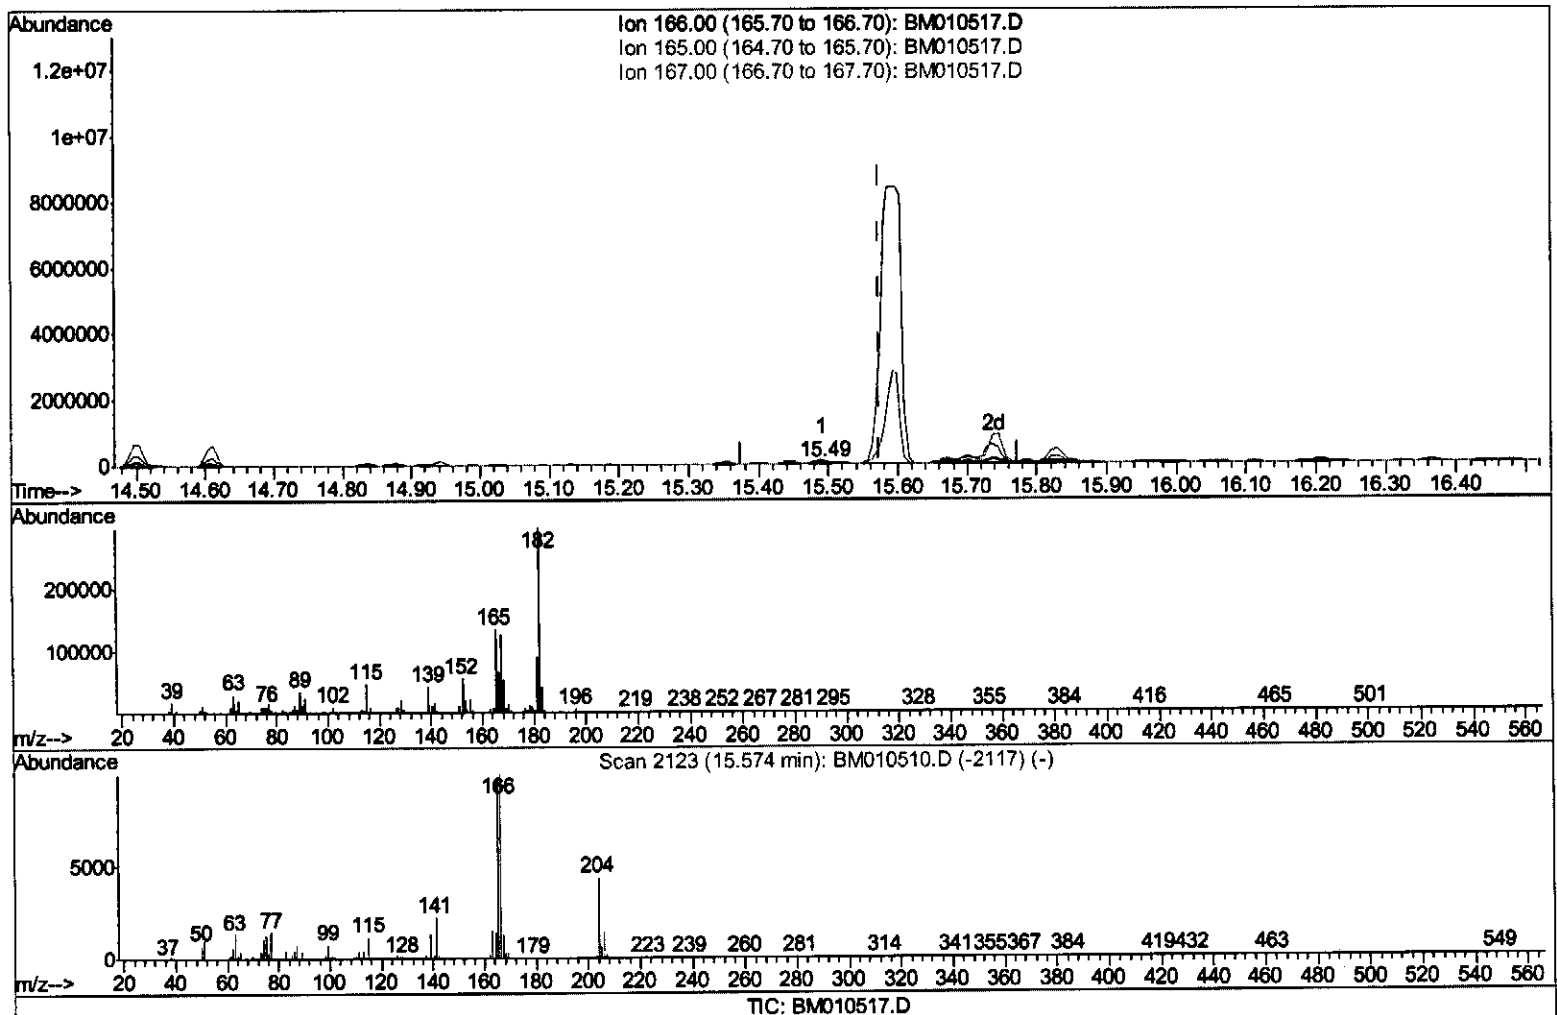

(58) Fluorene

15.492min (-0.082) 2.92ng/ul

response 99389

Ion	Exp%	Act%
166.00	100	100
165.00	97.40	203.54#
167.00	13.30	191.88#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

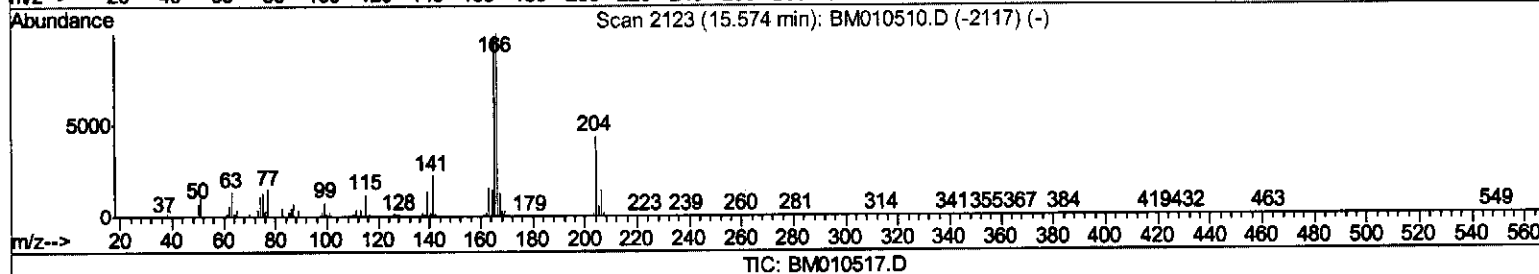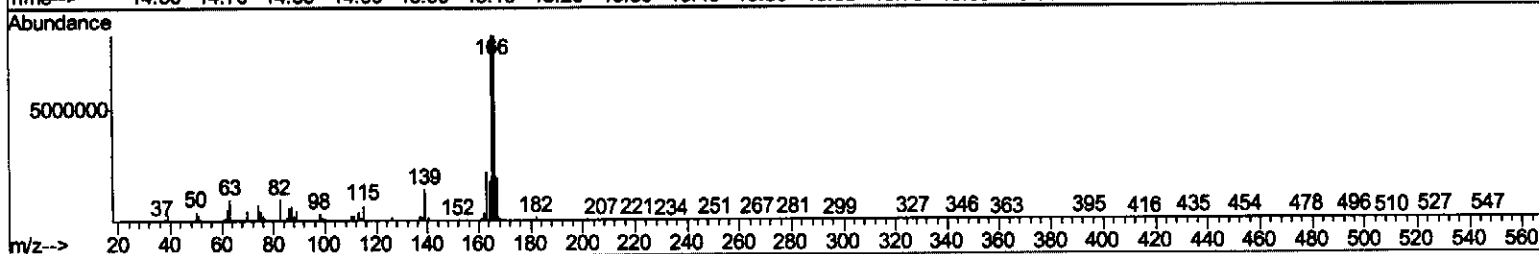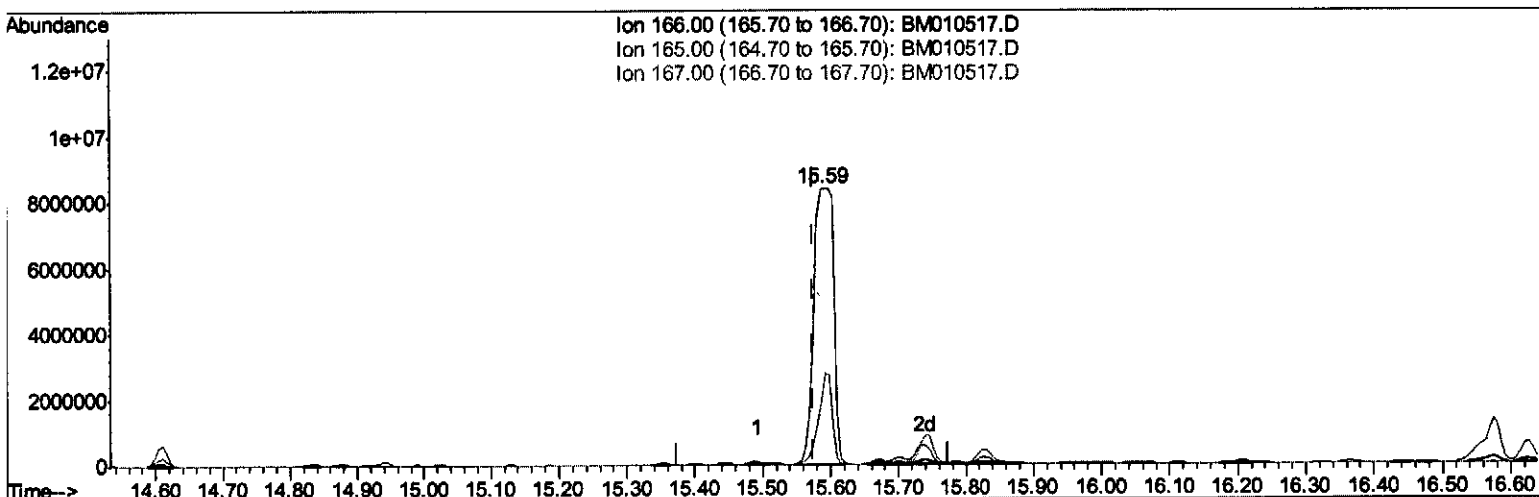

(58) Fluorene

15.586min (+0.012) 505.50ng/ul m *SJ 6/19/17*

response 17194006

Ion	Exp%	Act%
166.00	100	100
165.00	97.40	100.00
167.00	13.30	23.21#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

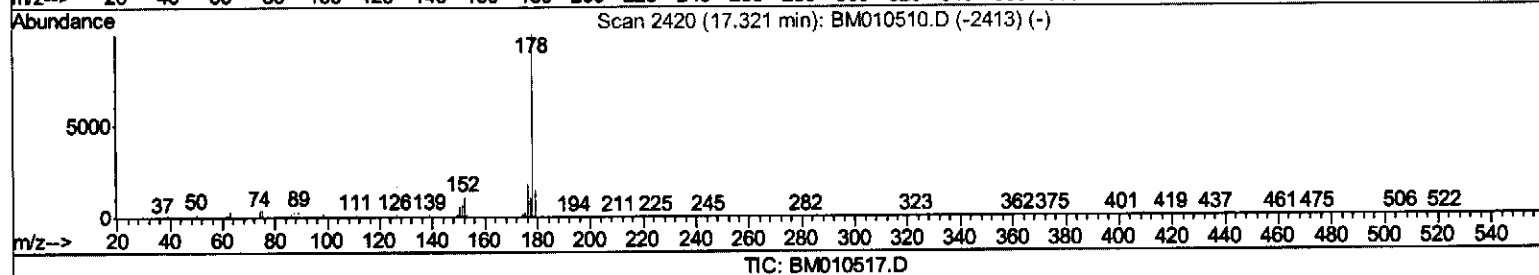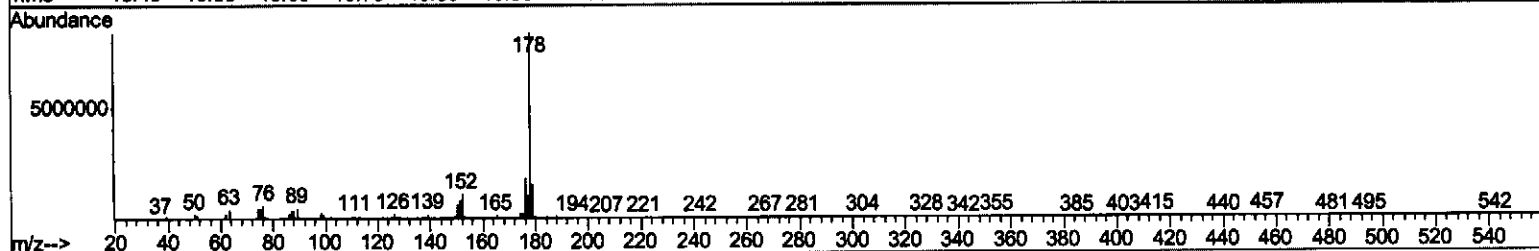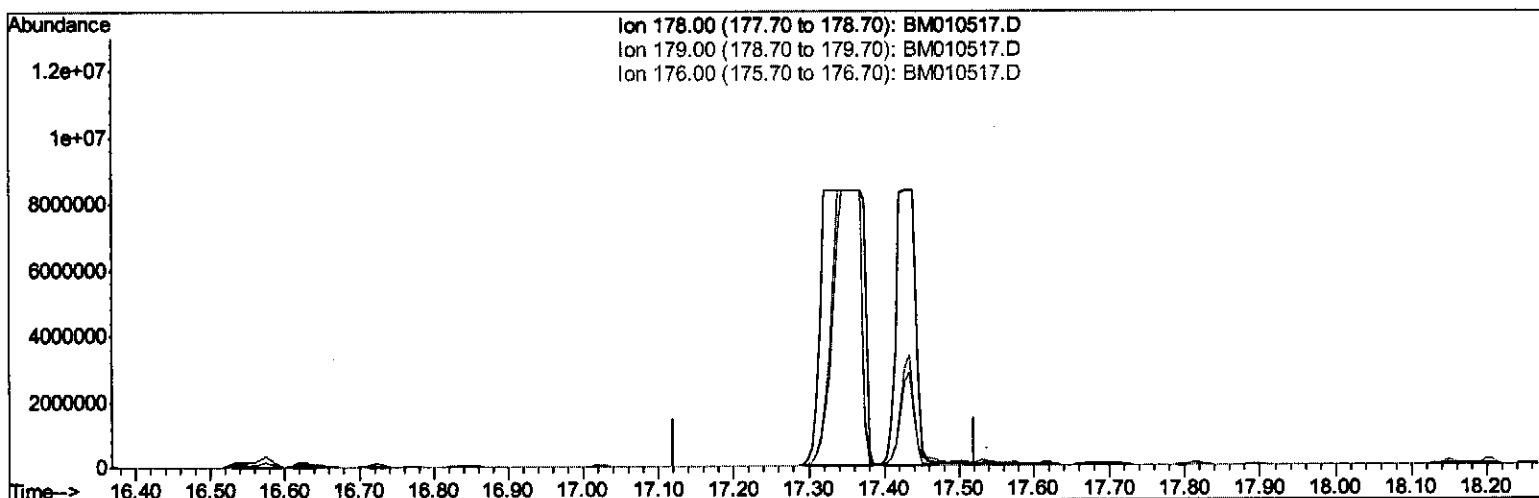

(69) Phenanthrene

17.321min (-17.321) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	15.80	0.00#
176.00	18.60	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

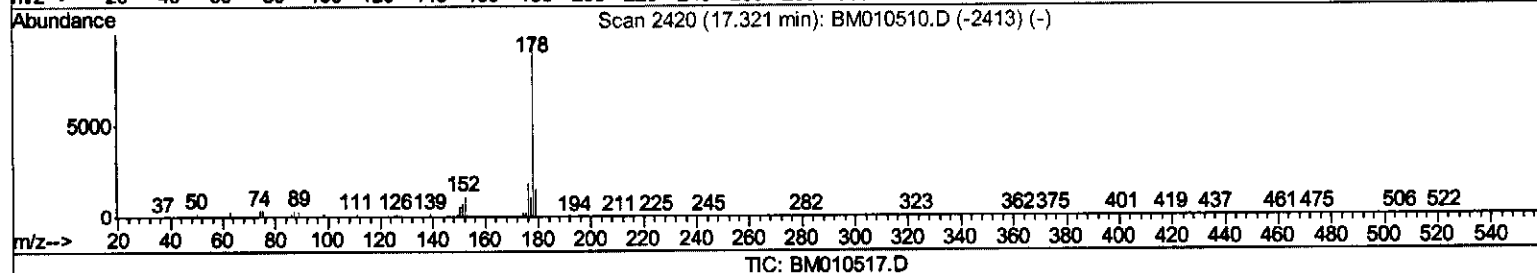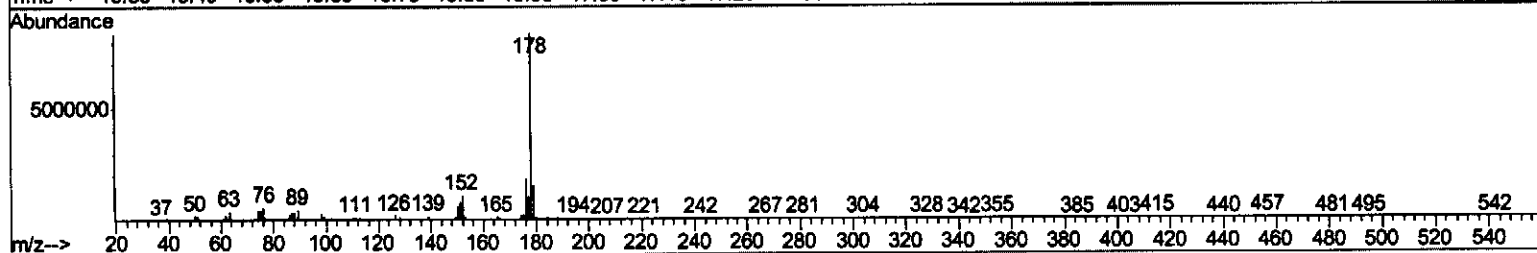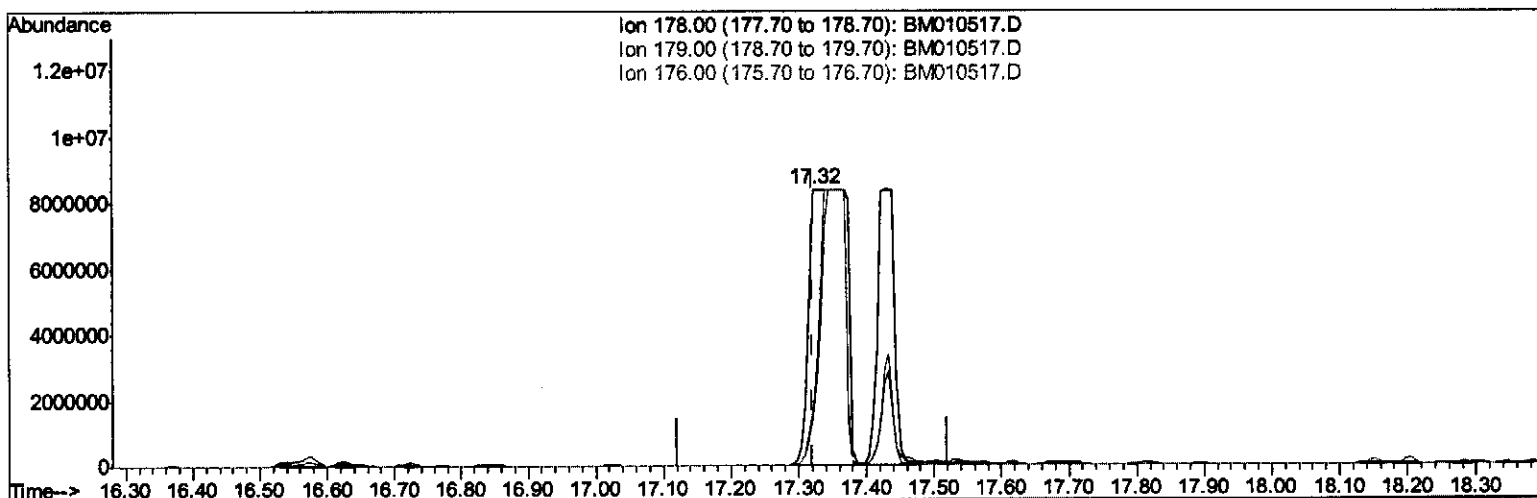

(69) Phenanthrene

17.321min (+0.000) 562.33ng/ul m

response 32120745

Ion	Exp%	Act%
178.00	100	100
179.00	15.80	18.60
176.00	18.60	21.66
0.00	0.00	0.00

56/19/17




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

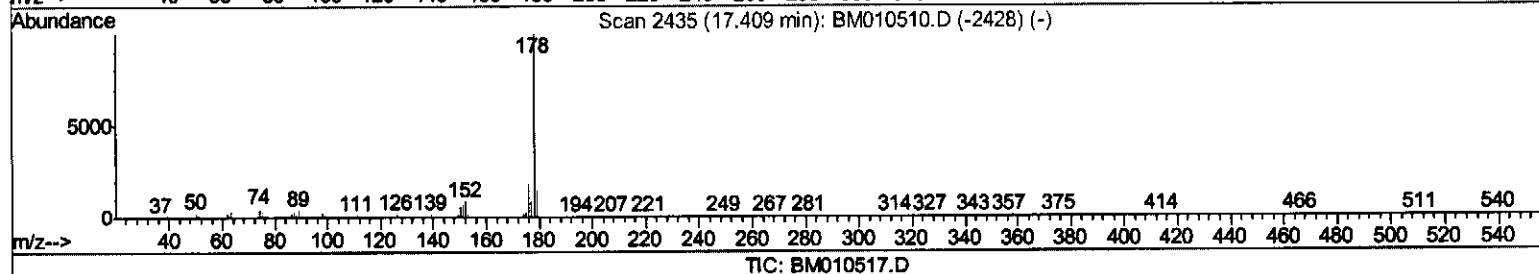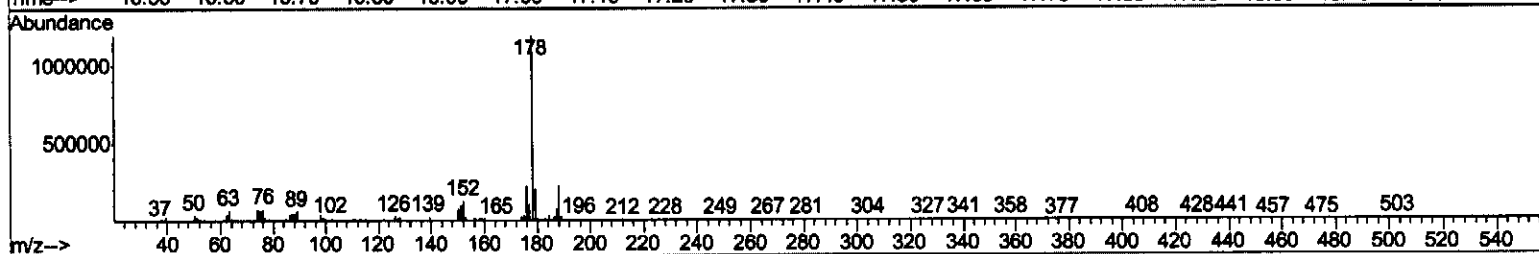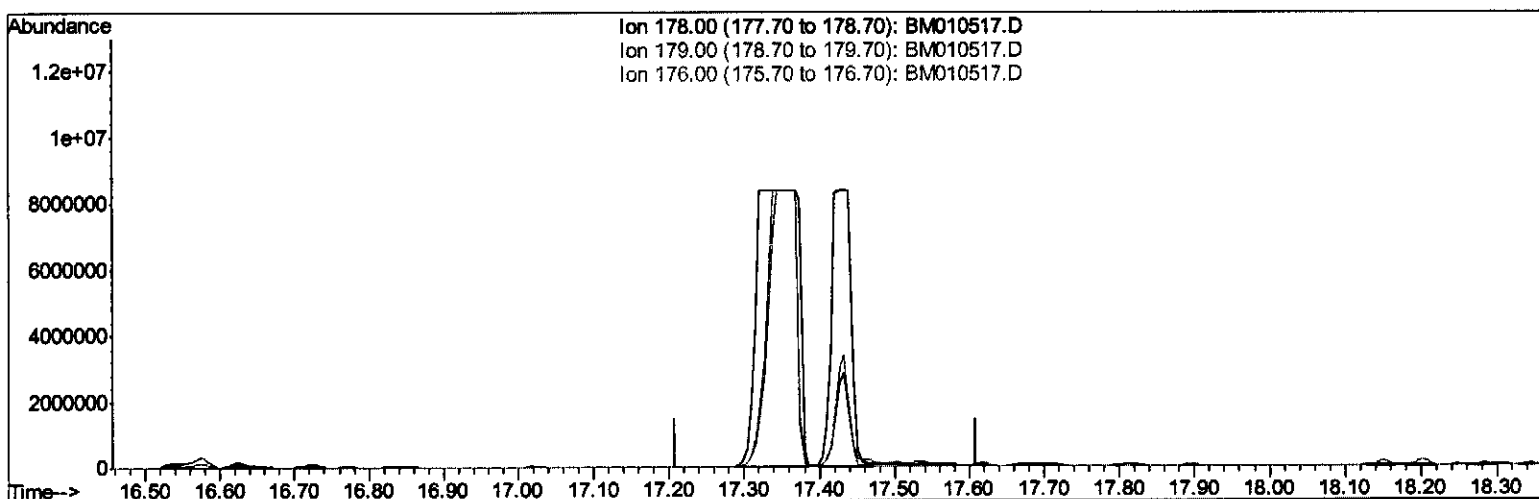

(71) Anthracene

17.409min (-17.409) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	14.60	0.00#
176.00	18.20	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

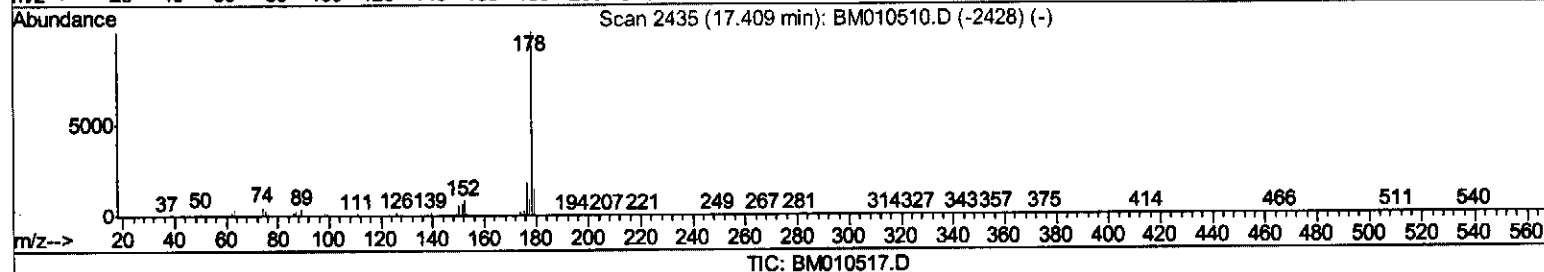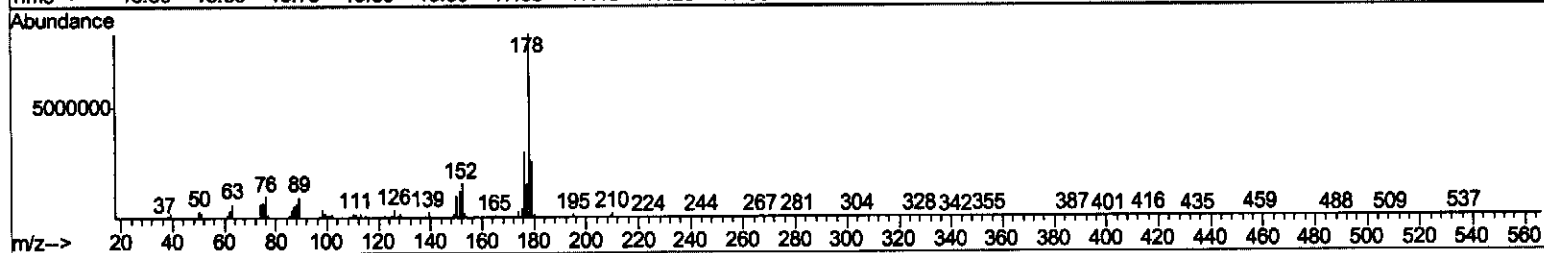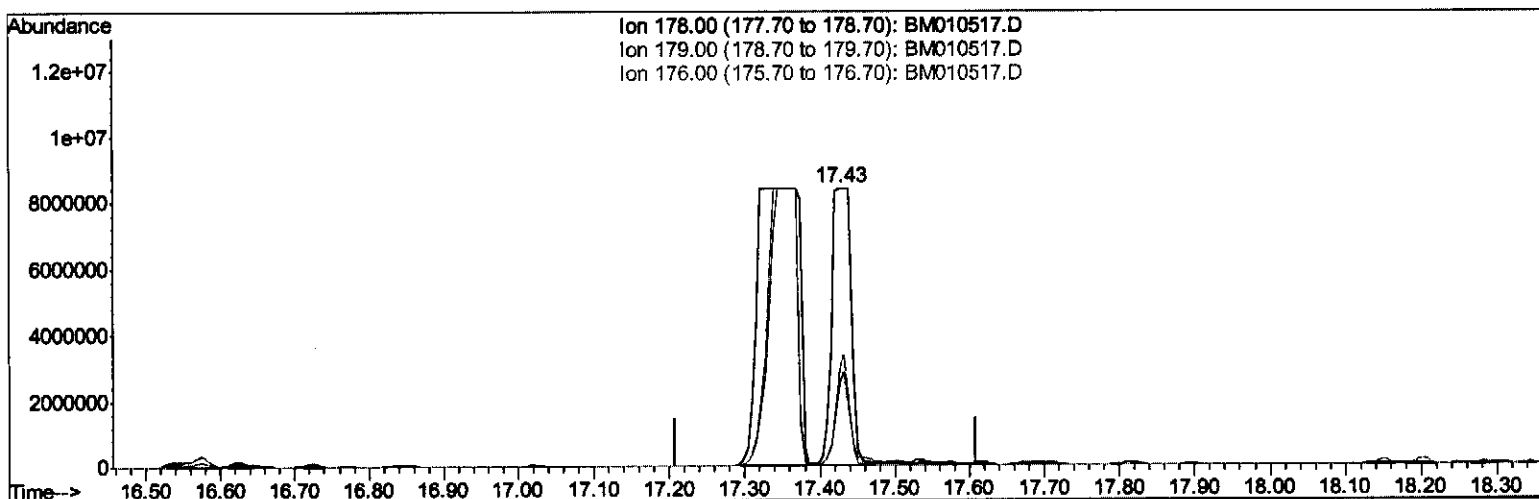

(71) Anthracene

17.427min (+0.018) 249.14ng/ul m

SS
06/19/17

response 14856732

Ion	Exp%	Act%
178.00	100	100
179.00	14.60	30.34#
176.00	18.20	35.60#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

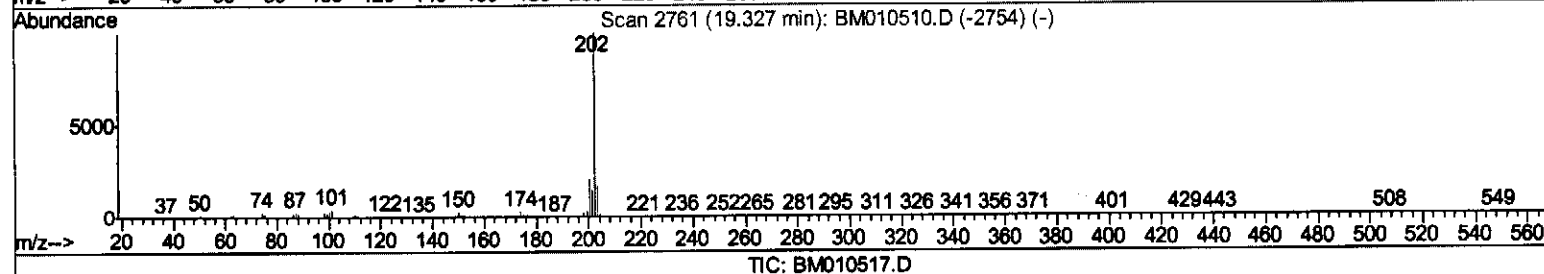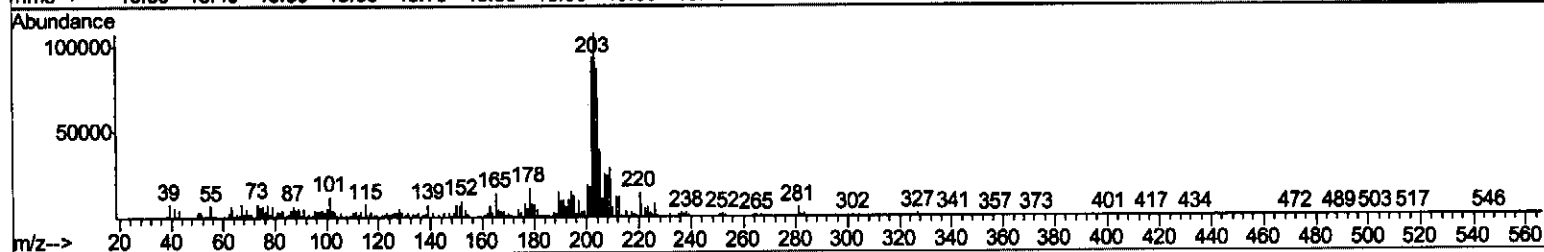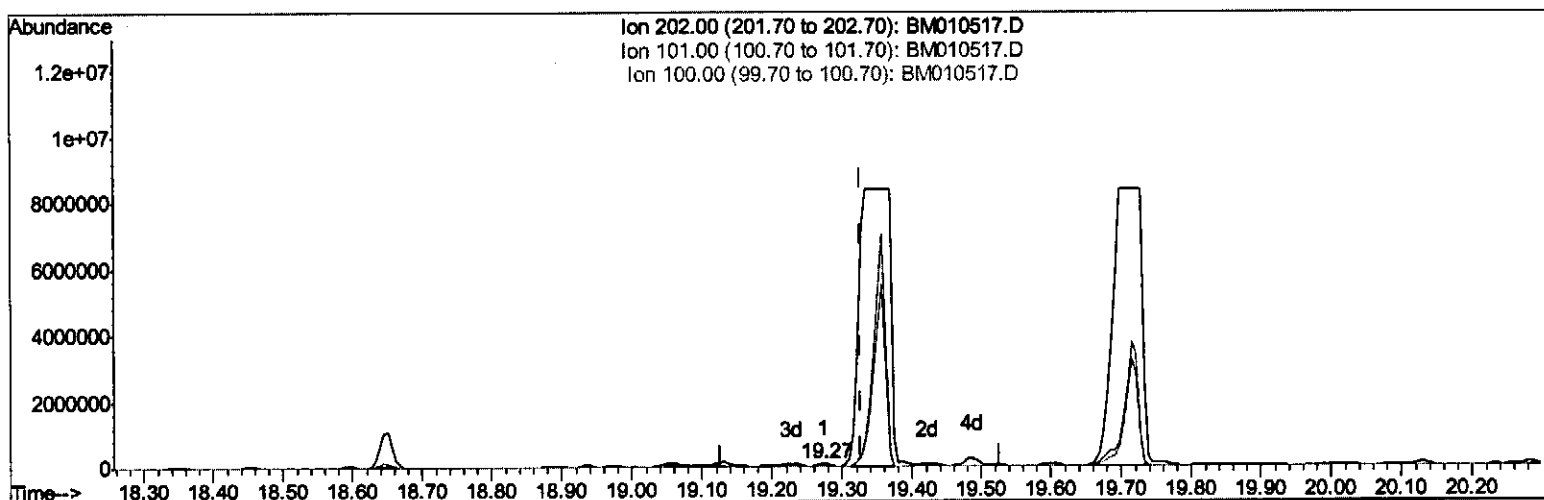

(74) Fluoranthene (C)

19.274min (-0.053) 1.15ng/ul

response 80863

Ion	Exp%	Act%
202.00	100	100
101.00	5.80	13.00#
100.00	4.30	5.71#
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

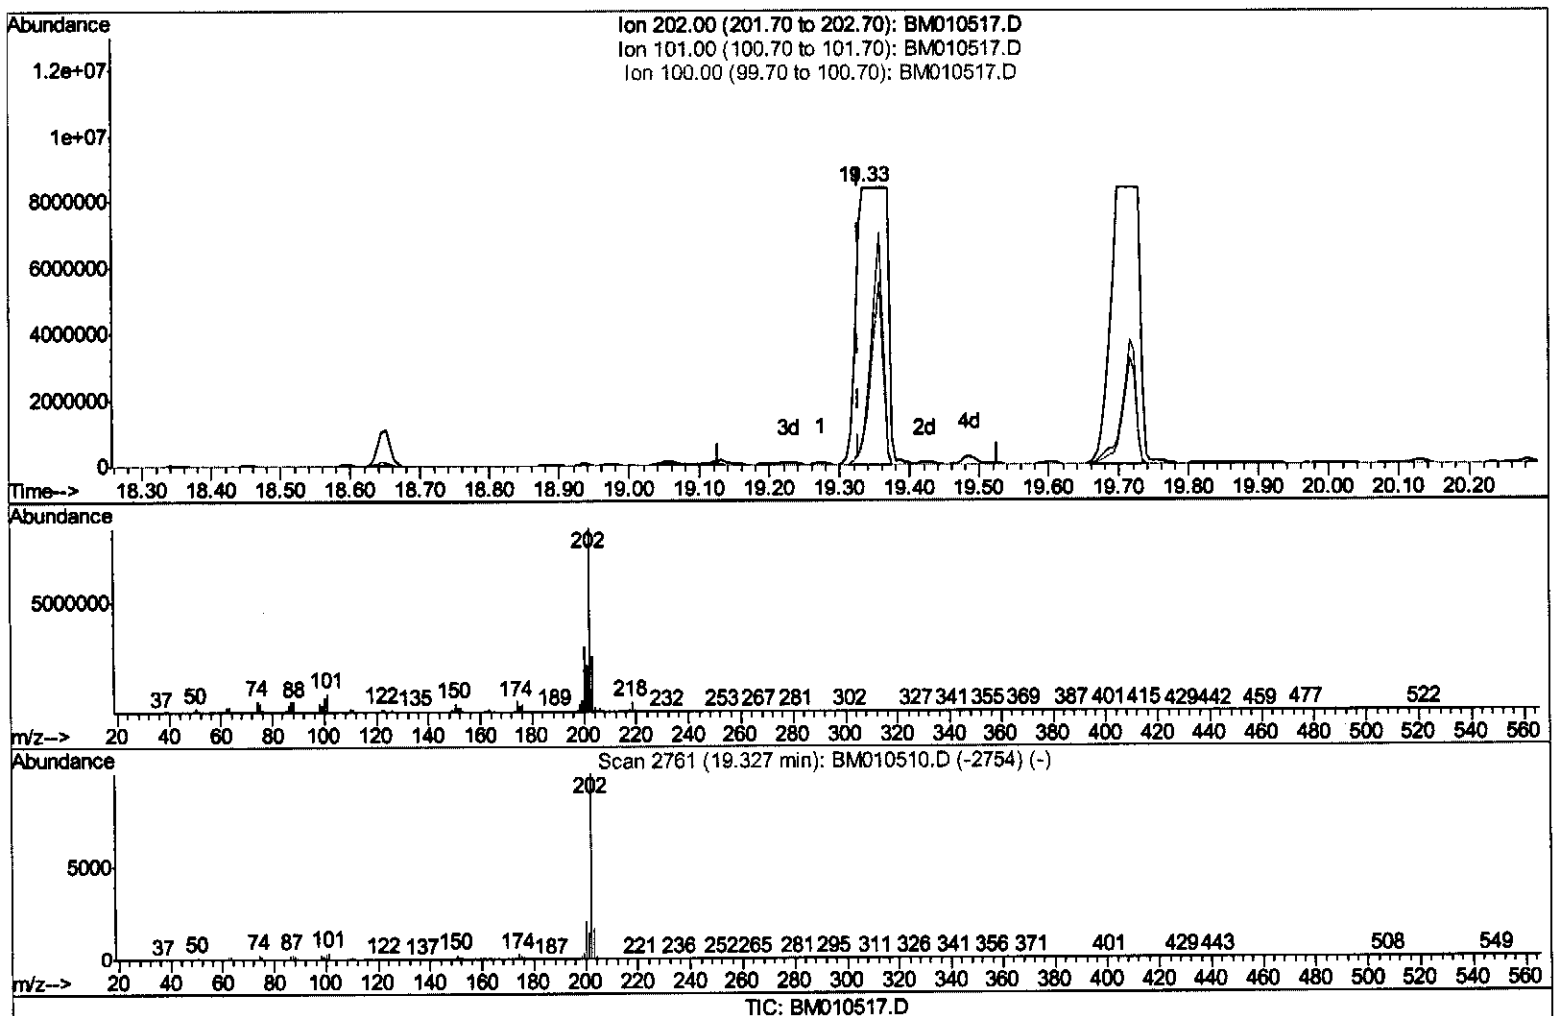

(74) Fluoranthene (C)

19.333min (+0.006) 359.96ng/ul m. *SJ* 6/19/17

response 25284800

Ion	Exp%	Act%
202.00	100	100
101.00	5.80	10.30#
100.00	4.30	8.51#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

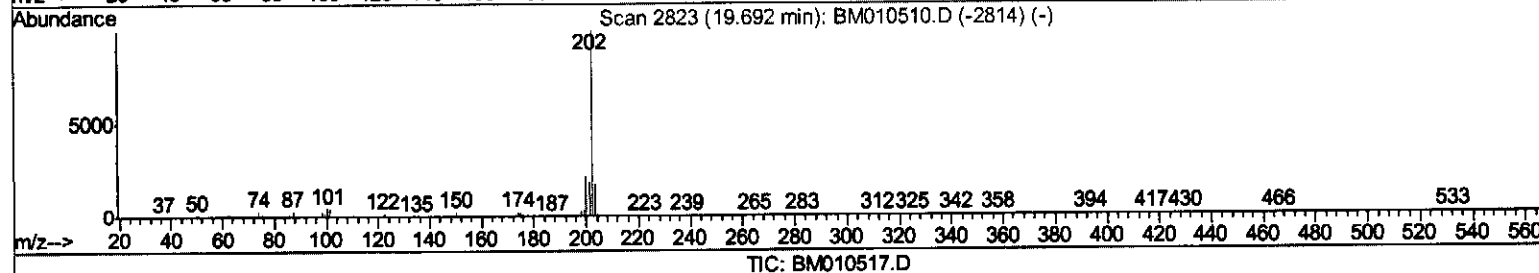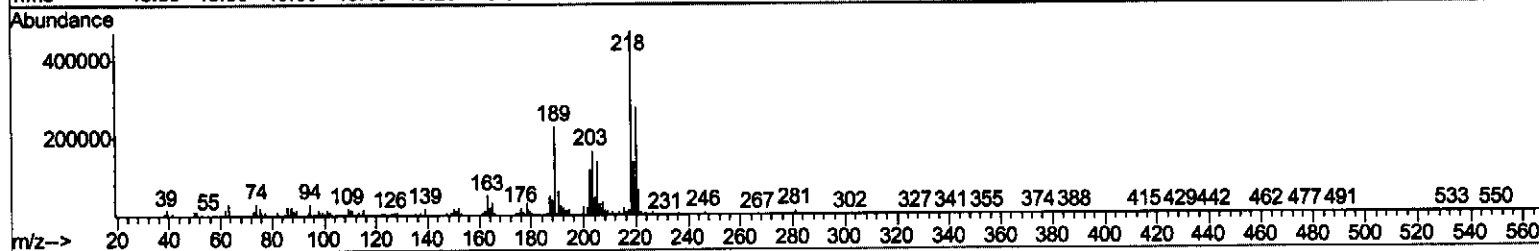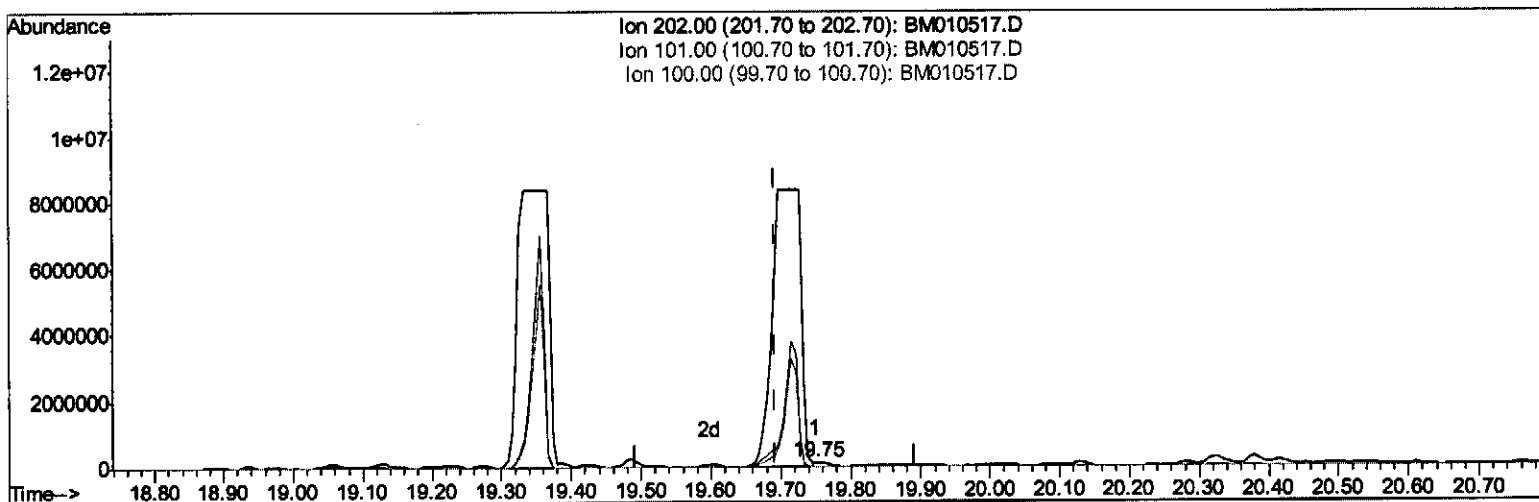

(77) Pyrene

19.751min (+0.059) 1.49ng/ul

response 135030

Ion	Exp%	Act%
202.00	100	100
101.00	6.40	14.59#
100.00	6.10	6.68
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

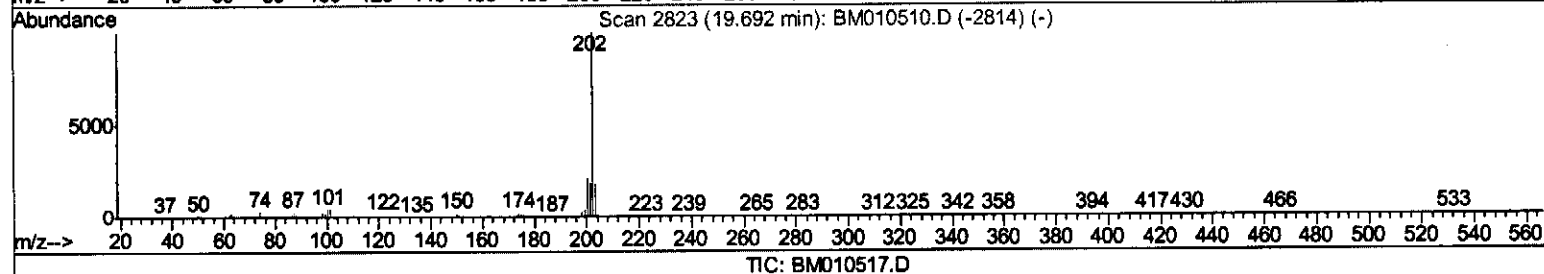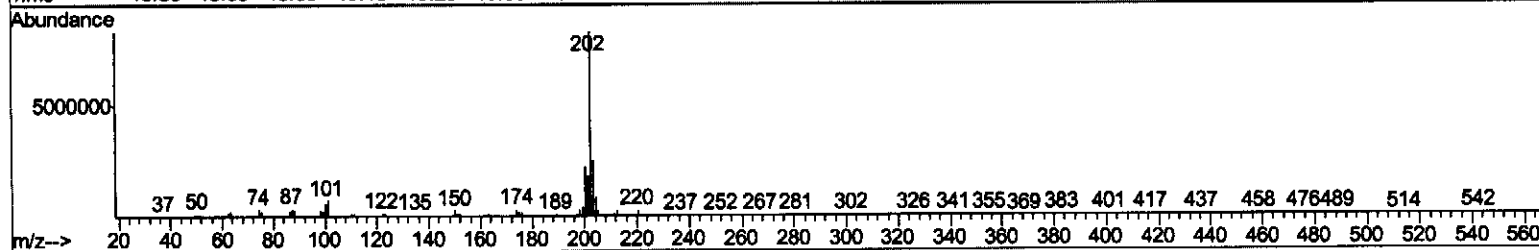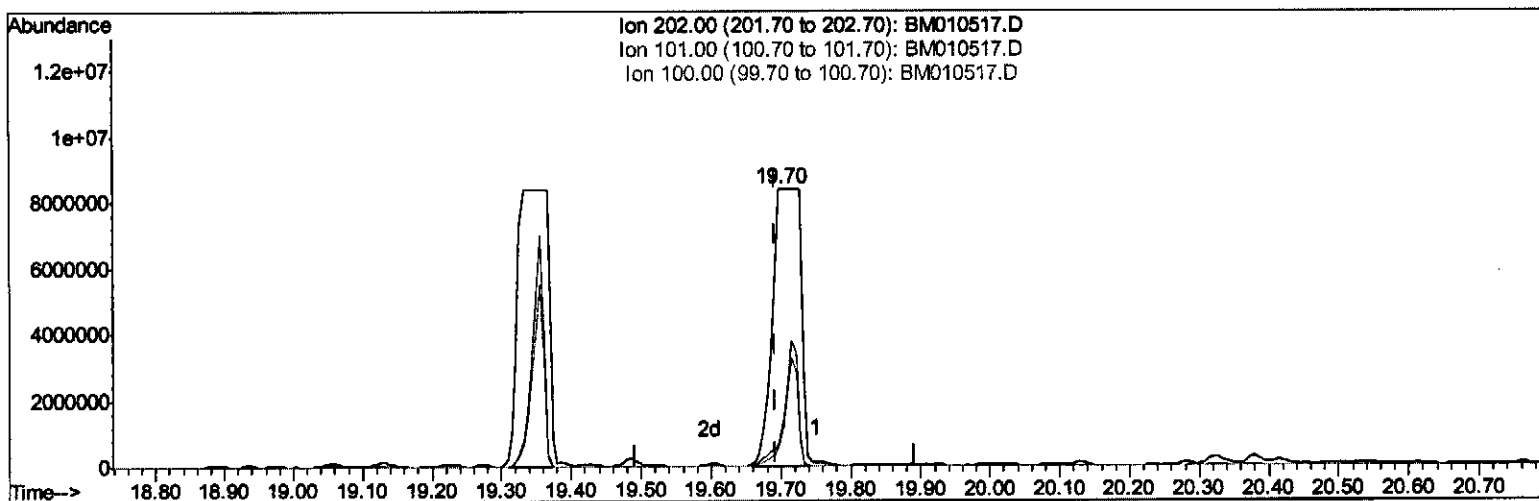

(77) Pyrene

19.698min (+0.006) 260.29ng/ul m

response 23540884

Ion	Exp%	Act%
202.00	100	100
101.00	6.40	8.68#
100.00	6.10	7.15
0.00	0.00	0.00

SJ
6/19/17


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

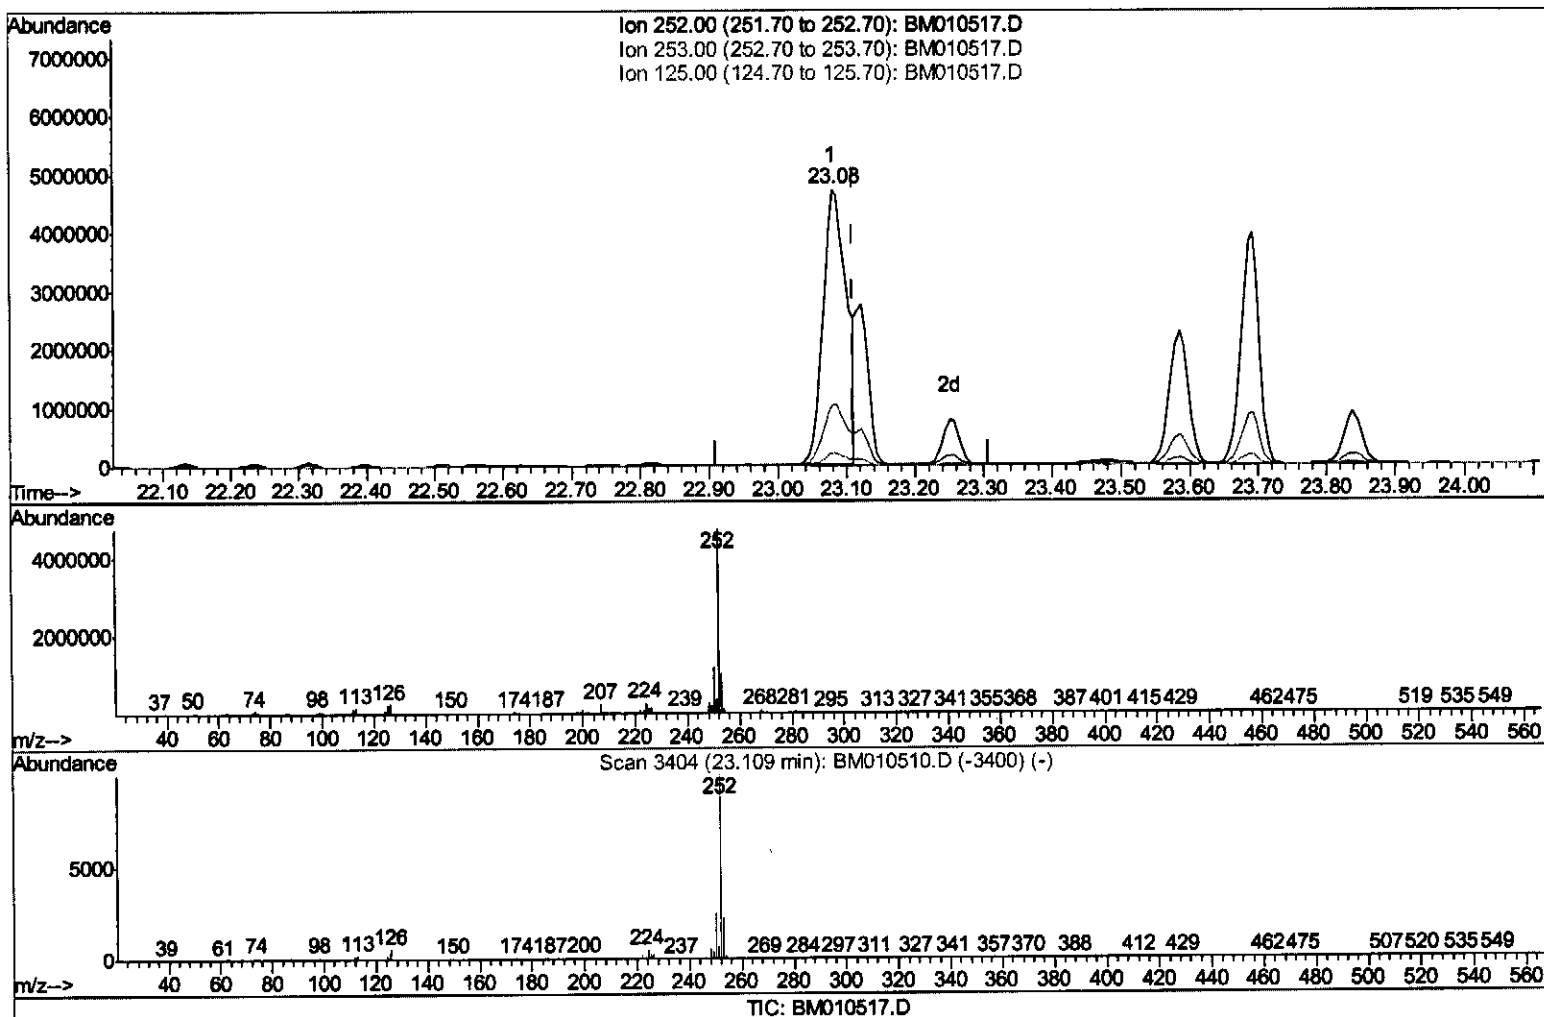

(86) Benzo(k)fluoranthene

23.080min (-0.029) 137.35ng/ul

response 11309164

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	21.94
125.00	4.30	4.51
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:47:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

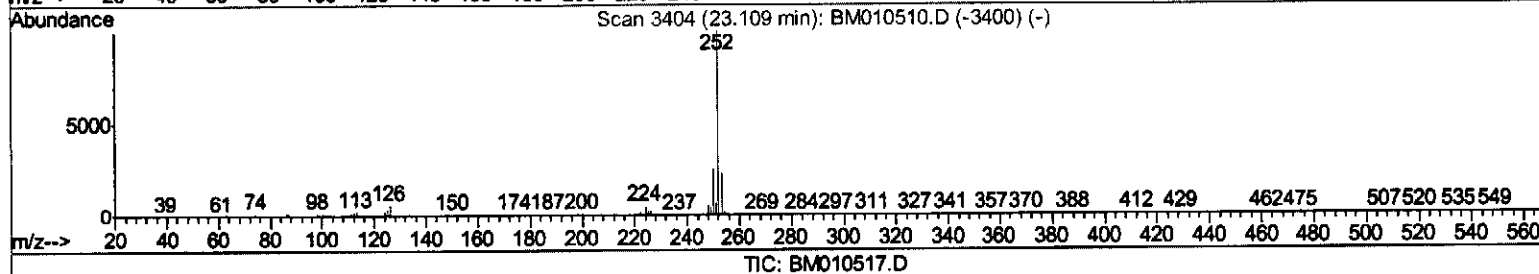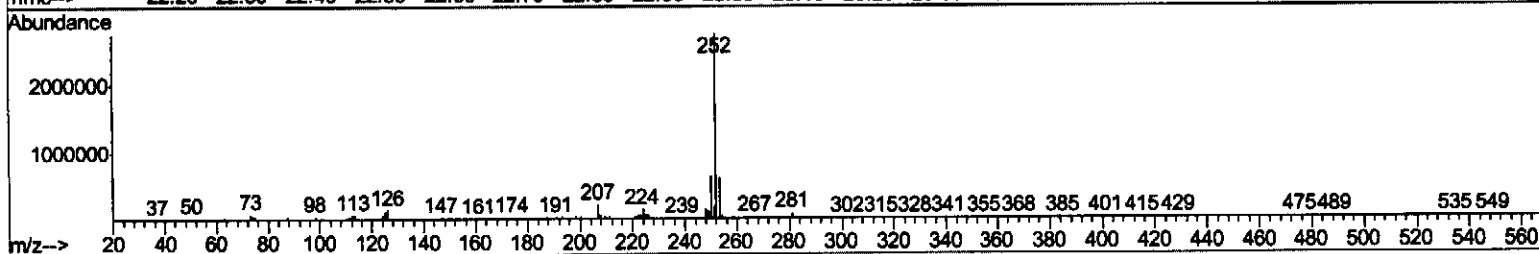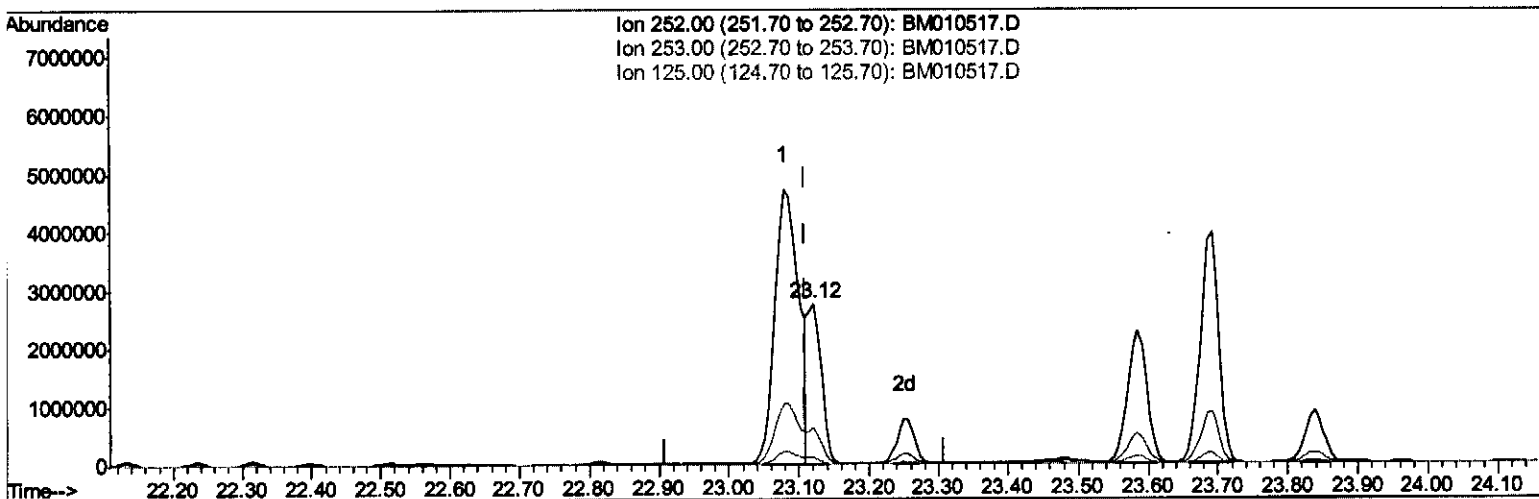

(86) Benzo(k)fluoranthene

23.121min (+0.012) 43.24ng/ul m

response 3560433

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.32
125.00	4.30	3.93
0.00	0.00	0.00

5/26/19/17

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
 Data File : BM010517.D
 Acq On : 11 Jun 2017 10:10
 Operator : SJ/MA
 Sample : I3558-09
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5C63

Manual Integrations
 APPROVED

mohammad
 6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:49:30 2017
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 12 09:00:46 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	167510	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	616482	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.53	164	422151	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.29	188	1069977	20.00	ng/ul	0.01
75) Chrysene-d12	21.45	240	1755123	20.00	ng/ul	0.00
83) Perylene-d12	23.79	264	1481219	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.36	96	10876	2.66	ng/uL	0.00
5) Phenol-d5	7.07	99	215643	16.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.23	67	124201	17.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.43	132	191459	18.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.62	113	177914	17.37	ng/ul	0.00
19) Nitrobenzene-d5	9.08	128	97823	21.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.79	143	115274	22.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.32	165	243606	22.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.86	131	320406m	30.90	ng/ul	0.00
43) Dimethylphthalate-d6	13.95	166	841171	23.98	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	916506	22.40	ng/ul	0.00
51) 4-Nitrophenol-d4	14.77	143	94429	17.99	ng/ul	0.00
57) Fluorene-d10	15.53	176	712576	23.11	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	112116	14.79	ng/ul	0.02
70) Anthracene-d10	17.39	188	1283857	24.66	ng/ul	0.02
76) Pyrene-d10	19.67	212	1857710	25.60	ng/ul	0.01
87) Benzo(a)pyrene-d12	23.64	264	1518349	22.02	ng/ul	0.01

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
28) Naphthalene	10.75	128	25939201m	838.884	ng/ul	92
34) 2-Methylnaphthalene	12.36	142	15110784	644.551	ng/ul	99
40) 1,1'-Biphenyl	13.36	154	3938753	115.013	ng/ul	98
44) Dimethylphthalate	13.99	163	361096	10.468	ng/ul	93
47) Acenaphthylene	14.26	152	587596	14.695	ng/ul#	77
49) Acenaphthene	14.60	153	15759051	561.964	ng/ul#	98
53) Dibenzofuran	14.93	168	15942700m	384.471	ng/ul	98
58) Fluorene	15.59	166	17194006m	505.496	ng/ul	99
69) Phenanthrene	17.32	178	32120745m	562.329	ng/ul	99
71) Anthracene	17.43	178	14856732m	249.140	ng/ul	98
72) Carbazole	17.70	167	4190767	83.029	ng/ul	98
74) Fluoranthene	19.33	202	25284800m	359.964	ng/ul	99
77) Pyrene	19.70	202	23540884m	260.285	ng/ul	99
80) Benzo(a)anthracene	21.43	228	14163360	143.102	ng/ul#	99
82) Chrysene	21.49	228	12750852	142.516	ng/ul#	99
85) Benzo(b)fluoranthene	23.08	252	11309164	131.213	ng/ul	99
86) Benzo(k)fluoranthene	23.12	252	3560433m	43.242	ng/ul	99
88) Benzo(a)pyrene	23.69	252	7201643	84.296	ng/ul	99
89) Indeno(1,2,3-cd)pyrene	26.17	276	2903503	26.900	ng/ul#	99
90) Dibenzo(a,h)anthracene	26.17	278	866387	9.320	ng/ul#	99
91) Benzo(g,h,i)perylene	26.91	276	2227200	25.047	ng/ul	96

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010517.D
Acq On : 11 Jun 2017 10:10
Operator : SJ/MA
Sample : I3558-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C63

Manual Integrations
APPROVED

mohammad
6/12/2017 3:41:24 PM

Quant Time: Jun 12 09:49:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 09:00:46 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						