

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
 Data File : BM010488.D
 Acq On : 10 Jun 2017 16:46
 Operator : SJ/MA
 Sample : I3522-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5A61

Quant Time: Jun 12 06:48:48 2017
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 12 04:15:09 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	169684	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	611569	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.53	164	418274	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.28	188	1057210	20.00	ng/ul	0.00
75) Chrysene-d12	21.44	240	1442862	20.00	ng/ul	0.00
83) Perylene-d12	23.78	264	1517759	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.36	96	9067	2.19	ng/uL	0.00
5) Phenol-d5	7.08	99	125994	9.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.24	67	77294	10.70	ng/ul	0.00
9) 2-Chlorophenol-d4	7.43	132	123807	12.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.62	113	104491	10.07	ng/ul	0.00
19) Nitrobenzene-d5	9.08	128	57867	12.92	ng/ul	0.00
22) 2-Nitrophenol-d4	9.79	143	69054	13.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.32	165	141894	13.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.86	131	127000	12.35	ng/ul	0.00
43) Dimethylphthalate-d6	13.94	166	514778	14.81	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	535571	13.21	ng/ul	0.00
51) 4-Nitrophenol-d4	14.77	143	53510	10.29	ng/ul	0.00
57) Fluorene-d10	15.52	176	422954	13.85	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.65	200	85268	11.39	ng/ul	0.00
70) Anthracene-d10	17.37	188	729472	14.18	ng/ul	0.00
76) Pyrene-d10	19.67	212	941328	15.78	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.63	264	1029859	14.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.99	163	337461	9.874	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010488.D
Acq On : 10 Jun 2017 16:46
Operator : SJ/MA
Sample : I3522-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5A61

Quant Time: Jun 12 06:48:48 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 04:15:09 2017
Response via : Initial Calibration

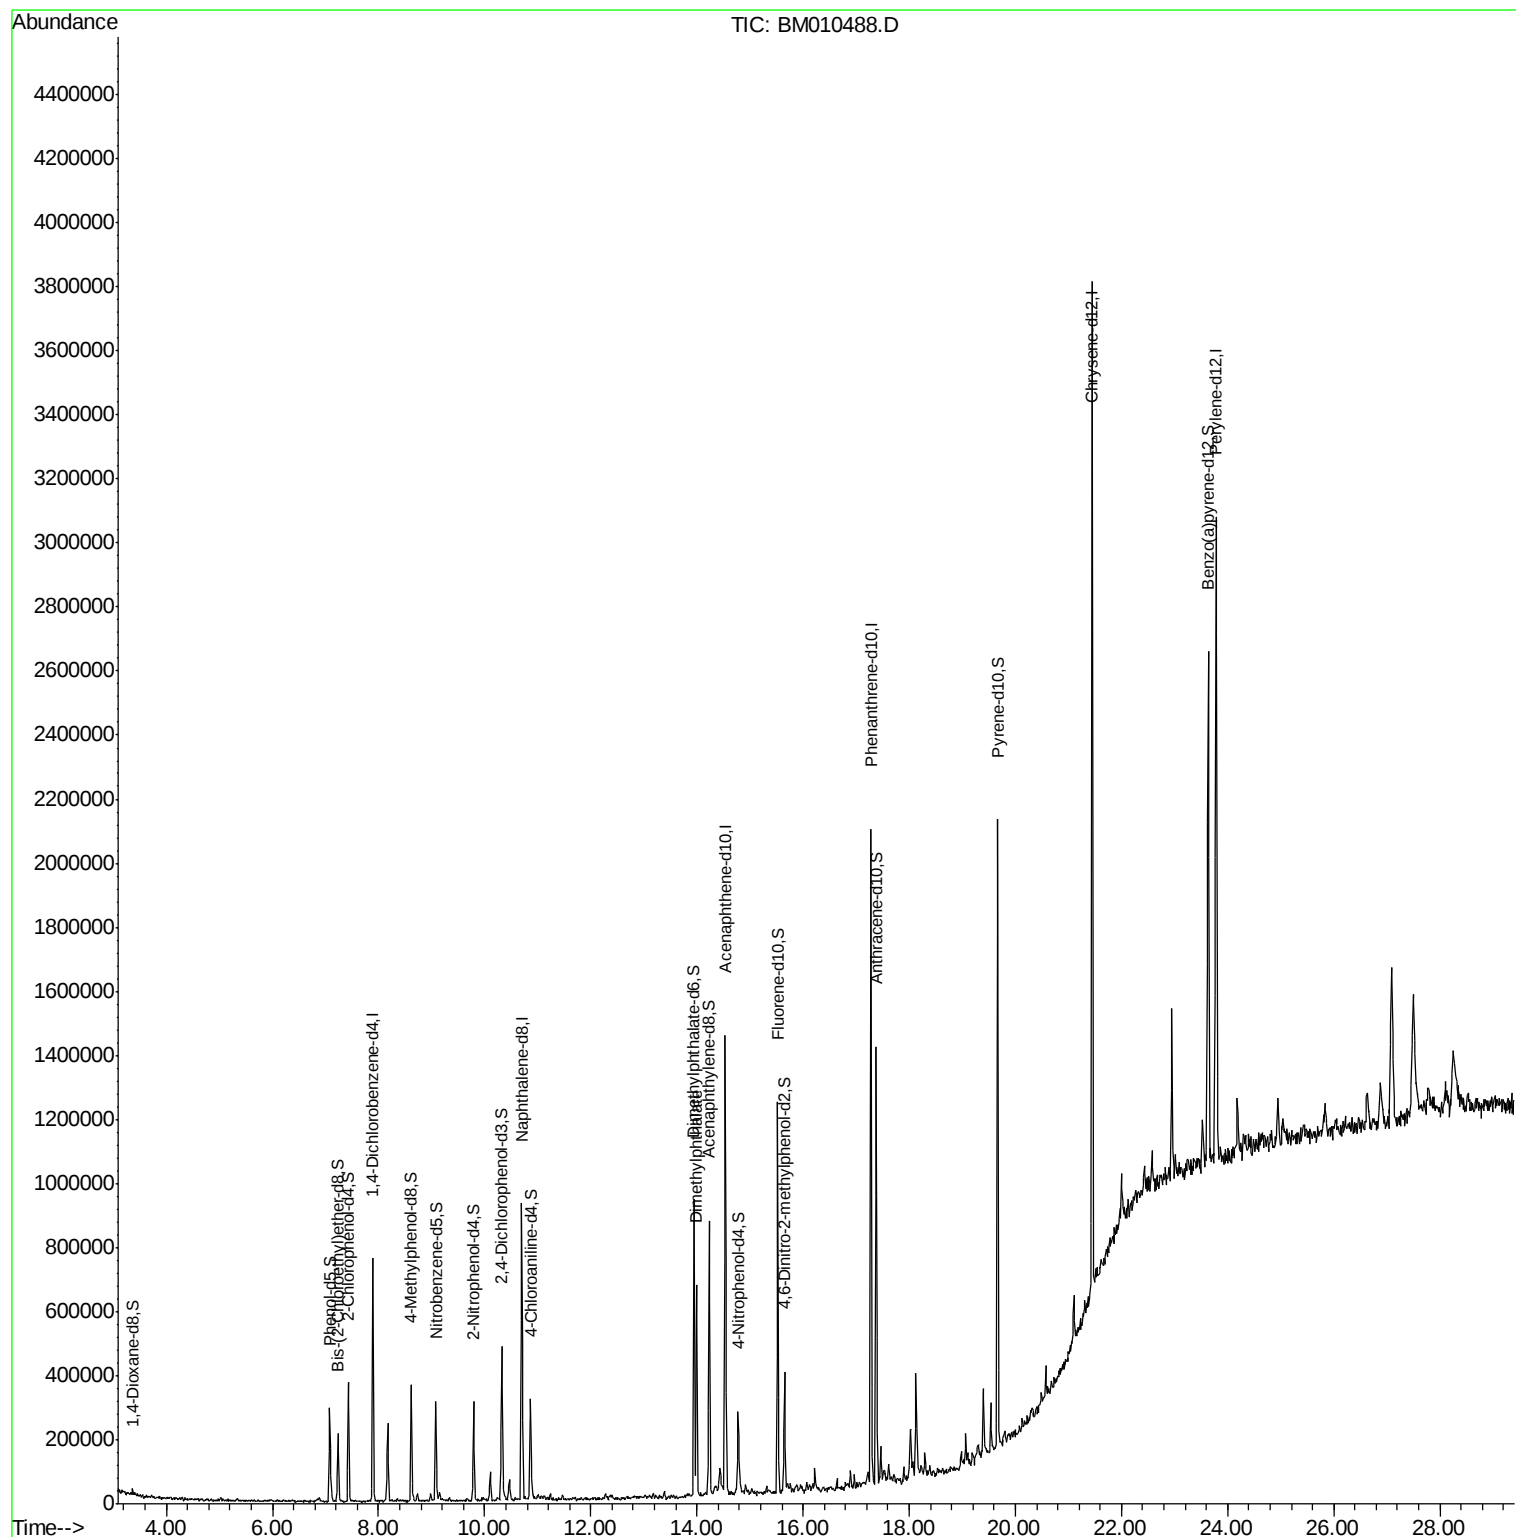


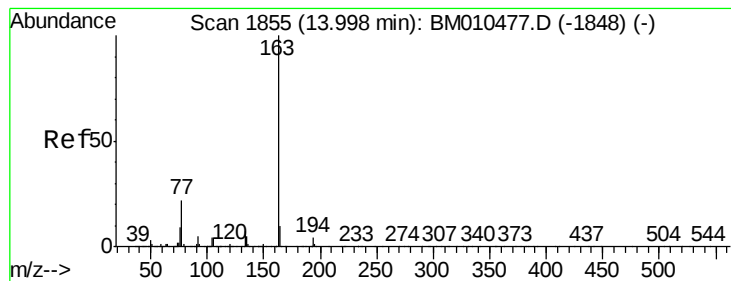

#44
 Dimethylphthalate
 Concen: 9.874 ng/ul
 RT: 13.99 min Scan# 1854
 Delta R.T. -0.01 min
 Lab File: BM010488.D
 Acq: 10 Jun 2017 16:46

Instrument :
 BNA_M
 ClientSampleId :
 F5A61

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.5	5.3
164	9.9	8.2	12.4

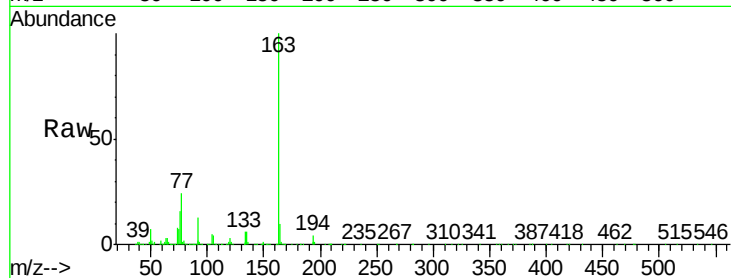

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

