

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
 Data File : BM010489.D
 Acq On : 10 Jun 2017 17:22
 Operator : SJ/MA
 Sample : I3522-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5C90

Quant Time: Jun 12 04:18:04 2017
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 12 04:15:09 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	141304	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	510386	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.53	164	367746	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.28	188	927704	20.00	ng/ul	0.00
75) Chrysene-d12	21.44	240	1330296	20.00	ng/ul	0.00
83) Perylene-d12	23.79	264	1412334	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.36	96	7427	2.16	ng/uL	0.00
5) Phenol-d5	7.08	99	120278	11.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.24	67	68476	11.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.43	132	106546	12.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.62	113	99489	11.52	ng/ul	0.00
19) Nitrobenzene-d5	9.08	128	49819	13.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.79	143	60641	14.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.32	165	125222	14.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.86	131	127585	14.86	ng/ul	0.00
43) Dimethylphthalate-d6	13.95	166	465242	15.23	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	461848	12.96	ng/ul	0.00
51) 4-Nitrophenol-d4	14.77	143	54363	11.89	ng/ul	0.00
57) Fluorene-d10	15.52	176	372171	13.86	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.65	200	75037	11.42	ng/ul	0.00
70) Anthracene-d10	17.38	188	641302	14.21	ng/ul	0.00
76) Pyrene-d10	19.67	212	842708	15.32	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.63	264	951802	14.47	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.99	163	244422	8.134	ng/ul 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010489.D
Acq On : 10 Jun 2017 17:22
Operator : SJ/MA
Sample : I3522-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C90

Quant Time: Jun 12 04:18:04 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 04:15:09 2017
Response via : Initial Calibration

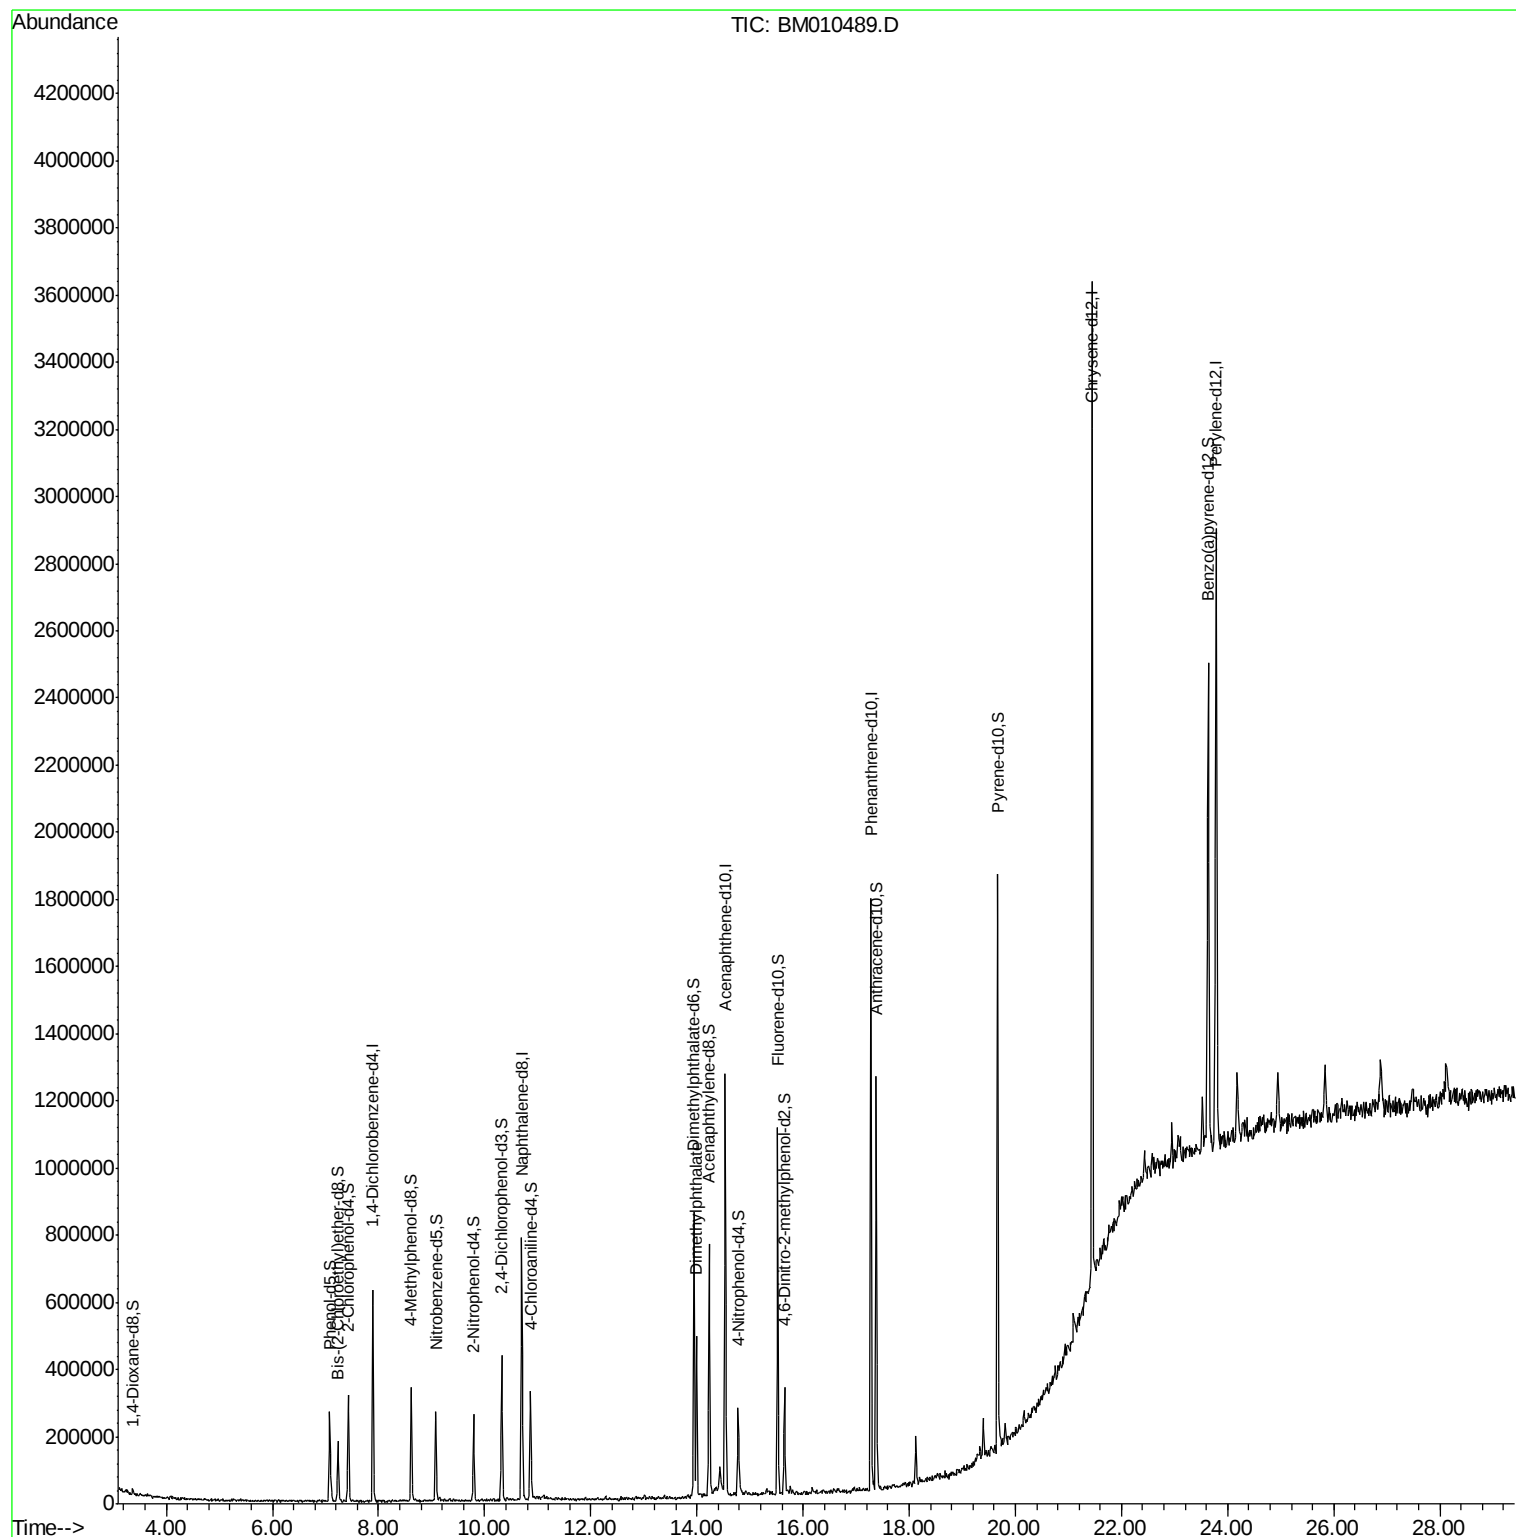

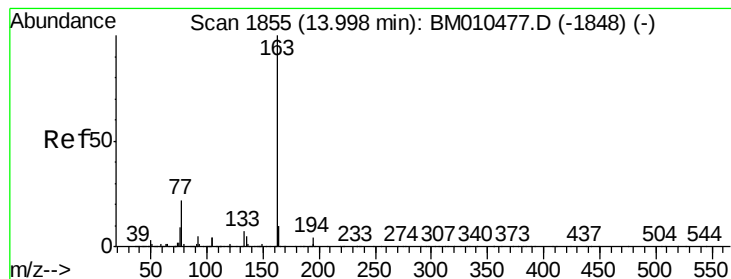

#44

Dimethylphthalate

Concen: 8.134 ng/ul

RT: 13.99 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BM010489.D

Acq: 10 Jun 2017 17:22

Instrument :

BNA_M

ClientSampleId :

F5C90

Tgt Ion:163 Resp: 244422

Ion Ratio Lower Upper

163 100

194 5.0 3.5 5.3

164 9.1 8.2 12.4

