

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
 Data File : BM010508.D
 Acq On : 11 Jun 2017 04:46
 Operator : SJ/MA
 Sample : I3558-18
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5D39

Quant Time: Jun 12 08:51:31 2017
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 12 07:08:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	162670	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	571240	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.53	164	404573	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.28	188	1001351	20.00	ng/ul	0.00
75) Chrysene-d12	21.44	240	1359601	20.00	ng/ul	0.00
83) Perylene-d12	23.78	264	1402048	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.36	96	20887	5.27	ng/uL	0.00
5) Phenol-d5	7.07	99	364796	29.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.23	67	213463	30.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.43	132	321107	32.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.62	113	317553	31.93	ng/ul	0.00
19) Nitrobenzene-d5	9.08	128	151751	36.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.79	143	193034	39.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.32	165	397525	39.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.86	131	397351	41.36	ng/ul	0.00
43) Dimethylphthalate-d6	13.94	166	1349011	40.13	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	1456996	37.16	ng/ul	0.00
51) 4-Nitrophenol-d4	14.77	143	162985	32.41	ng/ul	0.00
57) Fluorene-d10	15.52	176	1162156	39.33	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.65	200	233127	32.87	ng/ul	0.00
70) Anthracene-d10	17.37	188	1888391	38.76	ng/ul	0.00
76) Pyrene-d10	19.66	212	2348658	41.77	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.63	264	2530835	38.77	ng/ul	0.00
Target Compounds						
6) Phenol	7.10	94	25369	2.007	ng/ul#	71
44) Dimethylphthalate	13.99	163	505247	15.284	ng/ul	97
69) Phenanthrene	17.32	178	55899	1.046	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010508.D
Acq On : 11 Jun 2017 04:46
Operator : SJ/MA
Sample : I3558-18
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5D39

Quant Time: Jun 12 08:51:31 2017
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 12 07:08:51 2017
Response via : Initial Calibration

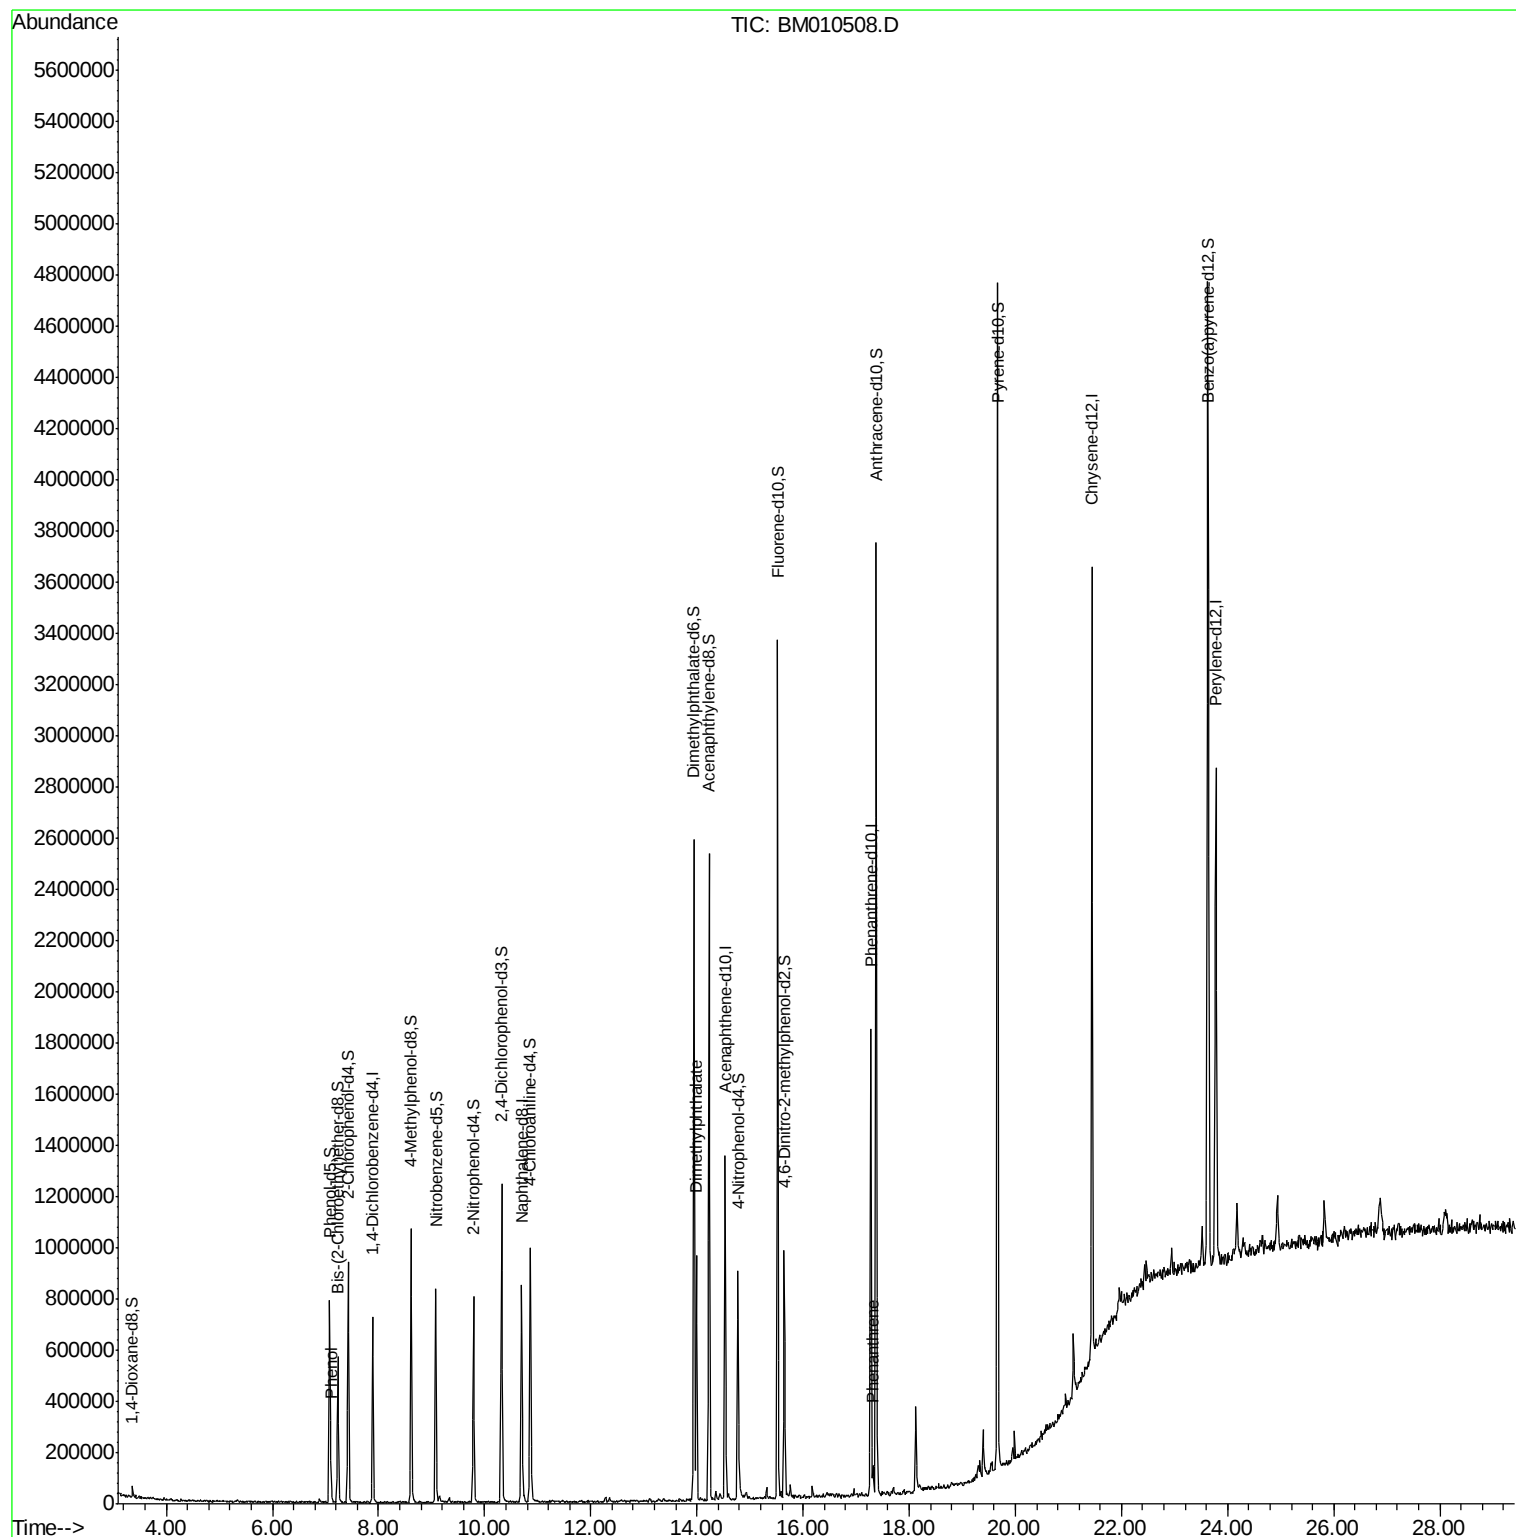

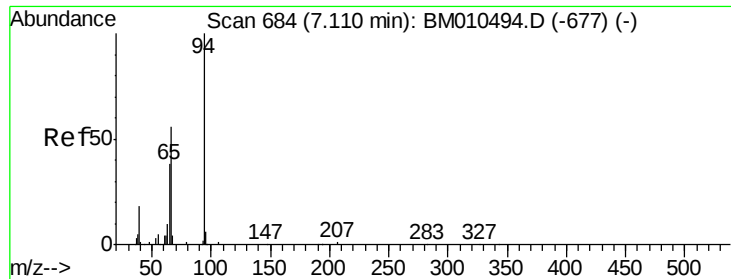

#6

Phenol

Concen: 2.007 ng/ul

RT: 7.10 min Scan# 683

Delta R.T. -0.01 min

Lab File: BM010508.D

Acq: 11 Jun 2017 04:46

Instrument :

BNA_M

ClientSampleId :

F5D39


Tgt Ion: 94 Resp: 25369

Ion Ratio Lower Upper

94 100

65 44.6 28.2 42.4#




66 86.0 47.2 70.8#

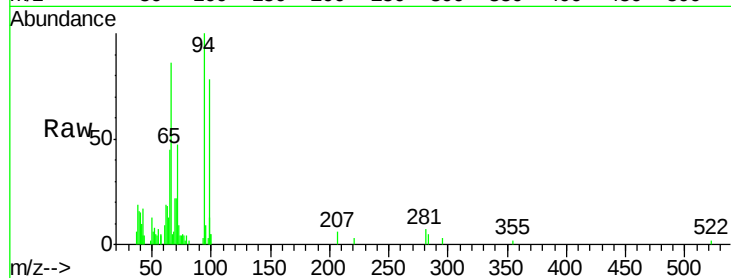

Abundance Ion 94.00 (93.70 to 94.70): BM010494.D (-677) (-)

Ion 65.00 (64.70 to 65.70): BM010494.D (-677) (-)

Ion 66.00 (65.70 to 66.70): BM010494.D (-677) (-)

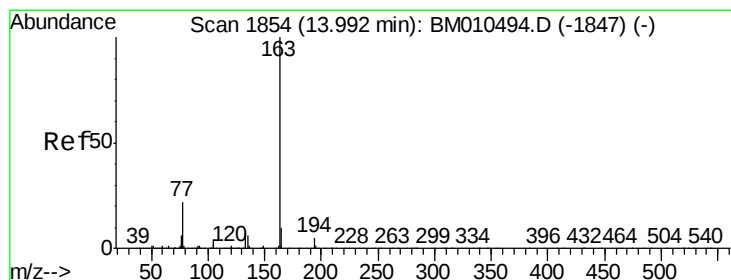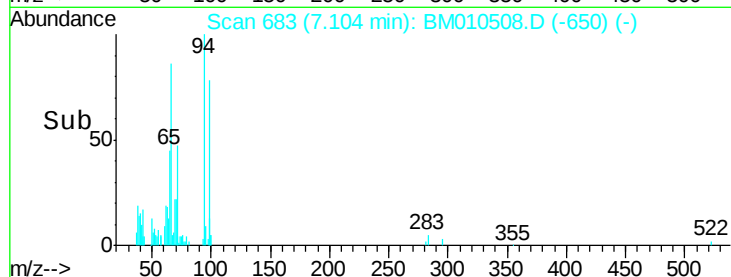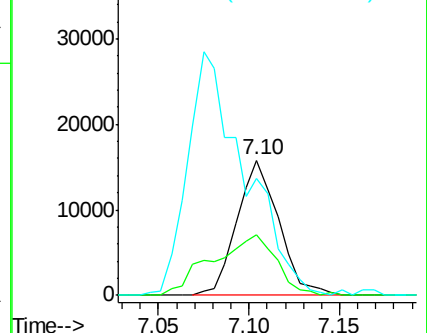

#44

Dimethylphthalate

Concen: 15.284 ng/ul

RT: 13.99 min Scan# 1854

Delta R.T. 0.00 min

Lab File: BM010508.D

Acq: 11 Jun 2017 04:46


Tgt Ion: 163 Resp: 505247

Ion Ratio Lower Upper

163 100

194 4.8 3.5 5.3



164 9.0 8.2 12.4

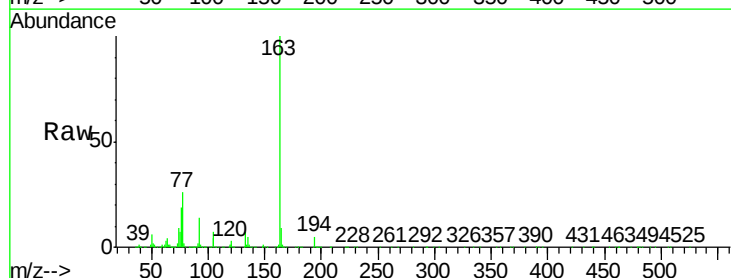


Abundance Ion 163.00 (162.70 to 163.70): BM010494.D (-1847) (-)

Ion 194.00 (193.70 to 194.70): BM010494.D (-1847) (-)

Ion 164.00 (163.70 to 164.70): BM010494.D (-1847) (-)

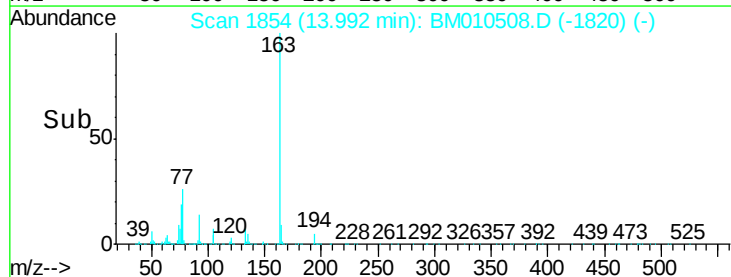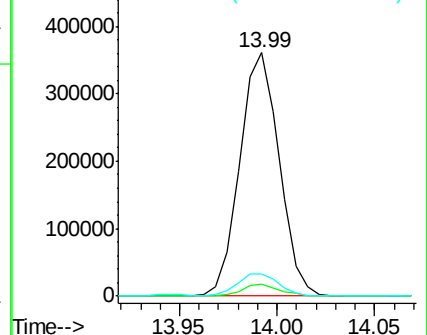

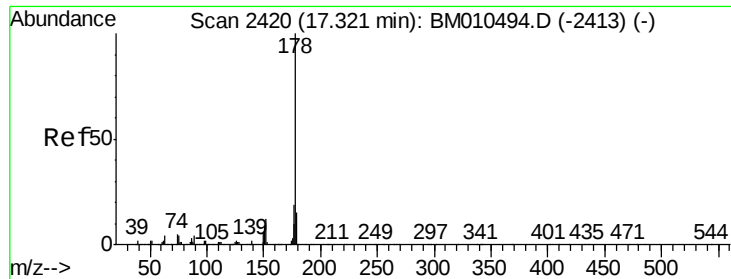

#69

Phenanthrene

Concen: 1.046 ng/ul

RT: 17.32 min Scan# 2419

Delta R.T. -0.01 min

Lab File: BM010508.D

Acq: 11 Jun 2017 04:46

Instrument :

BNA_M

ClientSampleId :

F5D39


Tgt Ion:178 Resp: 55899

Ion Ratio Lower Upper

178 100

179 19.0 12.6 19.0#

176 17.3 14.9 22.3

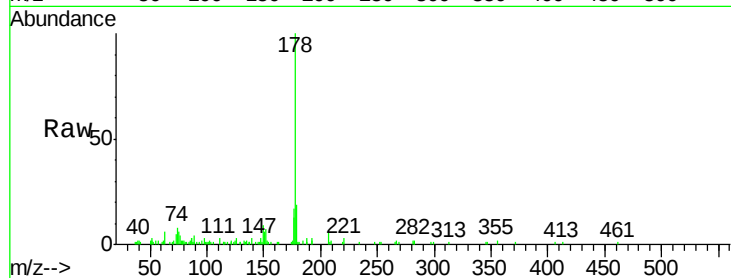

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

