

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
 Data File : BM010486.D
 Acq On : 10 Jun 2017 15:34
 Operator : SJ/MA
 Sample : PB99638BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK38

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.081	671	679	687	rBV	831152	1276197	18.30%	2.109%
2	7.240	699	706	716	rVB	558747	868369	12.45%	1.435%
3	7.434	730	739	746	rBV	952233	1501163	21.53%	2.481%
4	7.892	810	817	825	rVB	778475	1226479	17.59%	2.027%
5	8.616	934	940	949	rBV2	1005832	1655433	23.74%	2.736%
6	9.081	1011	1019	1028	rBV	827554	1366973	19.61%	2.259%
7	9.792	1131	1140	1150	rBV	831332	1393675	19.99%	2.303%
8	10.322	1223	1230	1240	rBV	1221222	2067473	29.65%	3.417%
9	10.698	1286	1294	1301	rBV	960292	1593834	22.86%	2.634%
10	10.863	1315	1322	1333	rBV	1008545	1751344	25.12%	2.894%
11	13.945	1839	1846	1854	rBV	2526565	3511281	50.36%	5.803%
12	14.233	1887	1895	1901	rBV	2409469	3444250	49.40%	5.692%
13	14.433	1919	1929	1937	rBV3	76715	213820	3.07%	0.353%
14	14.533	1940	1946	1954	rVB2	1479895	2266065	32.50%	3.745%
15	14.774	1980	1987	1997	rBV	996069	1605196	23.02%	2.653%
16	15.527	2107	2115	2123	rBV	3095386	4512850	64.73%	7.458%
17	15.651	2129	2136	2145	rBV	1144941	1527229	21.90%	2.524%
18	15.757	2150	2154	2159	rVB5	51385	81802	1.17%	0.135%
19	17.280	2406	2413	2419	rBV	2041548	2847238	40.84%	4.706%
20	17.380	2424	2430	2438	rBV	3964593	5311799	76.19%	8.779%
21	19.298	2753	2756	2761	rBV2	49685	81815	1.17%	0.135%
22	19.398	2770	2773	2781	rBV9	52298	95361	1.37%	0.158%
23	19.668	2813	2819	2825	rBV	4634466	6130872	87.93%	10.132%
24	21.445	3117	3121	3128	rVB	2832321	3545059	50.85%	5.859%
25	23.633	3487	3493	3503	rVB2	3764051	6972081	100.00%	11.523%
26	23.786	3513	3519	3526	rVB	1962693	3660264	52.50%	6.049%


Sum of corrected areas: 60507922

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010486.D
Acq On : 10 Jun 2017 15:34
Operator : SJ/MA
Sample : PB99638BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK38

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

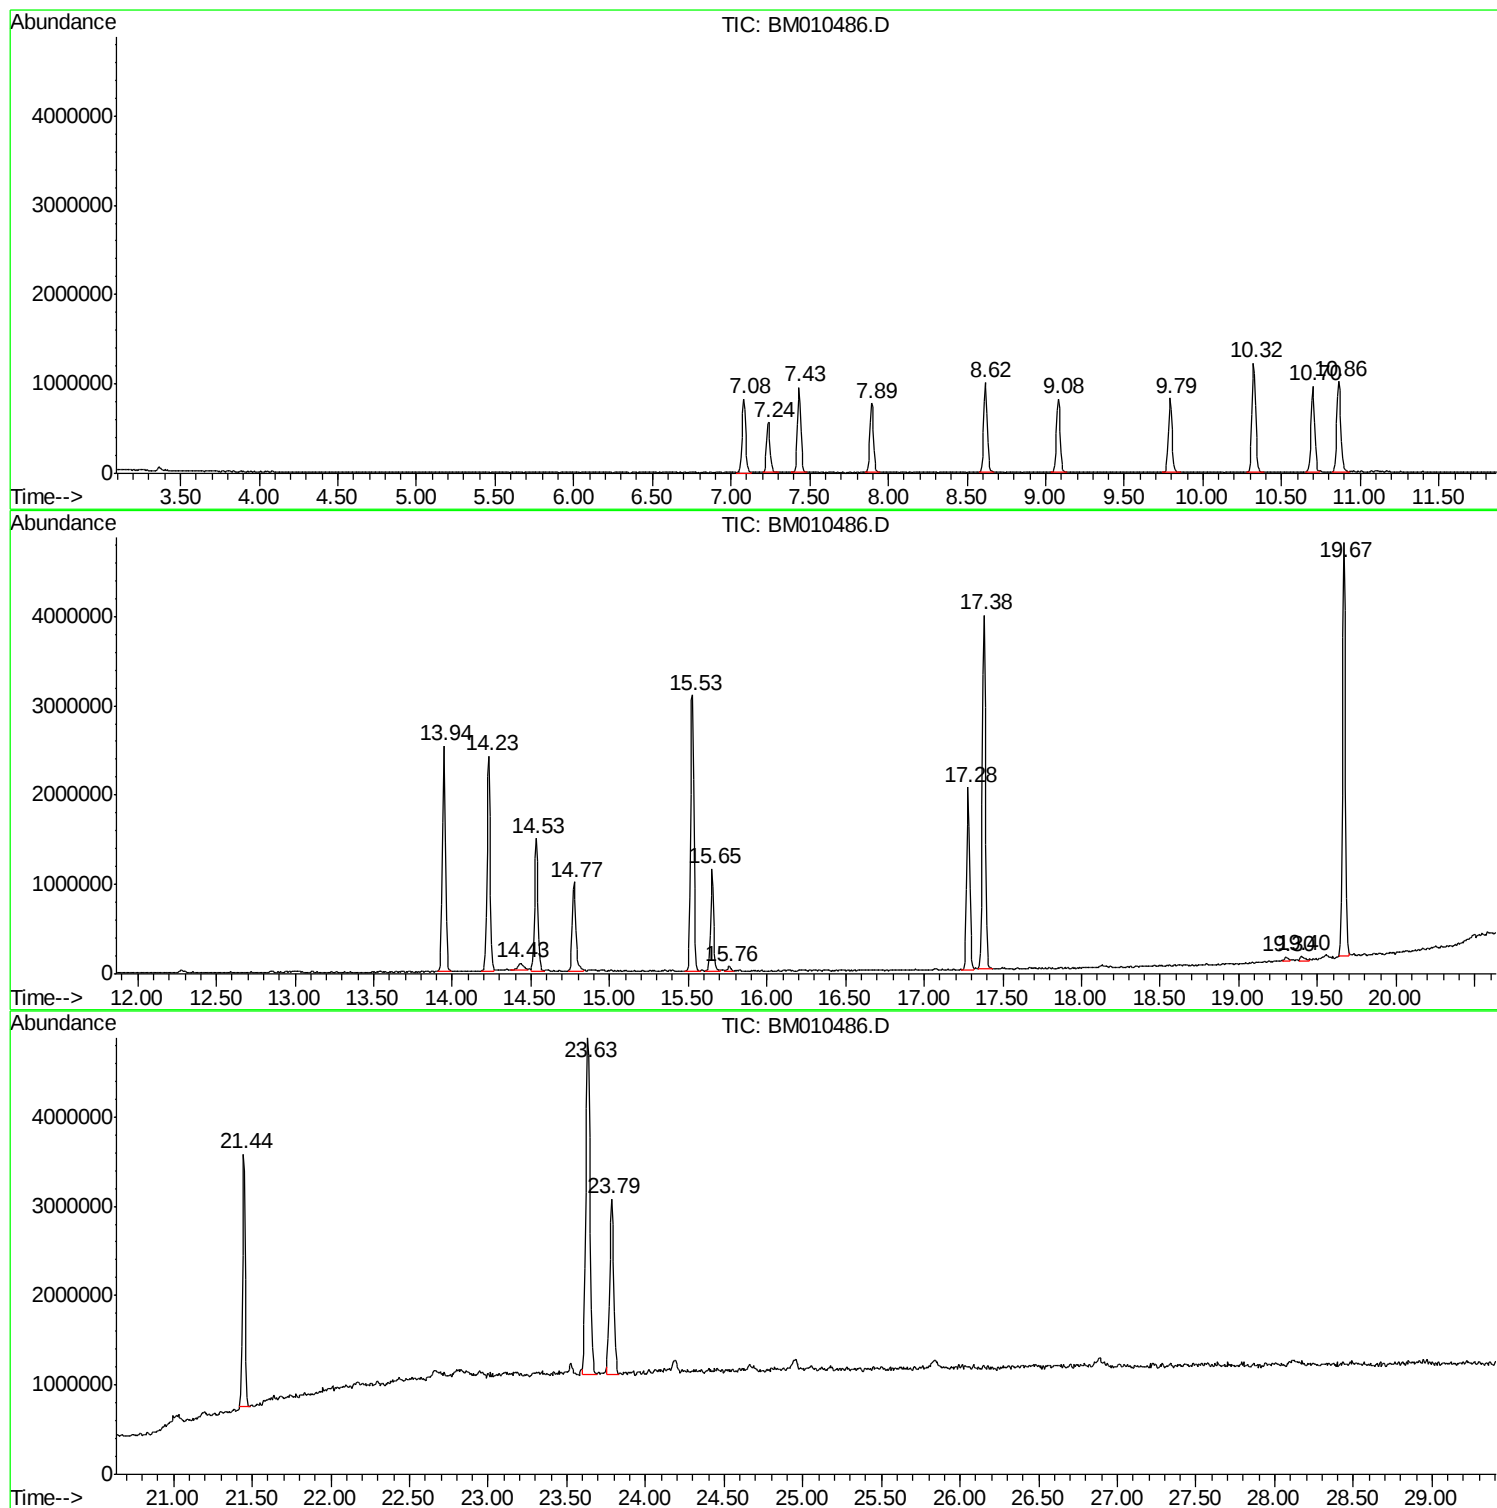

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010486.D
Acq On : 10 Jun 2017 15:34
Operator : SJ/MA
Sample : PB99638BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK38

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010486.D
Acq On : 10 Jun 2017 15:34
Operator : SJ/MA
Sample : PB99638BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK38

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
