

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
 Data File : BM010496.D
 Acq On : 10 Jun 2017 21:35
 Operator : SJ/MA
 Sample : I3522-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5D36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.081	671	679	689	rBV	385558	694232	16.39%	1.702%
2	7.234	700	705	713	rBV	277291	418959	9.89%	1.027%
3	7.434	731	739	748	rBV	465547	736368	17.39%	1.805%
4	7.892	808	817	827	rBV	747940	1214367	28.68%	2.977%
5	8.616	934	940	948	rBV	500803	788691	18.62%	1.933%
6	9.081	1013	1019	1026	rBV	393094	640977	15.14%	1.571%
7	9.792	1131	1140	1150	rBV2	354112	637307	15.05%	1.562%
8	10.322	1222	1230	1242	rBV	595784	1014838	23.97%	2.488%
9	10.698	1284	1294	1300	rBV	894920	1533283	36.21%	3.759%
10	10.863	1315	1322	1333	rBV	467754	834723	19.71%	2.046%
11	13.945	1840	1846	1850	rBV	1116937	1557505	36.78%	3.818%
12	13.992	1850	1854	1862	rVB	919405	1188192	28.06%	2.913%
13	14.227	1887	1894	1904	rBV	1094042	1614694	38.13%	3.958%
14	14.433	1923	1929	1938	rBV4	54440	125743	2.97%	0.308%
15	14.533	1939	1946	1953	rVB2	1421719	2178447	51.44%	5.340%
16	14.774	1981	1987	1994	rBV	358134	622954	14.71%	1.527%
17	15.521	2106	2114	2120	rBV	1469762	2160227	51.01%	5.296%
18	15.651	2130	2136	2145	rBV	429200	660623	15.60%	1.619%
19	17.280	2407	2413	2419	rBV	2061907	2873555	67.86%	7.044%
20	17.374	2424	2429	2441	rVB	1630622	2461172	58.12%	6.033%
21	17.603	2465	2468	2475	rBV9	19587	43472	1.03%	0.107%
22	18.121	2552	2556	2563	rBV4	177919	257943	6.09%	0.632%
23	19.327	2758	2761	2767	rVB	169482	226291	5.34%	0.555%
24	19.397	2769	2773	2780	rBV7	144706	218503	5.16%	0.536%
25	19.668	2811	2819	2829	rBV	2391894	3481008	82.20%	8.533%
26	19.809	2839	2843	2847	rVB7	54857	80249	1.90%	0.197%
27	21.444	3116	3121	3125	rBV	3429444	4234610	100.00%	10.381%
28	23.633	3487	3493	3507	rVB2	2055667	4145892	97.90%	10.163%
29	23.780	3512	3518	3527	rVV	2058072	4147519	97.94%	10.167%


Sum of corrected areas: 40792344

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010496.D
Acq On : 10 Jun 2017 21:35
Operator : SJ/MA
Sample : I3522-20
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5D36

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

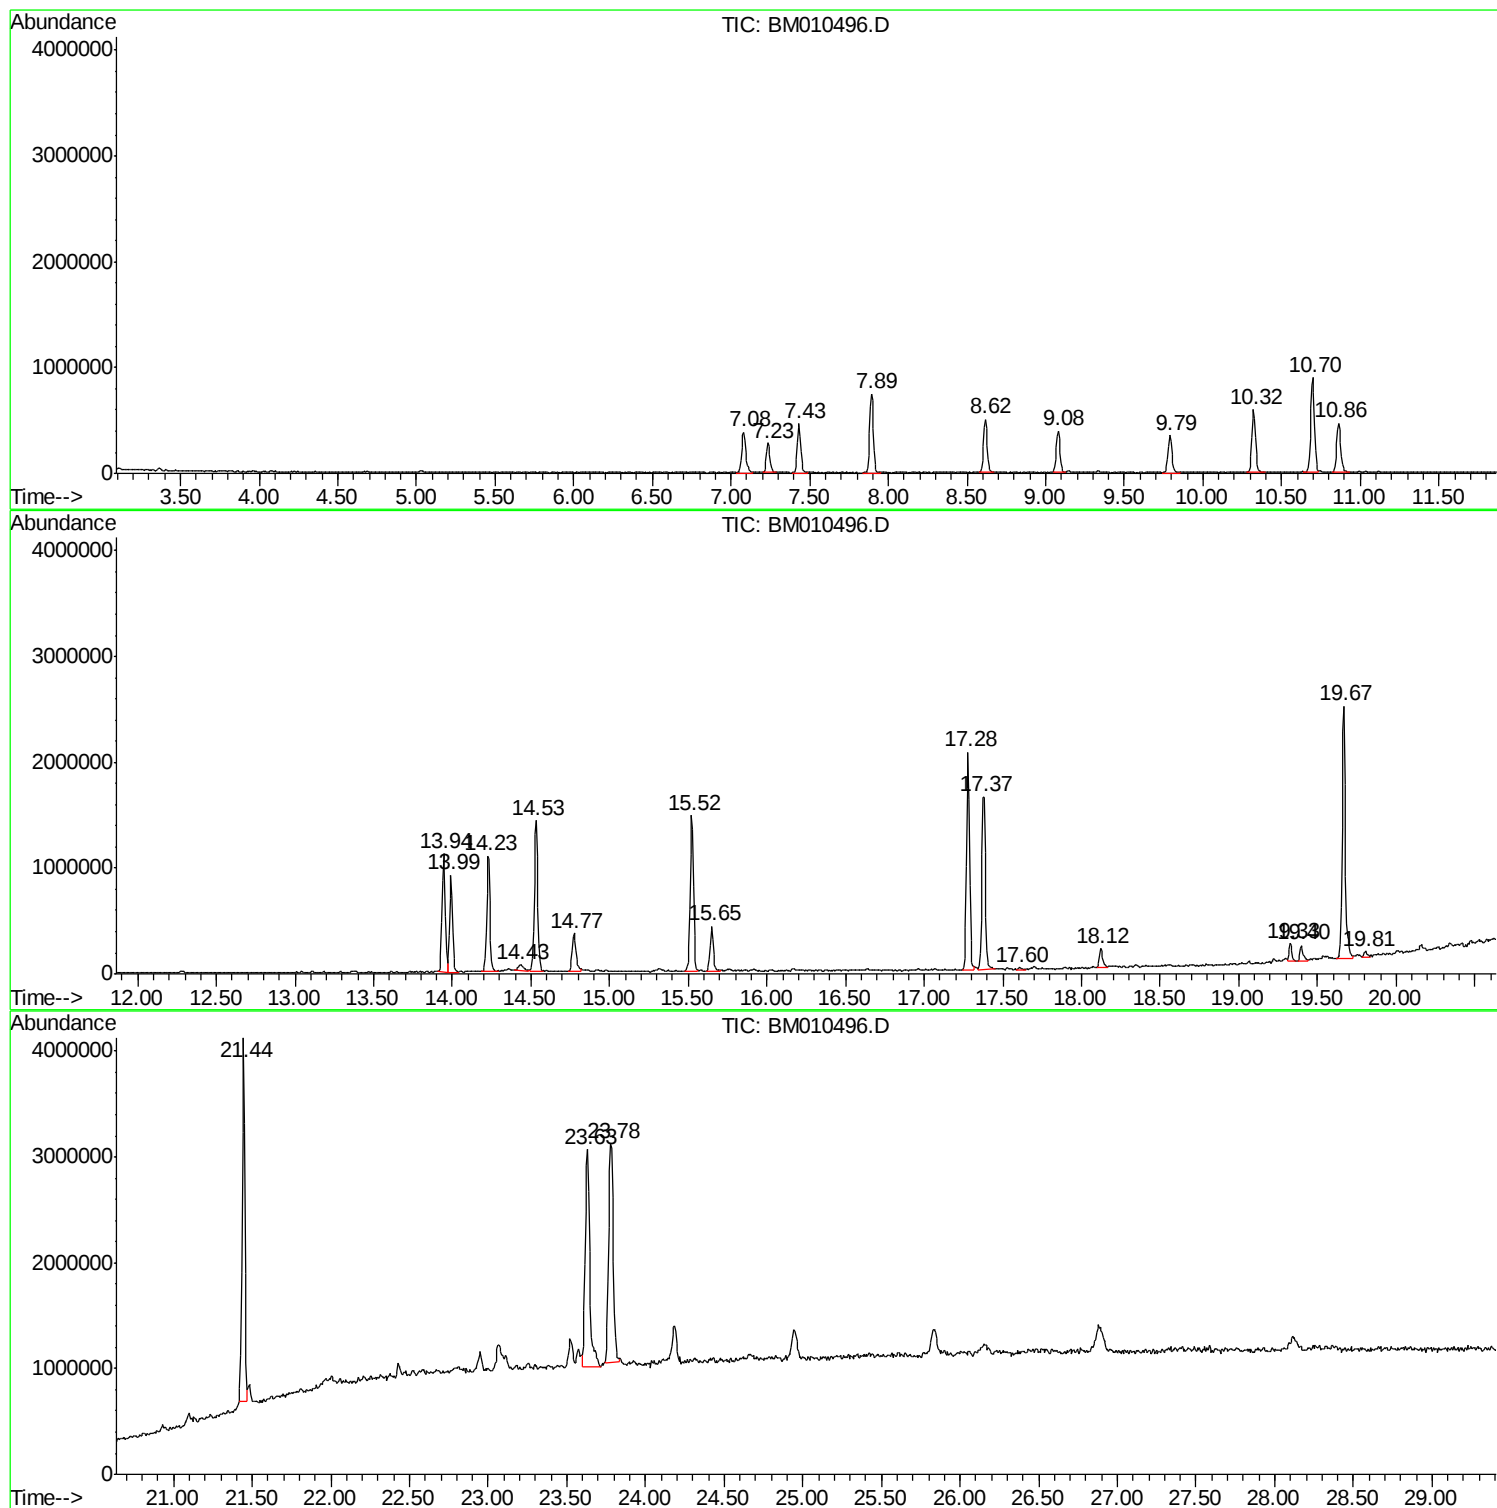

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010496.D
Acq On : 10 Jun 2017 21:35
Operator : SJ/MA
Sample : I3522-20
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5D36

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061017\
Data File : BM010496.D
Acq On : 10 Jun 2017 21:35
Operator : SJ/MA
Sample : I3522-20
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5D36

Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc