

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026325.D
 Acq On : 10 Jun 2020 12:08
 Operator : JU/CG
 Sample : L2933-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH7

Quant Time: Jun 10 12:43:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 10 10:35:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	149649	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	588160	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.07	164	326954	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.83	188	646438	20.00	ng/ul	0.00
78) Chrysene-d12	21.04	240	615308	20.00	ng/ul	0.00
86) Perylene-d12	23.14	264	653704	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.00	96	22146	4.46	ng/uL	0.00
5) Phenol-d5	6.63	99	71592	5.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.77	67	203671	21.69	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	197074	18.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	127080	12.42	ng/ul	0.00
19) Nitrobenzene-d5	8.57	128	117747	24.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	127332	26.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	206062	21.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.34	131	28349	2.93	ng/ul	0.01
44) Dimethylphthalate-d6	13.50	166	661561	25.23	ng/ul	0.00
47) Acenaphthylene-d8	13.76	160	781043	25.14	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	16109	3.47	ng/ul	0.01
58) Fluorene-d10	15.08	176	578844	25.38	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.22	200	92685	24.59	ng/ul	0.00
71) Anthracene-d10	16.93	188	900772	28.28	ng/ul	0.00
79) Pyrene-d10	19.23	212	969414	30.67	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.01	264	849857	24.43	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.54	163	128237	4.659	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
Data File : BM026325.D
Acq On : 10 Jun 2020 12:08
Operator : JU/CG
Sample : L2933-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH7

Quant Time: Jun 10 12:43:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 10 10:35:18 2020
Response via : Initial Calibration

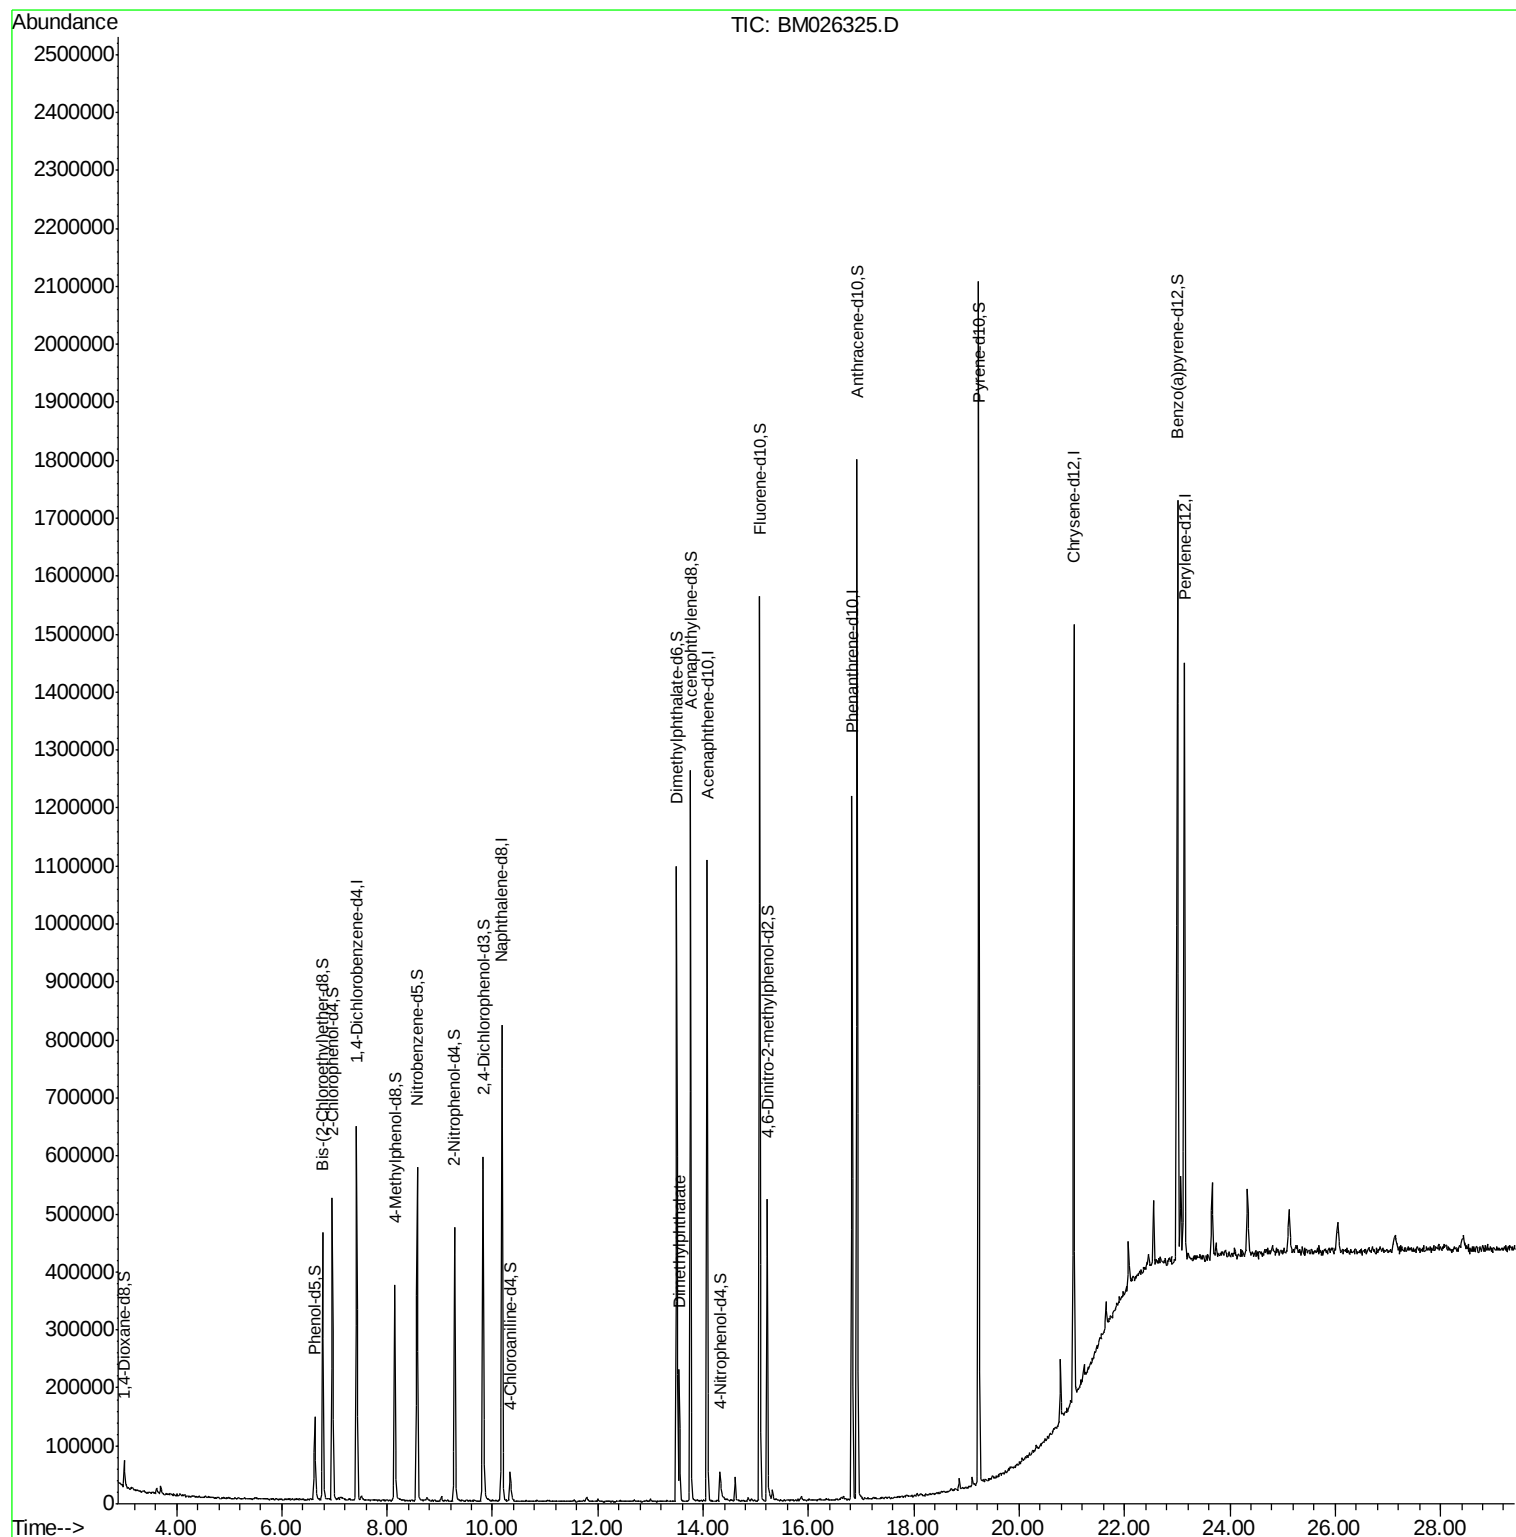

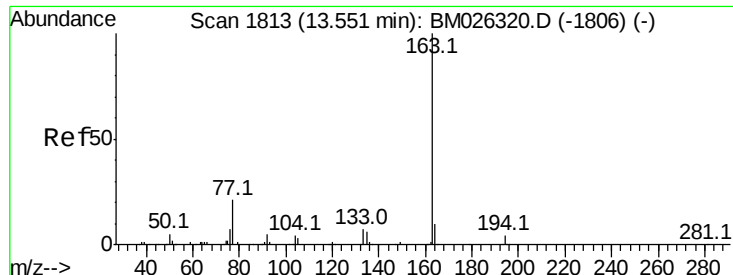

#45

Dimethylphthalate

Concen: 4.659 ng/ul

RT: 13.54 min Scan# 1812

Delta R.T. -0.01 min

Lab File: BM026325.D

Acq: 10 Jun 2020 12:08

Instrument :

BNA_M

ClientSampleId :

C0AH7


Tot Ion:163 Resp: 128237

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 10.1 8.2 12.4

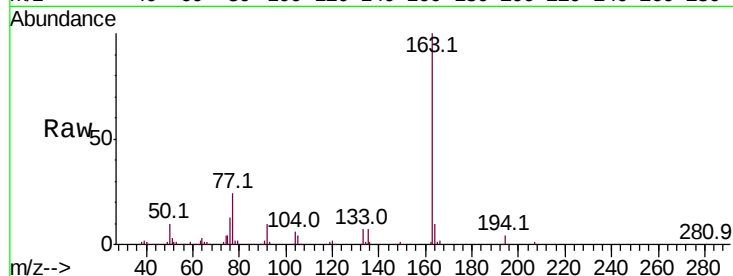

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

