

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026326.D
 Acq On : 10 Jun 2020 12:45
 Operator : JU/CG
 Sample : L2933-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH3

Quant Time: Jun 10 13:22:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 10 10:35:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	150548	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	612240	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.07	164	355445	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.83	188	704409	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	609896	20.00	ng/ul	0.00
86) Perylene-d12	23.13	264	621061	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.00	96	22509	4.51	ng/uL	0.00
5) Phenol-d5	6.63	99	101416	7.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	272621	28.86	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	263721	24.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	178335	17.33	ng/ul	0.00
19) Nitrobenzene-d5	8.57	128	159101	31.88	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	176575	35.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	282944	28.54	ng/ul	0.00
29) 4-Chloroaniline-d4	10.34	131	28663	2.85	ng/ul	0.01
44) Dimethylphthalate-d6	13.50	166	935551	32.82	ng/ul	0.00
47) Acenaphthylene-d8	13.76	160	1102132	32.64	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	24711	4.90	ng/ul	0.00
58) Fluorene-d10	15.07	176	810381	32.69	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.22	200	132689	32.31	ng/ul	0.00
71) Anthracene-d10	16.93	188	1209821	34.85	ng/ul	0.00
79) Pyrene-d10	19.23	212	1260365	40.23	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	1121103	33.91	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.55	163	160777	5.372	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
Data File : BM026326.D
Acq On : 10 Jun 2020 12:45
Operator : JU/CG
Sample : L2933-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH3

Quant Time: Jun 10 13:22:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 10 10:35:18 2020
Response via : Initial Calibration

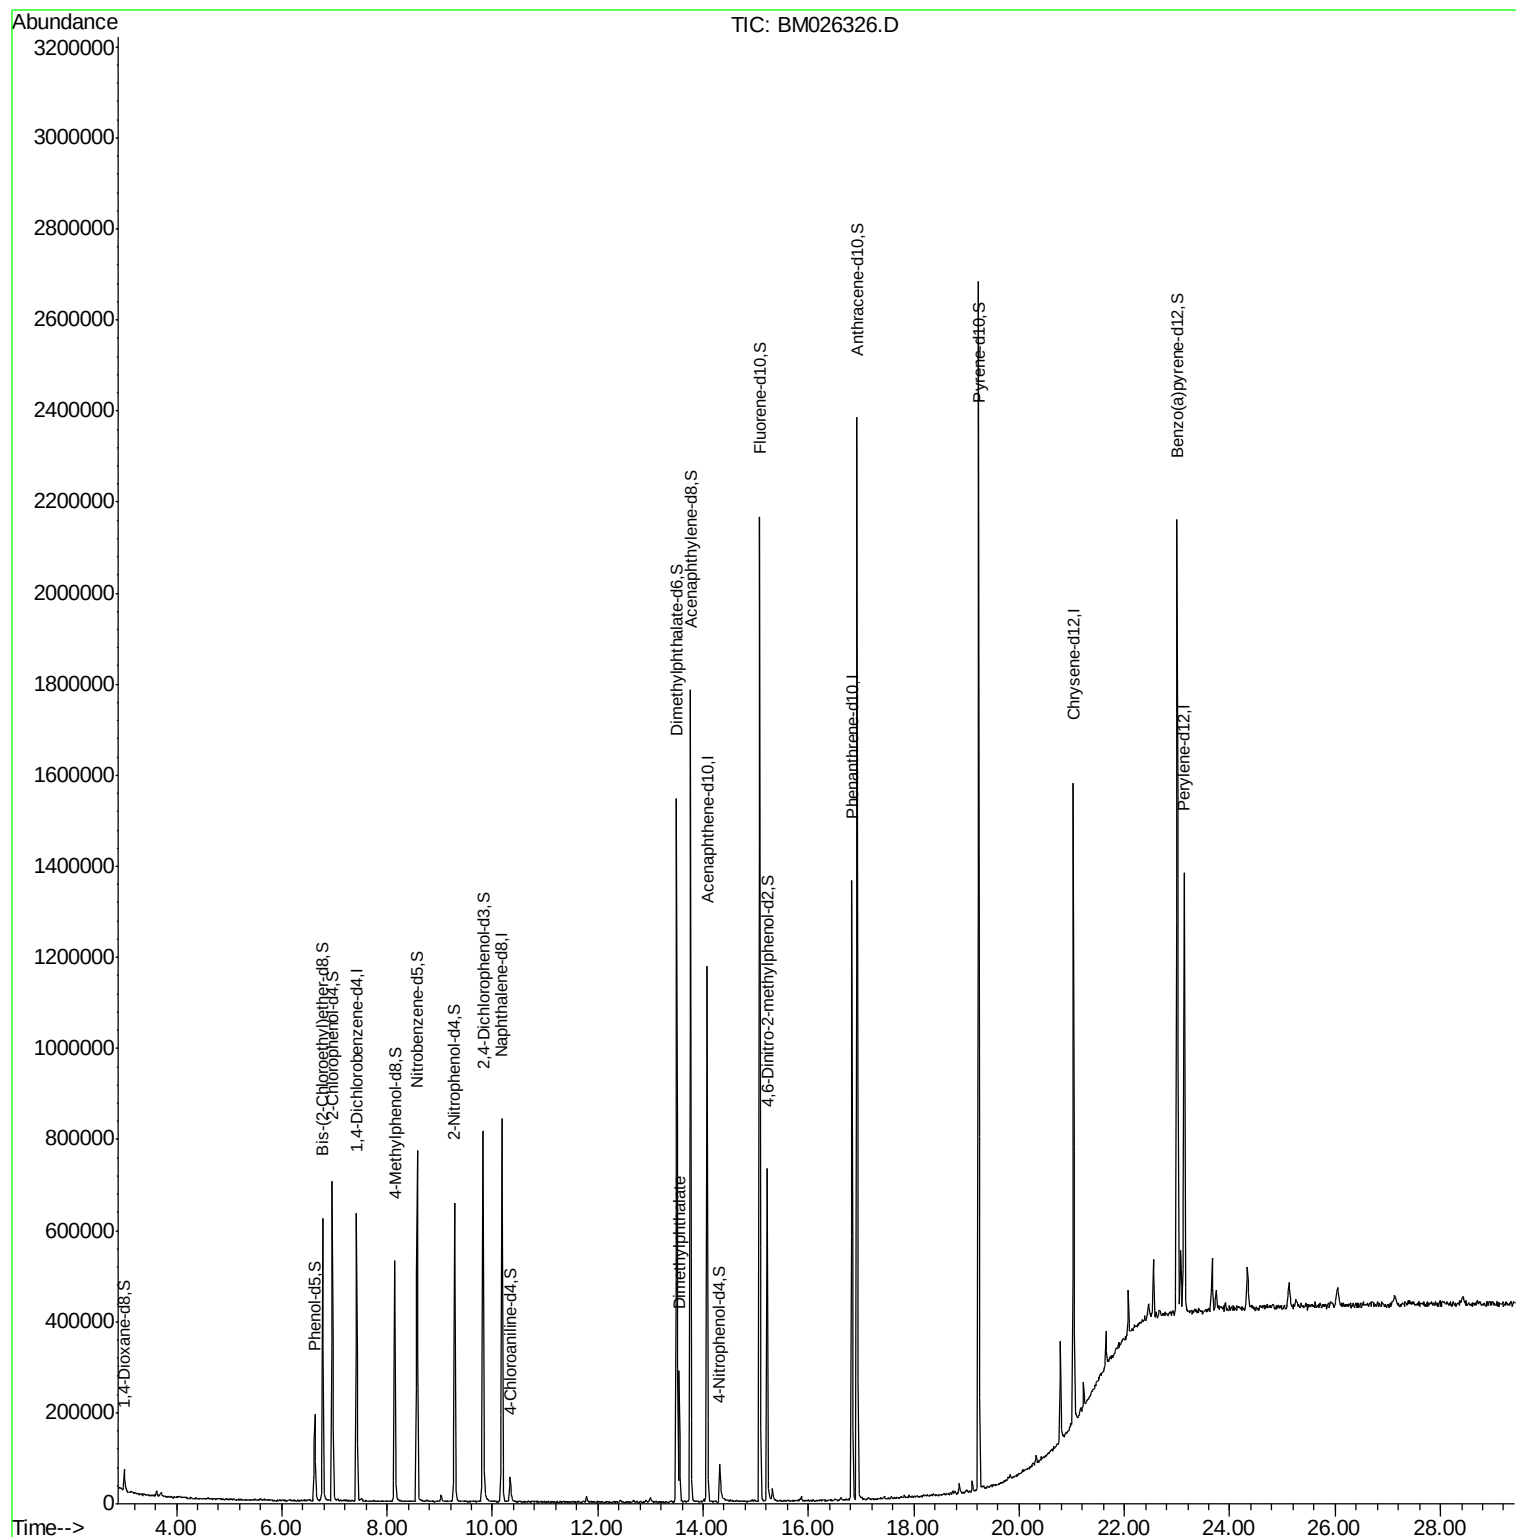

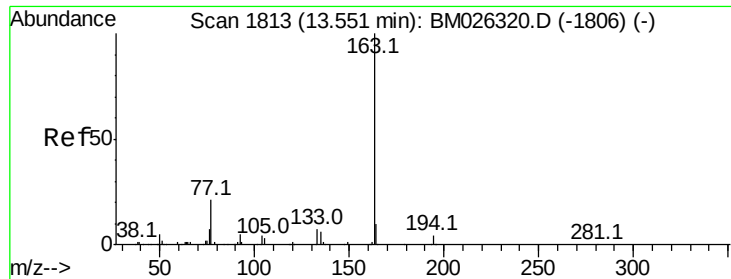

#45

Dimethylphthalate

Concen: 5.372 ng/ul

RT: 13.55 min Scan# 1812

Delta R.T. -0.01 min

Lab File: BM026326.D

Acq: 10 Jun 2020 12:45

Instrument :

BNA_M

ClientSampleId :

C0AH3


Tot Ion:163 Resp: 160777

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.6 8.2 12.4

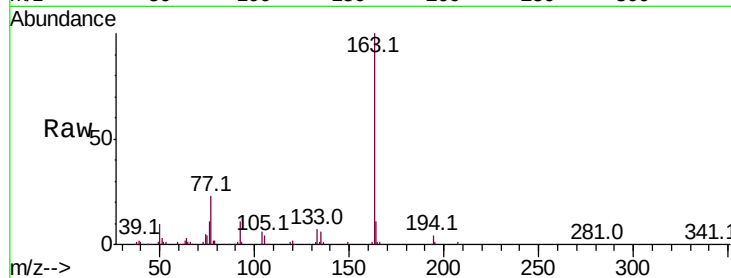

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

