

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026330.D
 Acq On : 10 Jun 2020 15:11
 Operator : JU/CG
 Sample : L2906-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF8

Quant Time: Jun 10 16:03:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 10 10:35:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	159285	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	622136	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.07	164	336315	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.83	188	648291	20.00	ng/ul	0.00
78) Chrysene-d12	21.04	240	622445	20.00	ng/ul	0.00
86) Perylene-d12	23.13	264	658520	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.00	96	21038	3.98	ng/uL	0.00
5) Phenol-d5	6.63	99	75514	5.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	229907	23.00	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	224120	19.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	143171	13.15	ng/ul	0.00
19) Nitrobenzene-d5	8.57	128	132216	26.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	148469	29.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	253625	25.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.34	131	9715	0.95	ng/ul	0.01
44) Dimethylphthalate-d6	13.50	166	782668	29.02	ng/ul	0.00
47) Acenaphthylene-d8	13.76	160	948253	29.68	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	18587	3.89	ng/ul	0.01
58) Fluorene-d10	15.08	176	676276	28.83	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.22	200	112829	29.85	ng/ul	0.00
71) Anthracene-d10	16.93	188	960828	30.08	ng/ul	0.00
79) Pyrene-d10	19.23	212	1048904	32.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	1006666	28.72	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.55	163	124770	4.406	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
Data File : BM026330.D
Acq On : 10 Jun 2020 15:11
Operator : JU/CG
Sample : L2906-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF8

Quant Time: Jun 10 16:03:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 10 10:35:18 2020
Response via : Initial Calibration

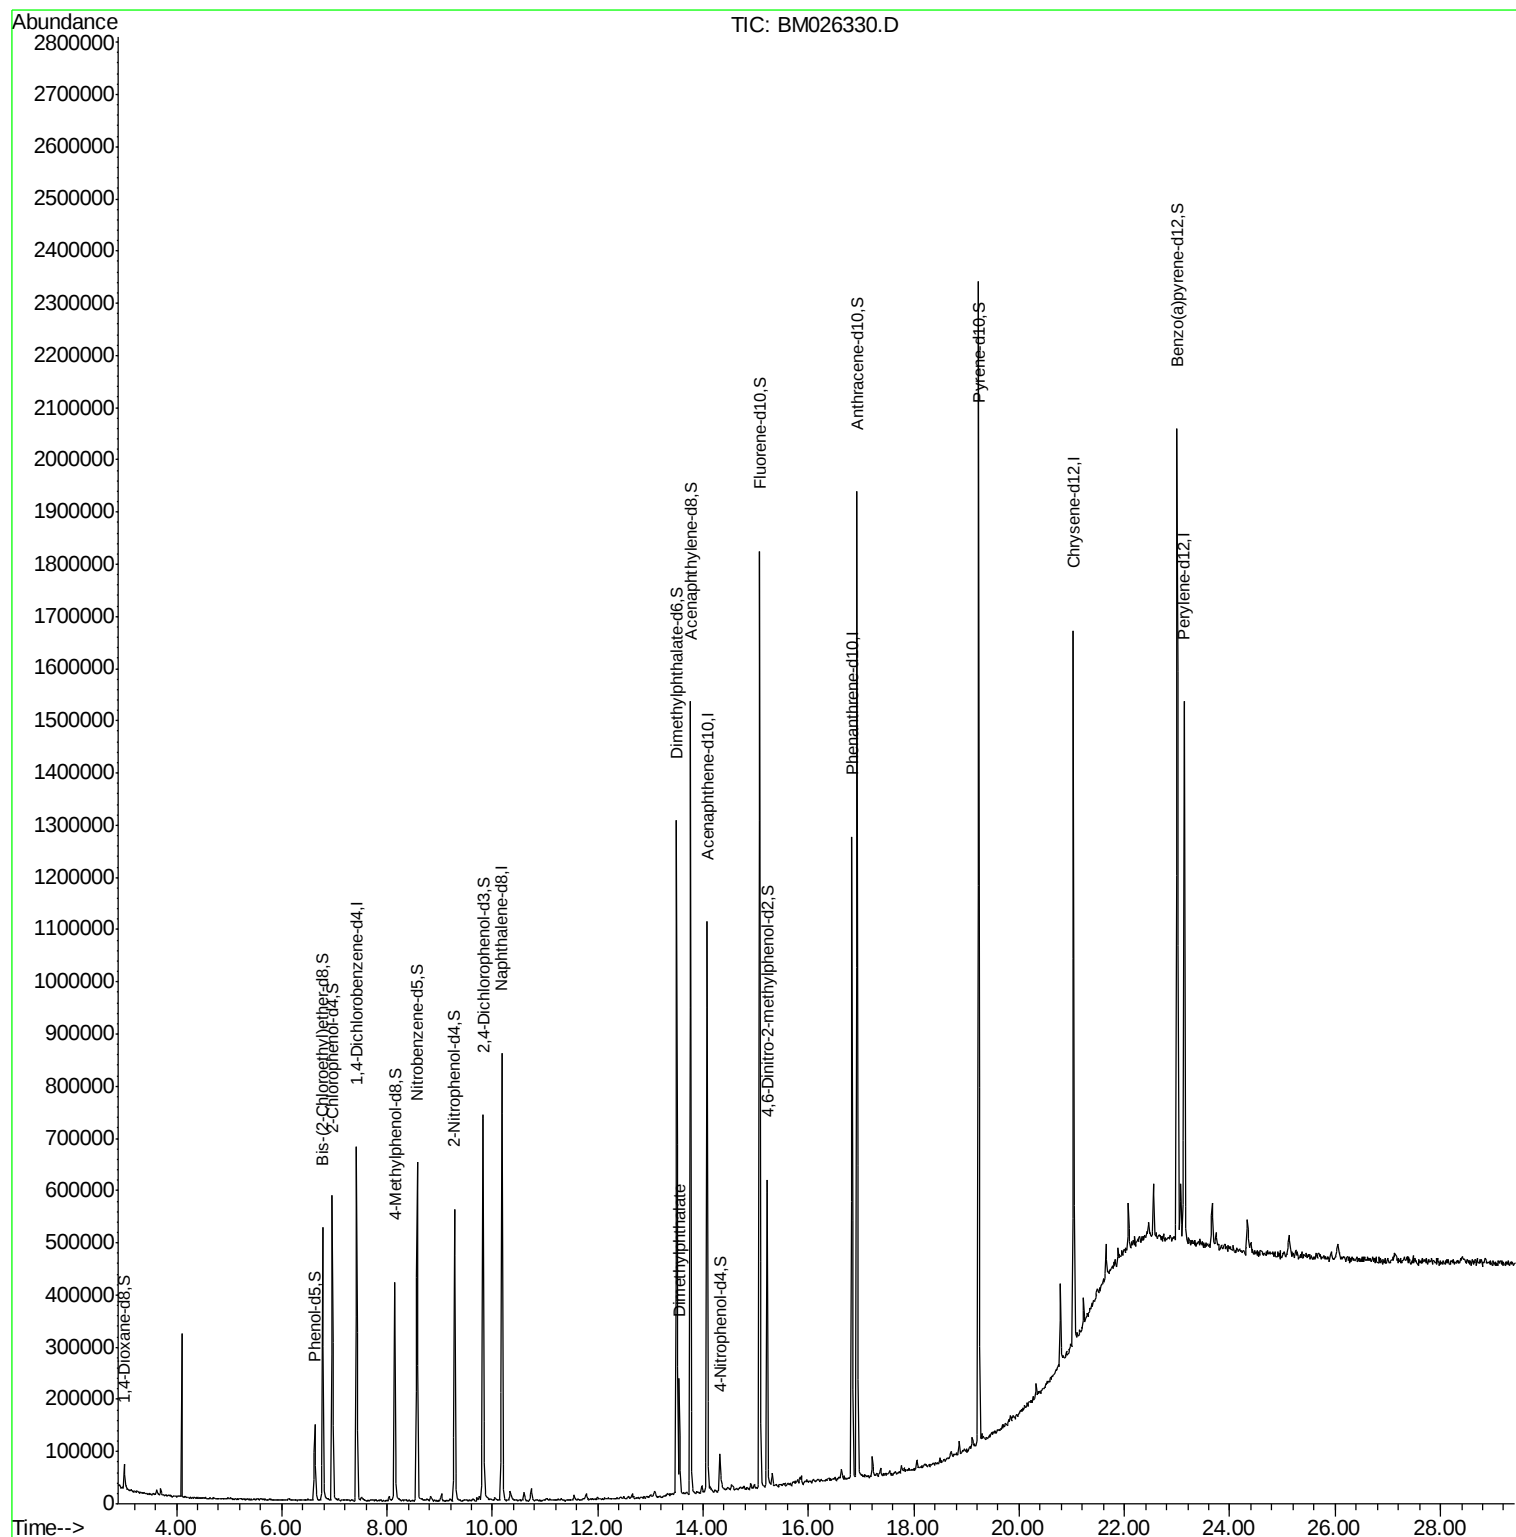

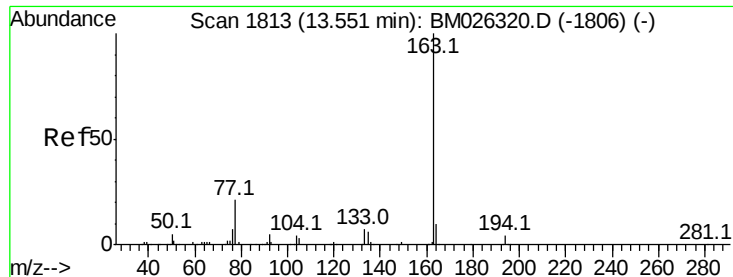

#45

Dimethylphthalate

Concen: 4.406 ng/ul

RT: 13.55 min Scan# 1812

Delta R.T. -0.01 min

Lab File: BM026330.D

Acq: 10 Jun 2020 15:11

Instrument :

BNA_M

ClientSampleId :

C0AF8

Tot Ion:163 Resp: 124770

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 10.3 8.2 12.4

