

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026332.D
 Acq On : 10 Jun 2020 16:24
 Operator : JU/CG
 Sample : L2933-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH3

Quant Time: Jun 10 17:05:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 10 10:35:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	162139	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	667937	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.07	164	393841	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.83	188	762257	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	661915	20.00	ng/ul	0.00
86) Perylene-d12	23.14	264	668149	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.00	96	15993	2.98	ng/uL	0.00
5) Phenol-d5	6.63	99	335832	22.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	221205	21.74	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	250911	21.80	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	284330	25.65	ng/ul	0.00
19) Nitrobenzene-d5	8.57	128	133592	24.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	148454	27.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	262656	24.29	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	367707	33.52	ng/ul	0.00
44) Dimethylphthalate-d6	13.50	166	873684	27.66	ng/ul	0.00
47) Acenaphthylene-d8	13.76	160	1019521	27.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.31	143	128181	22.92	ng/ul	0.00
58) Fluorene-d10	15.07	176	742268	27.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.22	200	124810	28.08	ng/ul	0.00
71) Anthracene-d10	16.93	188	1153574	30.71	ng/ul	0.00
79) Pyrene-d10	19.23	212	1220331	35.89	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.01	264	1122392	31.56	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.55	163	268676	8.103	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
Data File : BM026332.D
Acq On : 10 Jun 2020 16:24
Operator : JU/CG
Sample : L2933-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH3

Quant Time: Jun 10 17:05:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 10 10:35:18 2020
Response via : Initial Calibration

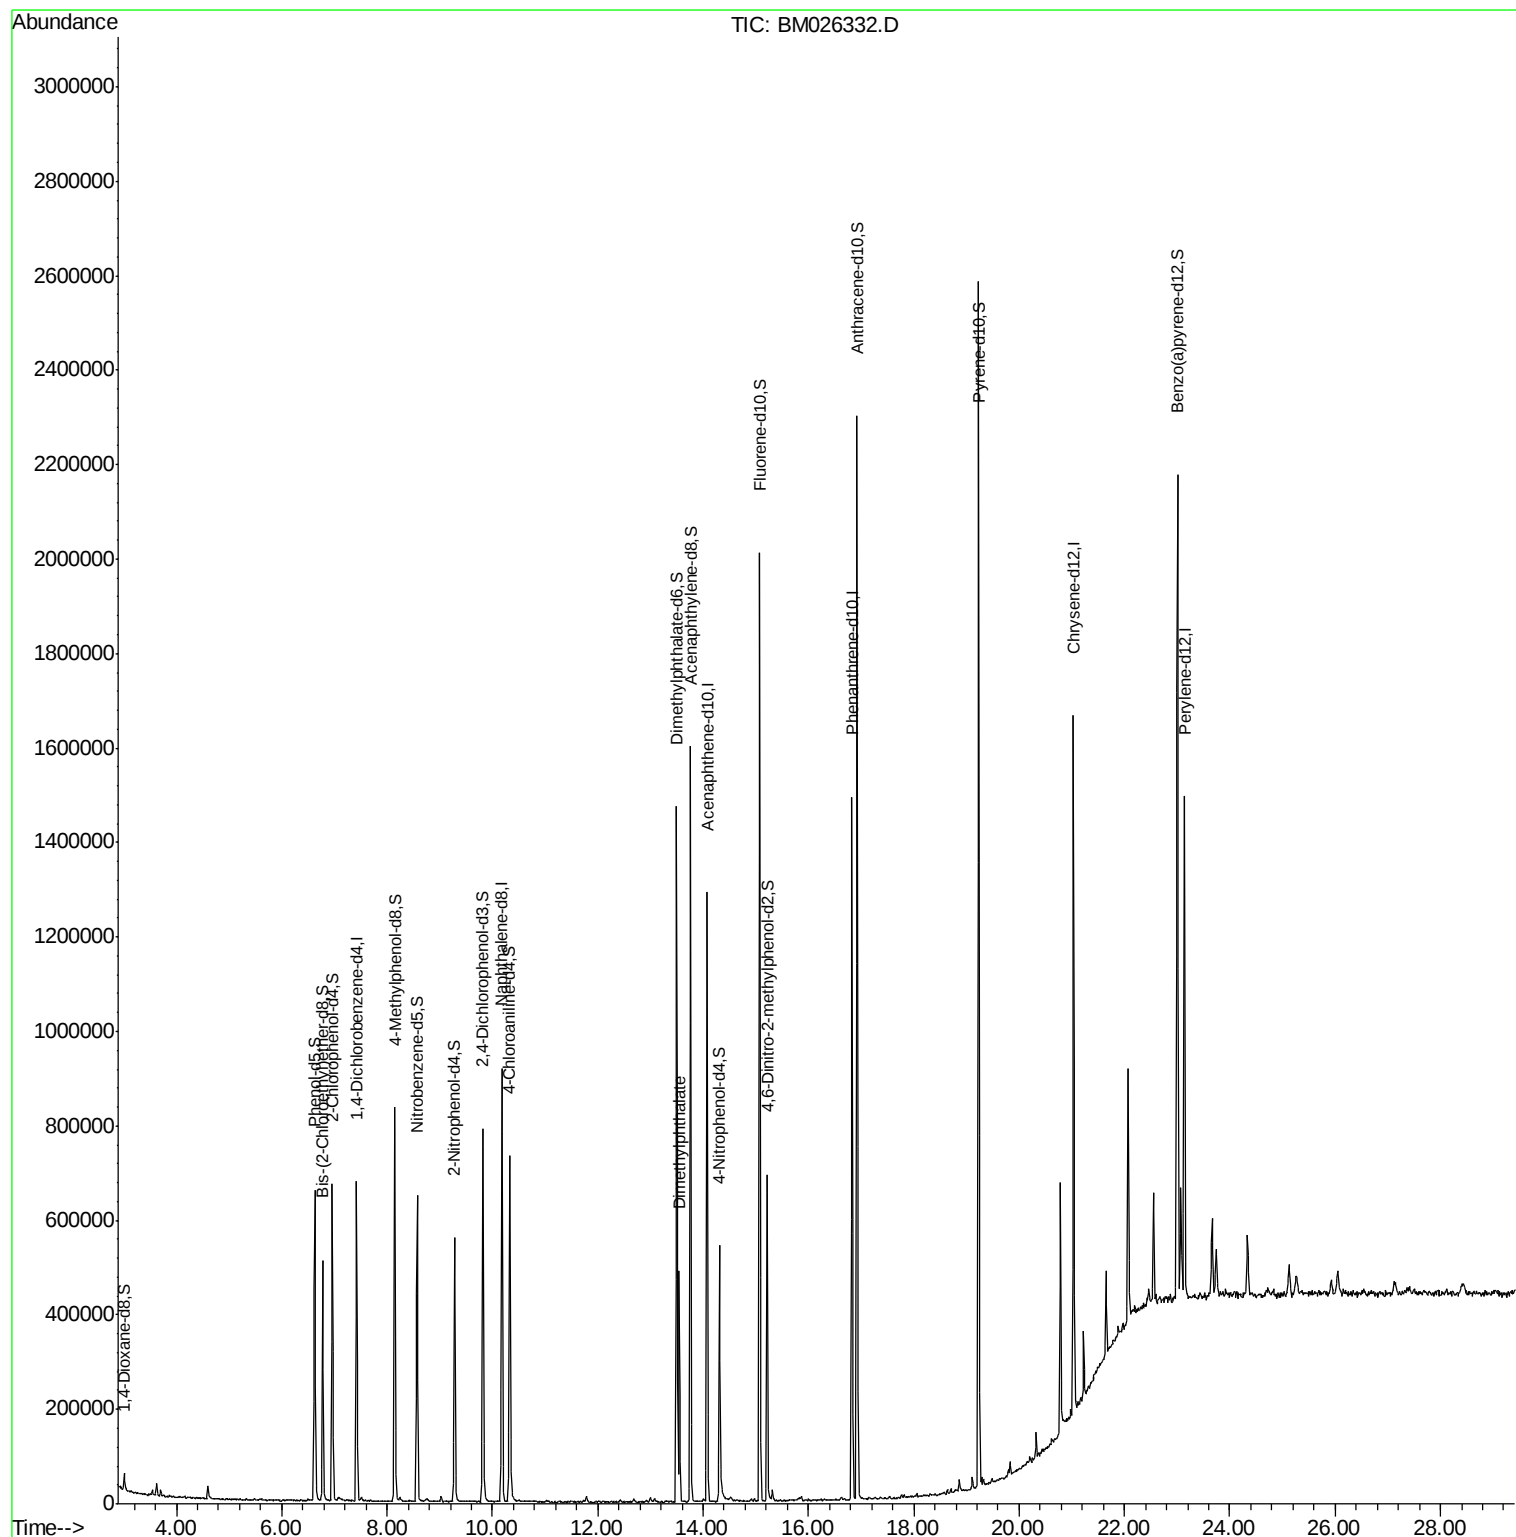

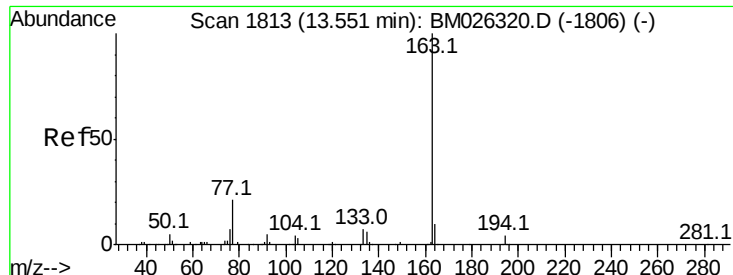

#45

Dimethylphthalate

Concen: 8.103 ng/ul

RT: 13.55 min Scan# 1812

Delta R.T. -0.01 min

Lab File: BM026332.D

Acq: 10 Jun 2020 16:24

Instrument :

BNA_M

ClientSampleId :

C0AH3


Tot Ion:163 Resp: 268676

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 10.6 8.2 12.4

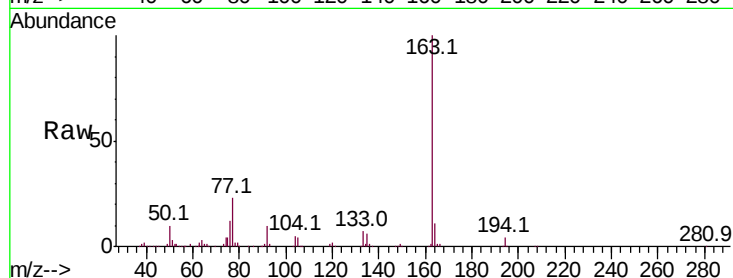

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

