

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026333.D
 Acq On : 10 Jun 2020 17:01
 Operator : JU/CG
 Sample : L2884-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFXD7

Quant Time: Jun 10 17:35:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 10 10:35:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	164614	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	644751	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.07	164	363489	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.83	188	737708	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	739664	20.00	ng/ul	0.00
86) Perylene-d12	23.14	264	770175	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.00	96	26117	4.79	ng/uL	0.00
5) Phenol-d5	6.62	99	90818	6.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	258659	25.04	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	253697	21.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	162686	14.46	ng/ul	0.00
19) Nitrobenzene-d5	8.57	128	147386	28.04	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	165986	31.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	268903	25.76	ng/ul	0.00
29) 4-Chloroaniline-d4	10.34	131	13713	1.30	ng/ul	0.01
44) Dimethylphthalate-d6	13.50	166	830880	28.50	ng/ul	0.00
47) Acenaphthylene-d8	13.76	160	1003387	29.06	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	26080	5.05	ng/ul	0.01
58) Fluorene-d10	15.07	176	710955	28.04	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.22	200	126092	29.31	ng/ul	0.00
71) Anthracene-d10	16.93	188	1055747	29.04	ng/ul	0.00
79) Pyrene-d10	19.23	212	1161034	30.56	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	1175720	28.68	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.55	163	149414	4.882	ng/ul	99
65) N-Nitrosodiphenylamine	15.35	169	72167	2.919	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
Data File : BM026333.D
Acq On : 10 Jun 2020 17:01
Operator : JU/CG
Sample : L2884-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFXD7

Quant Time: Jun 10 17:35:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 10 10:35:18 2020
Response via : Initial Calibration




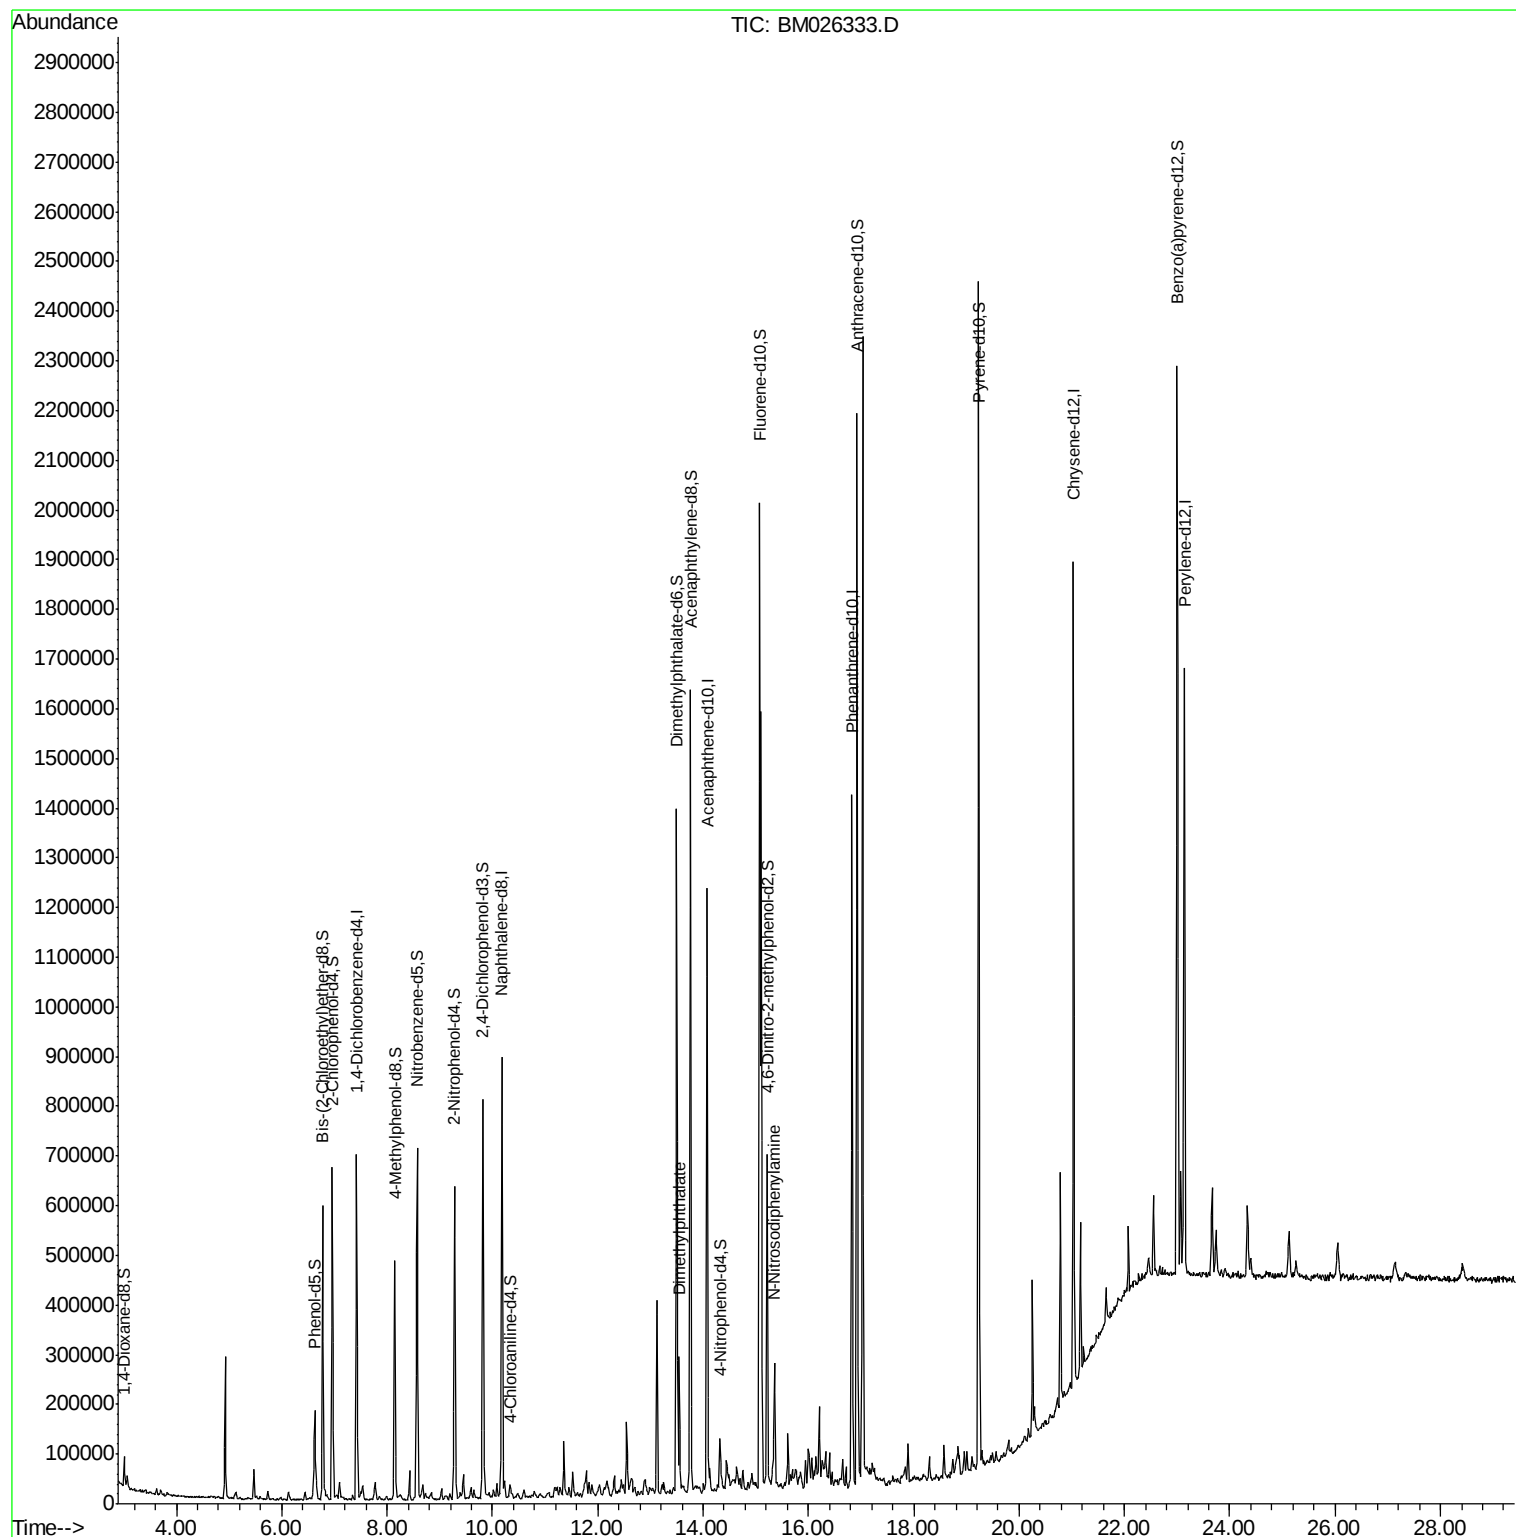


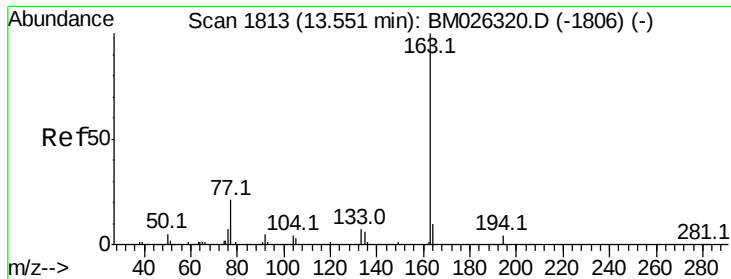

#45
 Dimethylphthalate
 Concen: 4.882 ng/ul
 RT: 13.55 min Scan# 1812
 Delta R.T. -0.01 min
 Lab File: BM026333.D
 Acq: 10 Jun 2020 17:01

Instrument :
 BNA_M
 ClientSampleId :
 BFXD7

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.8	3.5	5.3
164	10.1	8.2	12.4

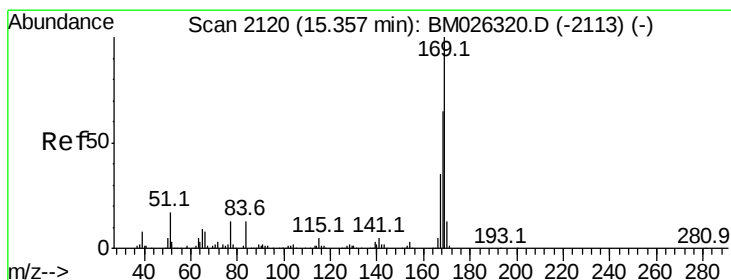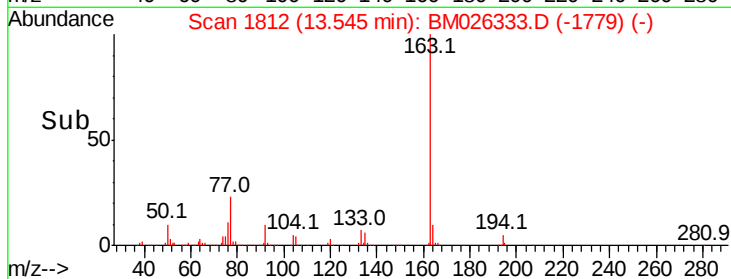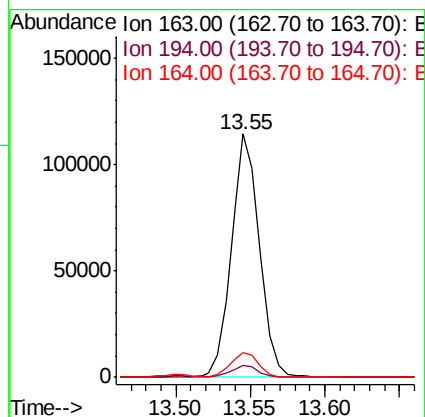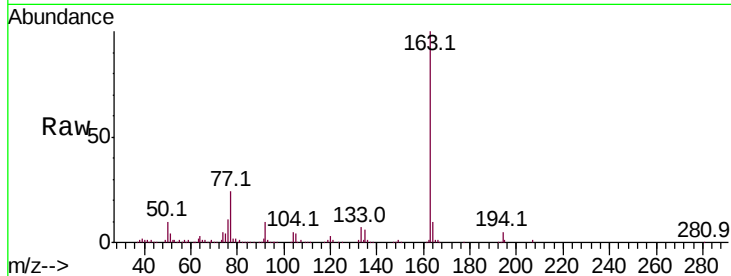

#65
 N-Nitrosodiphenylamine
 Concen: 2.919 ng/ul
 RT: 15.35 min Scan# 2119
 Delta R.T. -0.01 min
 Lab File: BM026333.D
 Acq: 10 Jun 2020 17:01

Tgt Ion	Ratio	Lower	Upper
169	100		
168	62.7	52.2	78.4
167	35.5	28.6	42.8

