

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026325.D
 Acq On : 10 Jun 2020 12:08
 Operator : JU/CG
 Sample : L2933-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.004	17	20	30	rVB	46833	67917	2.55%	0.239%
2	3.622	121	125	130	rVB2	8513	12343	0.46%	0.043%
3	3.704	135	139	146	rVB	13263	19585	0.73%	0.069%
4	4.069	196	201	206	rBV7	3708	7334	0.27%	0.026%
5	6.628	629	636	647	rBV	144392	248886	9.33%	0.875%
6	6.775	655	661	674	rBV	460567	699869	26.23%	2.462%
7	6.963	687	693	704	rBV	520732	800837	30.01%	2.817%
8	7.075	709	712	715	rVB5	3610	3619	0.14%	0.013%
9	7.104	715	717	718	rBV2	2897	2745	0.10%	0.010%
10	7.139	721	723	726	rVB3	3392	3563	0.13%	0.013%
11	7.422	763	771	778	rBV	645404	960181	35.98%	3.377%
12	7.510	783	786	799	rVB6	7116	17024	0.64%	0.060%
13	8.145	888	894	905	rBV	371825	586335	21.97%	2.062%
14	8.569	959	966	978	rBV	574379	924890	34.66%	3.253%
15	8.751	994	997	1002	rVB5	4229	6441	0.24%	0.023%
16	9.033	1040	1045	1052	rVB2	9033	14086	0.53%	0.050%
17	9.281	1081	1087	1098	rBV	472049	751437	28.16%	2.643%
18	9.822	1172	1179	1195	rBV	591963	1029580	38.58%	3.621%
19	10.180	1233	1240	1250	rBV	820538	1281830	48.03%	4.509%
20	10.339	1259	1267	1277	rBV	51168	105663	3.96%	0.372%
21	10.851	1348	1354	1357	rVB6	2219	4217	0.16%	0.015%
22	11.627	1481	1486	1489	rBV5	1866	3145	0.12%	0.011%
23	11.727	1498	1503	1507	rBV5	2672	3375	0.13%	0.012%
24	11.792	1509	1514	1520	rVB3	8279	15957	0.60%	0.056%
25	11.998	1547	1549	1552	rBV2	3184	3370	0.13%	0.012%
26	12.692	1661	1667	1670	rVB5	2586	4331	0.16%	0.015%
27	12.998	1716	1719	1723	rBV4	3926	5907	0.22%	0.021%
28	13.498	1798	1804	1809	rBV	1095145	1491227	55.88%	5.245%
29	13.545	1809	1812	1823	rVB	226525	302730	11.34%	1.065%
30	13.763	1837	1849	1866	rBV	1260570	1802936	67.56%	6.342%
31	13.874	1866	1868	1873	rVB4	2180	3339	0.13%	0.012%
32	14.010	1889	1891	1896	rVB3	2846	3484	0.13%	0.012%
33	14.074	1896	1902	1909	rBV	1106006	1520318	56.97%	5.348%
34	14.121	1909	1910	1915	rVB4	3117	3650	0.14%	0.013%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026325.D
 Acq On : 10 Jun 2020 12:08
 Operator : JU/CG
 Sample : L2933-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	14.321	1937	1944	1956	rBV2	52111	130024	4.87%	0.457%
36	14.468	1968	1969	1974	rVB5	3123	3550	0.13%	0.012%
37	14.510	1974	1976	1981	rBV4	2065	3929	0.15%	0.014%
38	14.610	1987	1993	2001	rBV	41967	53376	2.00%	0.188%
39	14.851	2029	2034	2041	rBV	7273	12377	0.46%	0.044%
40	14.915	2041	2045	2052	rVV6	3861	8112	0.30%	0.029%
41	14.974	2052	2055	2060	rVB3	2864	4073	0.15%	0.014%
42	15.080	2066	2073	2083	rBV	1559359	2213595	82.95%	7.786%
43	15.215	2090	2096	2110	rBV	520088	724063	27.13%	2.547%
44	15.315	2110	2113	2121	rVB	17979	25680	0.96%	0.090%
45	15.657	2169	2171	2174	rBV4	2148	2712	0.10%	0.010%
46	15.804	2192	2196	2198	rBV4	2797	3484	0.13%	0.012%
47	15.862	2198	2206	2211	rBV8	7600	16392	0.61%	0.058%
48	16.333	2281	2286	2288	rBV4	2858	3892	0.15%	0.014%
49	16.515	2314	2317	2320	rVB5	3224	3308	0.12%	0.012%
50	16.621	2331	2335	2338	rBV4	4128	7289	0.27%	0.026%
51	16.662	2338	2342	2345	rVB5	4023	5692	0.21%	0.020%
52	16.827	2364	2370	2377	rBV	1213327	1635477	61.29%	5.753%
53	16.927	2381	2387	2401	rVB	1790496	2422132	90.76%	8.520%
54	17.368	2459	2462	2465	rBV4	2885	3165	0.12%	0.011%
55	18.056	2577	2579	2585	rVB6	3537	4573	0.17%	0.016%
56	18.868	2713	2717	2720	rVB2	18903	22086	0.83%	0.078%
57	19.115	2756	2759	2764	rBV2	16608	23579	0.88%	0.083%
58	19.233	2773	2779	2787	rBV	2069993	2668601	100.00%	9.387%
59	20.792	3040	3044	3048	rBV	103930	133650	5.01%	0.470%
60	21.039	3081	3086	3091	rBV	1335113	1712246	64.16%	6.023%
61	23.009	3415	3421	3427	rVB	1287790	2122630	79.54%	7.466%
62	23.138	3437	3443	3451	rVB	1024750	1748188	65.51%	6.149%


Sum of corrected areas: 28430026

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
Data File : BM026325.D
Acq On : 10 Jun 2020 12:08
Operator : JU/CG
Sample : L2933-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

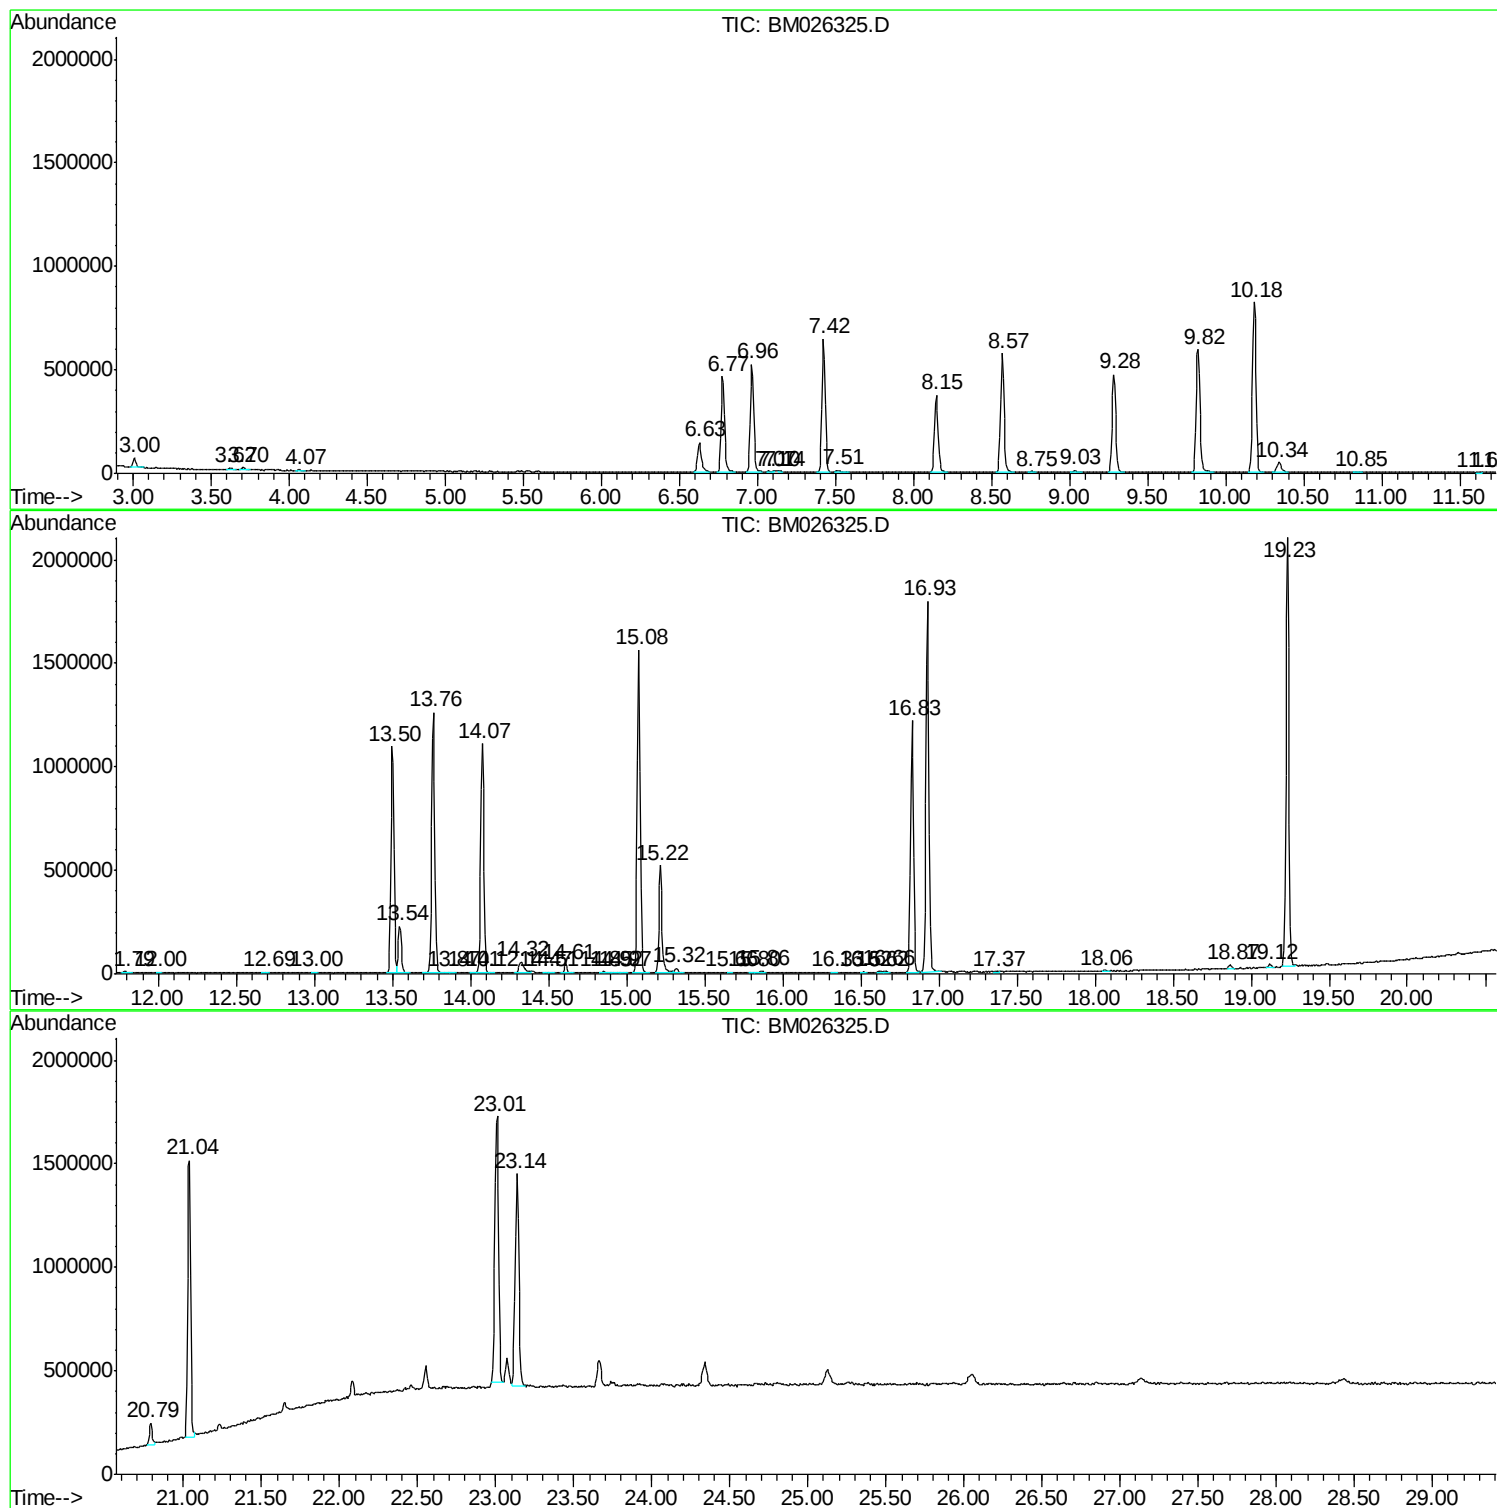

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061020\
Data File : BM026325.D
Acq On : 10 Jun 2020 12:08
Operator : JU/CG
Sample : L2933-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061020\
Data File : BM026325.D
Acq On : 10 Jun 2020 12:08
Operator : JU/CG
Sample : L2933-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc