

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026335.D
 Acq On : 10 Jun 2020 18:15
 Operator : JU/CG
 Sample : PB129318BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK18

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.922	3	6	10	rVB	224317	216389	17.74%	3.242%
2	3.240	57	60	64	rVB	13695	15693	1.29%	0.235%
3	3.699	134	138	143	rVB2	9578	11580	0.95%	0.173%
4	4.163	216	217	220	rVB3	1507	1456	0.12%	0.022%
5	4.246	229	231	233	rBV3	1841	1710	0.14%	0.026%
6	4.322	242	244	248	rVB4	5082	6031	0.49%	0.090%
7	4.481	269	271	273	rVB3	1929	1766	0.14%	0.026%
8	4.505	273	275	276	rBV2	1786	1221	0.10%	0.018%
9	4.528	276	279	281	rBV3	1130	1243	0.10%	0.019%
10	4.622	292	295	296	rBV3	2457	2877	0.24%	0.043%
11	4.787	321	323	326	rVB4	1764	1680	0.14%	0.025%
12	4.863	334	336	338	rBV2	1497	1260	0.10%	0.019%
13	5.263	400	404	406	rVV4	1517	1579	0.13%	0.024%
14	5.875	504	508	509	rBV4	1661	2475	0.20%	0.037%
15	5.975	524	525	529	rBV4	2541	2938	0.24%	0.044%
16	6.110	544	548	549	rBV4	1318	1474	0.12%	0.022%
17	6.199	560	563	565	rBV4	1863	1580	0.13%	0.024%
18	6.222	565	567	570	rVB4	1797	1772	0.15%	0.027%
19	6.604	630	632	635	rVV3	1692	1774	0.15%	0.027%
20	6.751	654	657	658	rBV3	1953	1538	0.13%	0.023%
21	6.769	658	660	663	rBV3	1407	1357	0.11%	0.020%
22	6.793	663	664	669	rBV3	1936	1904	0.16%	0.029%
23	6.957	689	692	697	rBV7	1313	1804	0.15%	0.027%
24	7.034	701	705	708	rBV4	1530	1615	0.13%	0.024%
25	7.169	726	728	732	rBV3	1804	1884	0.15%	0.028%
26	7.257	739	743	747	rVB6	1238	1772	0.15%	0.027%
27	7.293	747	749	752	rBV4	1122	1230	0.10%	0.018%
28	7.416	761	770	782	rBV	512816	808904	66.31%	12.118%
29	7.534	788	790	793	rBV4	1265	1311	0.11%	0.020%
30	7.681	813	815	817	rBV3	1448	1277	0.10%	0.019%
31	7.851	841	844	847	rVB5	1610	1977	0.16%	0.030%
32	7.893	849	851	853	rBV2	1627	1749	0.14%	0.026%
33	7.987	865	867	869	rBV2	1426	1647	0.14%	0.025%
34	8.187	897	901	903	rBV4	1059	1664	0.14%	0.025%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026335.D
 Acq On : 10 Jun 2020 18:15
 Operator : JU/CG
 Sample : PB129318BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK18

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	8.369	929	932	935	rBV4	1215	1676	0.14%	0.025%
36	8.528	958	959	962	rBV2	1764	1562	0.13%	0.023%
37	9.045	1044	1047	1049	rBV3	1073	1414	0.12%	0.021%
38	9.151	1063	1065	1068	rBV4	1918	1310	0.11%	0.020%
39	9.445	1112	1115	1120	rBV4	1155	2202	0.18%	0.033%
40	9.504	1123	1125	1128	rVV3	1560	2069	0.17%	0.031%
41	9.557	1132	1134	1139	rVB5	1529	2159	0.18%	0.032%
42	10.181	1233	1240	1252	rBV	634218	1034529	84.81%	15.498%
43	10.657	1319	1321	1324	rBV4	999	1255	0.10%	0.019%
44	10.898	1356	1362	1365	rBV4	928	1900	0.16%	0.028%
45	11.863	1523	1526	1529	rBV4	1289	1504	0.12%	0.023%
46	12.428	1620	1622	1625	rVB3	1258	1239	0.10%	0.019%
47	12.680	1661	1665	1669	rVV4	964	1348	0.11%	0.020%
48	12.980	1711	1716	1717	rBV3	1296	1727	0.14%	0.026%
49	13.151	1743	1745	1752	rVB5	977	1617	0.13%	0.024%
50	13.398	1785	1787	1790	rVB2	1427	1264	0.10%	0.019%
51	13.810	1855	1857	1860	rVB4	1700	2046	0.17%	0.031%
52	13.869	1864	1867	1868	rBV3	1256	1269	0.10%	0.019%
53	14.075	1896	1902	1912	rBV2	836474	1203694	98.68%	18.033%
54	14.422	1958	1961	1962	rBV3	1189	1225	0.10%	0.018%
55	14.492	1970	1973	1976	rBV3	870	1272	0.10%	0.019%
56	14.974	2049	2055	2059	rBV4	1247	2663	0.22%	0.040%
57	15.027	2063	2064	2068	rBV3	989	1254	0.10%	0.019%
58	15.404	2125	2128	2130	rBV2	933	1291	0.11%	0.019%
59	15.610	2160	2163	2165	rBV4	1326	1538	0.13%	0.023%
60	15.657	2168	2171	2173	rVV2	1692	1629	0.13%	0.024%
61	15.898	2209	2212	2215	rBV5	869	1496	0.12%	0.022%
62	15.992	2224	2228	2229	rBV4	1255	1386	0.11%	0.021%
63	16.027	2233	2234	2238	rVB3	1362	1231	0.10%	0.018%
64	16.068	2238	2241	2243	rBV2	1518	1524	0.12%	0.023%
65	16.498	2309	2314	2315	rBV4	1476	2303	0.19%	0.035%
66	16.539	2318	2321	2322	rBV2	1539	1387	0.11%	0.021%
67	16.616	2331	2334	2338	rBV3	2248	2963	0.24%	0.044%
68	16.827	2364	2370	2384	rBV	868181	1219830	100.00%	18.274%
69	16.933	2384	2388	2389	rVV4	2801	3371	0.28%	0.051%
70	17.021	2401	2403	2406	rBV4	1244	1494	0.12%	0.022%
71	17.115	2416	2419	2420	rBV3	1622	1482	0.12%	0.022%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026335.D
 Acq On : 10 Jun 2020 18:15
 Operator : JU/CG
 Sample : PB129318BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK18

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

72	17.133	2420	2422	2425	rVV3	1711	1655	0.14%	0.025%
73	17.198	2429	2433	2435	rBV5	1979	3014	0.25%	0.045%
74	17.345	2455	2458	2462	rVB5	1927	2841	0.23%	0.043%
75	17.415	2469	2470	2473	rBV3	1629	1482	0.12%	0.022%
76	17.510	2483	2486	2487	rBV3	1795	2078	0.17%	0.031%
77	17.545	2490	2492	2494	rBV3	2187	2442	0.20%	0.037%
78	17.586	2497	2499	2502	rVB3	2368	2442	0.20%	0.037%
79	17.610	2502	2503	2504	rBV	2428	1402	0.11%	0.021%
80	17.768	2529	2530	2533	rBV3	2052	2189	0.18%	0.033%
81	17.874	2546	2548	2551	rBV4	1892	2855	0.23%	0.043%
82	17.921	2554	2556	2558	rBV3	1718	1291	0.11%	0.019%
83	17.951	2558	2561	2564	rBV5	2319	2763	0.23%	0.041%
84	18.362	2629	2631	2633	rBV3	1831	1931	0.16%	0.029%
85	18.404	2636	2638	2640	rVB2	2082	1513	0.12%	0.023%
86	18.462	2645	2648	2649	rBV3	2581	2795	0.23%	0.042%
87	18.521	2652	2658	2659	rBV6	3985	6424	0.53%	0.096%
88	18.551	2662	2663	2664	rBV	2994	1273	0.10%	0.019%
89	18.904	2722	2723	2724	rVB	3756	1326	0.11%	0.020%
90	19.015	2740	2742	2743	rBV2	3708	2595	0.21%	0.039%
91	19.051	2746	2748	2752	rVV5	3269	4446	0.36%	0.067%
92	19.104	2755	2757	2758	rBV	3303	2029	0.17%	0.030%
93	21.033	3080	3085	3091	rBV	794457	1025873	84.10%	15.369%
94	23.133	3437	3442	3448	rVB	579789	975147	79.94%	14.609%


Sum of corrected areas: 6675060

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
Data File : BM026335.D
Acq On : 10 Jun 2020 18:15
Operator : JU/CG
Sample : PB129318BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK18

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

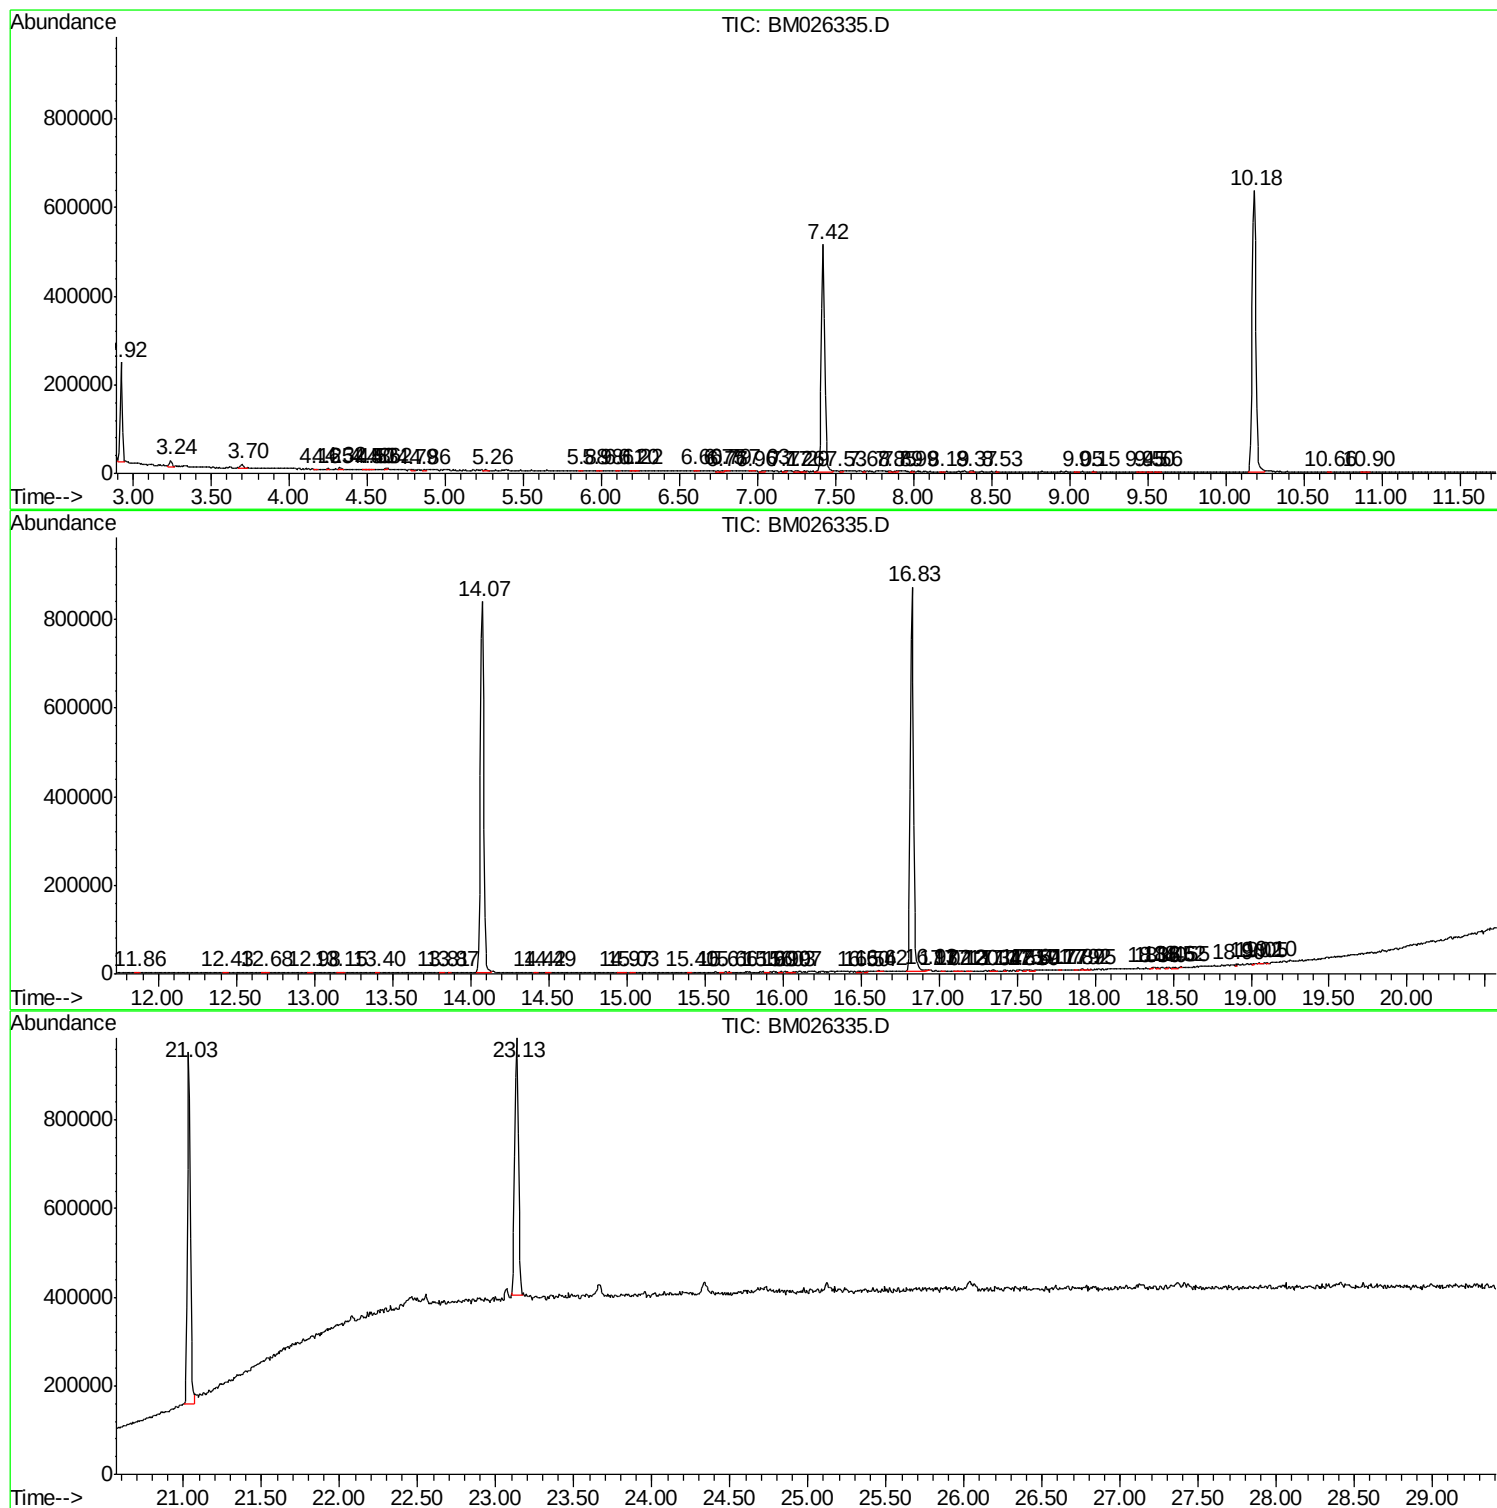

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
Data File : BM026335.D
Acq On : 10 Jun 2020 18:15
Operator : JU/CG
Sample : PB129318BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK18










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.92	5.35 ng/ul	216389	1,4-Dichlorobenzene-d4	7.42

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptane	100	C7H16	000142-82-5	95
2		Heptane	100	C7H16	000142-82-5	90
3		Heptane	100	C7H16	000142-82-5	87
4		Heptane	100	C7H16	000142-82-5	72
5		3-Hexanone, 4-ethyl-	128	C8H16O	006137-12-8	43

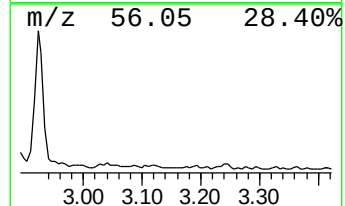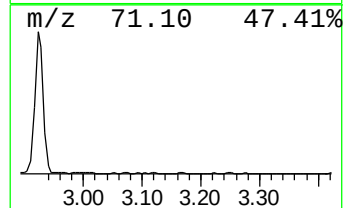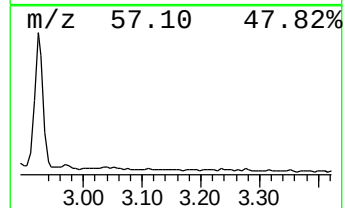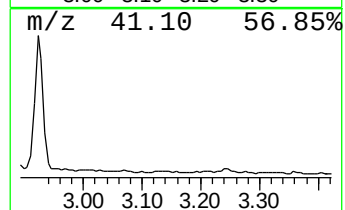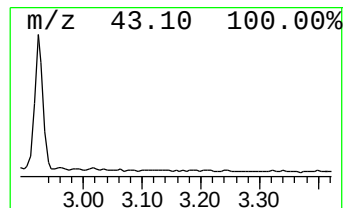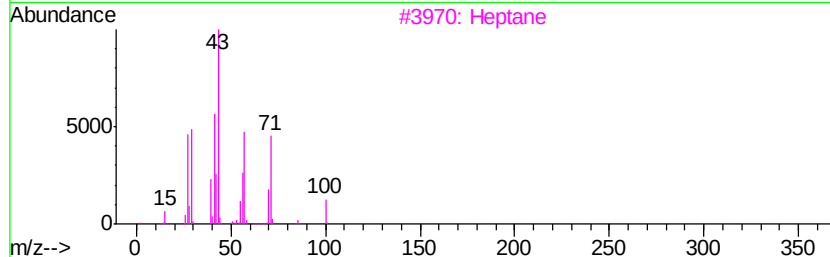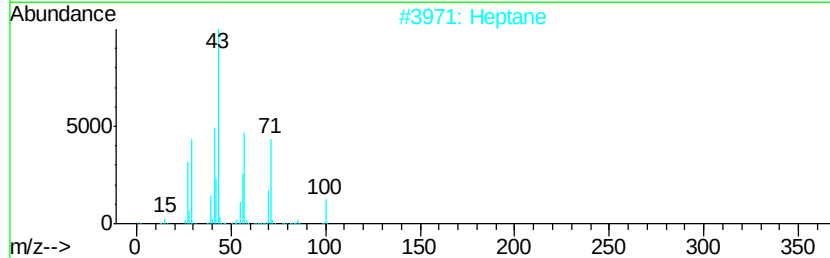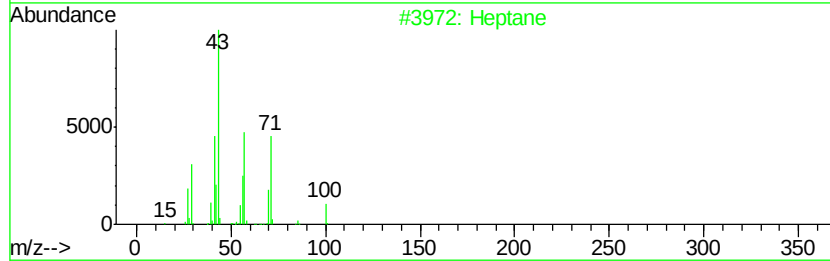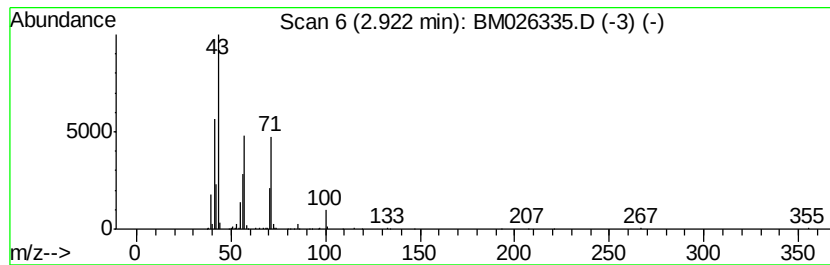

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061020\
Data File : BM026335.D
Acq On : 10 Jun 2020 18:15
Operator : JU/CG
Sample : PB129318BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK18

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	2.92	5.3	ng/ul	216389	1	7.42	808904	20.0