

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026338.D
 Acq On : 10 Jun 2020 20:05
 Operator : JU/CG
 Sample : PB129321BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK21

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.922	3	6	10	rVB	228068	205458	19.88%	3.643%
2	3.240	57	60	64	rVB2	11030	12389	1.20%	0.220%
3	3.416	88	90	92	rVB2	2428	1420	0.14%	0.025%
4	3.693	133	137	141	rBV	8576	12340	1.19%	0.219%
5	3.916	170	175	177	rBV6	2257	2992	0.29%	0.053%
6	4.305	237	241	242	rBV4	2208	2890	0.28%	0.051%
7	4.328	242	245	247	rVB4	2607	2840	0.27%	0.050%
8	4.605	289	292	293	rBV2	2182	2123	0.21%	0.038%
9	4.622	293	295	299	rVV4	2490	3718	0.36%	0.066%
10	4.911	341	344	345	rBV3	2283	1733	0.17%	0.031%
11	5.099	373	376	378	rBV4	1343	1346	0.13%	0.024%
12	5.234	397	399	401	rVB3	1826	1278	0.12%	0.023%
13	5.363	419	421	423	rVB3	1418	1362	0.13%	0.024%
14	5.416	429	430	433	rBV3	2083	1363	0.13%	0.024%
15	5.534	448	450	453	rVV4	1357	1452	0.14%	0.026%
16	5.758	487	488	491	rBV2	1585	1826	0.18%	0.032%
17	5.805	494	496	498	rVV3	1565	1574	0.15%	0.028%
18	5.834	499	501	503	rVB2	1579	1297	0.13%	0.023%
19	5.875	505	508	511	rBV4	1504	1800	0.17%	0.032%
20	6.140	551	553	556	rBV4	2289	2200	0.21%	0.039%
21	6.387	593	595	599	rVV4	1612	1363	0.13%	0.024%
22	6.440	602	604	606	rBV2	1347	1214	0.12%	0.022%
23	6.563	622	625	627	rBV4	1532	1579	0.15%	0.028%
24	6.875	675	678	679	rVB3	1405	1261	0.12%	0.022%
25	6.916	681	685	688	rVB3	1656	1427	0.14%	0.025%
26	7.016	699	702	705	rBV5	1427	2011	0.19%	0.036%
27	7.040	705	706	709	rVB3	1272	1224	0.12%	0.022%
28	7.063	709	710	713	rBV3	1732	1565	0.15%	0.028%
29	7.093	713	715	719	rVB4	1668	1418	0.14%	0.025%
30	7.416	764	770	782	rVV	435250	665316	64.36%	11.796%
31	7.634	806	807	813	rVB5	1162	1642	0.16%	0.029%
32	7.922	853	856	857	rBV3	1533	1337	0.13%	0.024%
33	8.057	877	879	881	rVB2	1874	1761	0.17%	0.031%
34	8.193	898	902	905	rVB3	1453	2111	0.20%	0.037%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026338.D
 Acq On : 10 Jun 2020 20:05
 Operator : JU/CG
 Sample : PB129321BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK21

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	8.246	907	911	913	rBV4	1676	1866	0.18%	0.033%
36	8.593	966	970	974	rBV3	1417	2842	0.27%	0.050%
37	8.722	989	992	995	rBV3	860	1214	0.12%	0.022%
38	8.822	1006	1009	1013	rVB4	819	1398	0.14%	0.025%
39	8.910	1021	1024	1026	rBV4	1393	1507	0.15%	0.027%
40	9.328	1093	1095	1099	rVB4	1215	1505	0.15%	0.027%
41	9.434	1111	1113	1117	rBV3	1837	1557	0.15%	0.028%
42	9.793	1170	1174	1177	rVB4	1135	1453	0.14%	0.026%
43	9.940	1198	1199	1204	rVB2	1118	1287	0.12%	0.023%
44	10.181	1232	1240	1253	rBV	493034	846573	81.90%	15.010%
45	10.445	1281	1285	1286	rBV4	1157	1568	0.15%	0.028%
46	10.604	1310	1312	1313	rBV2	1366	1253	0.12%	0.022%
47	10.716	1329	1331	1336	rBV3	859	1615	0.16%	0.029%
48	10.822	1346	1349	1352	rBV5	1179	1775	0.17%	0.031%
49	10.992	1373	1378	1380	rVB4	1070	1381	0.13%	0.024%
50	11.087	1391	1394	1399	rVB5	1344	2164	0.21%	0.038%
51	11.257	1421	1423	1426	rBV2	1066	1256	0.12%	0.022%
52	11.704	1495	1499	1501	rBV4	834	1312	0.13%	0.023%
53	11.745	1505	1506	1509	rBV3	1119	1263	0.12%	0.022%
54	12.010	1549	1551	1554	rBV3	1387	1613	0.16%	0.029%
55	12.198	1577	1583	1584	rBV5	1234	1606	0.16%	0.028%
56	12.604	1646	1652	1655	rBV4	916	1880	0.18%	0.033%
57	12.663	1659	1662	1666	rBV4	1037	1516	0.15%	0.027%
58	12.775	1678	1681	1683	rBV2	1000	1370	0.13%	0.024%
59	13.139	1740	1743	1744	rBV2	1005	1279	0.12%	0.023%
60	13.163	1746	1747	1750	rVV2	1308	1423	0.14%	0.025%
61	13.233	1754	1759	1760	rVV3	1087	1423	0.14%	0.025%
62	13.251	1760	1762	1765	rVV3	1236	1257	0.12%	0.022%
63	13.292	1765	1769	1770	rVB2	1366	1551	0.15%	0.028%
64	13.345	1775	1778	1781	rBV3	960	1294	0.13%	0.023%
65	13.392	1781	1786	1788	rBV2	1121	1388	0.13%	0.025%
66	13.686	1833	1836	1839	rBV4	1011	1700	0.16%	0.030%
67	14.075	1895	1902	1912	rBV	677559	997307	96.48%	17.683%
68	14.139	1912	1913	1916	rVB2	2777	2363	0.23%	0.042%
69	14.310	1939	1942	1944	rBV2	1112	1228	0.12%	0.022%
70	14.339	1944	1947	1949	rBV4	1521	1457	0.14%	0.026%
71	15.222	2096	2097	2101	rVB3	1600	1616	0.16%	0.029%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026338.D
 Acq On : 10 Jun 2020 20:05
 Operator : JU/CG
 Sample : PB129321BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK21

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

72	15.657	2167	2171	2172	rBV4	1224	1319	0.13%	0.023%
73	15.698	2172	2178	2180	rBV4	1182	1493	0.14%	0.026%
74	15.733	2180	2184	2185	rVB3	1704	1389	0.13%	0.025%
75	15.780	2190	2192	2193	rBV2	1372	1253	0.12%	0.022%
76	16.163	2254	2257	2259	rBV3	1622	1560	0.15%	0.028%
77	16.304	2278	2281	2284	rBV4	1303	2052	0.20%	0.036%
78	16.386	2293	2295	2297	rBV	1468	1494	0.14%	0.026%
79	16.433	2302	2303	2305	rVB2	2116	1244	0.12%	0.022%
80	16.474	2308	2310	2311	rBV	1530	1316	0.13%	0.023%
81	16.616	2331	2334	2336	rBV2	2138	2129	0.21%	0.038%
82	16.710	2347	2350	2352	rBV4	1187	1381	0.13%	0.024%
83	16.827	2364	2370	2381	rBV	728510	1033667	100.00%	18.328%
84	16.939	2387	2389	2392	rVB3	3099	3006	0.29%	0.053%
85	17.127	2418	2421	2422	rBV3	1114	1214	0.12%	0.022%
86	17.292	2447	2449	2452	rBV3	854	1278	0.12%	0.023%
87	17.598	2498	2501	2503	rVB4	2335	2586	0.25%	0.046%
88	17.616	2503	2504	2506	rBV2	1900	1591	0.15%	0.028%
89	17.663	2510	2512	2513	rBV2	1630	1375	0.13%	0.024%
90	17.951	2559	2561	2564	rVB4	1864	1465	0.14%	0.026%
91	17.974	2564	2565	2567	rBV2	2411	1533	0.15%	0.027%
92	18.033	2570	2575	2577	rBV5	2033	2788	0.27%	0.049%
93	18.098	2585	2586	2590	rBV4	2361	2522	0.24%	0.045%
94	18.910	2722	2724	2726	rBV3	2820	2657	0.26%	0.047%
95	19.045	2745	2747	2748	rBV2	2699	1313	0.13%	0.023%
96	19.127	2759	2761	2762	rBV2	3097	1637	0.16%	0.029%
97	19.174	2767	2769	2771	rBV3	4060	4542	0.44%	0.081%
98	19.210	2772	2775	2777	rVV4	7244	7929	0.77%	0.141%
99	21.033	3080	3085	3094	rBV	708489	905790	87.63%	16.060%
100	23.133	3437	3442	3448	rVB	482596	799736	77.37%	14.180%


Sum of corrected areas: 5639949

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
Data File : BM026338.D
Acq On : 10 Jun 2020 20:05
Operator : JU/CG
Sample : PB129321BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK21

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

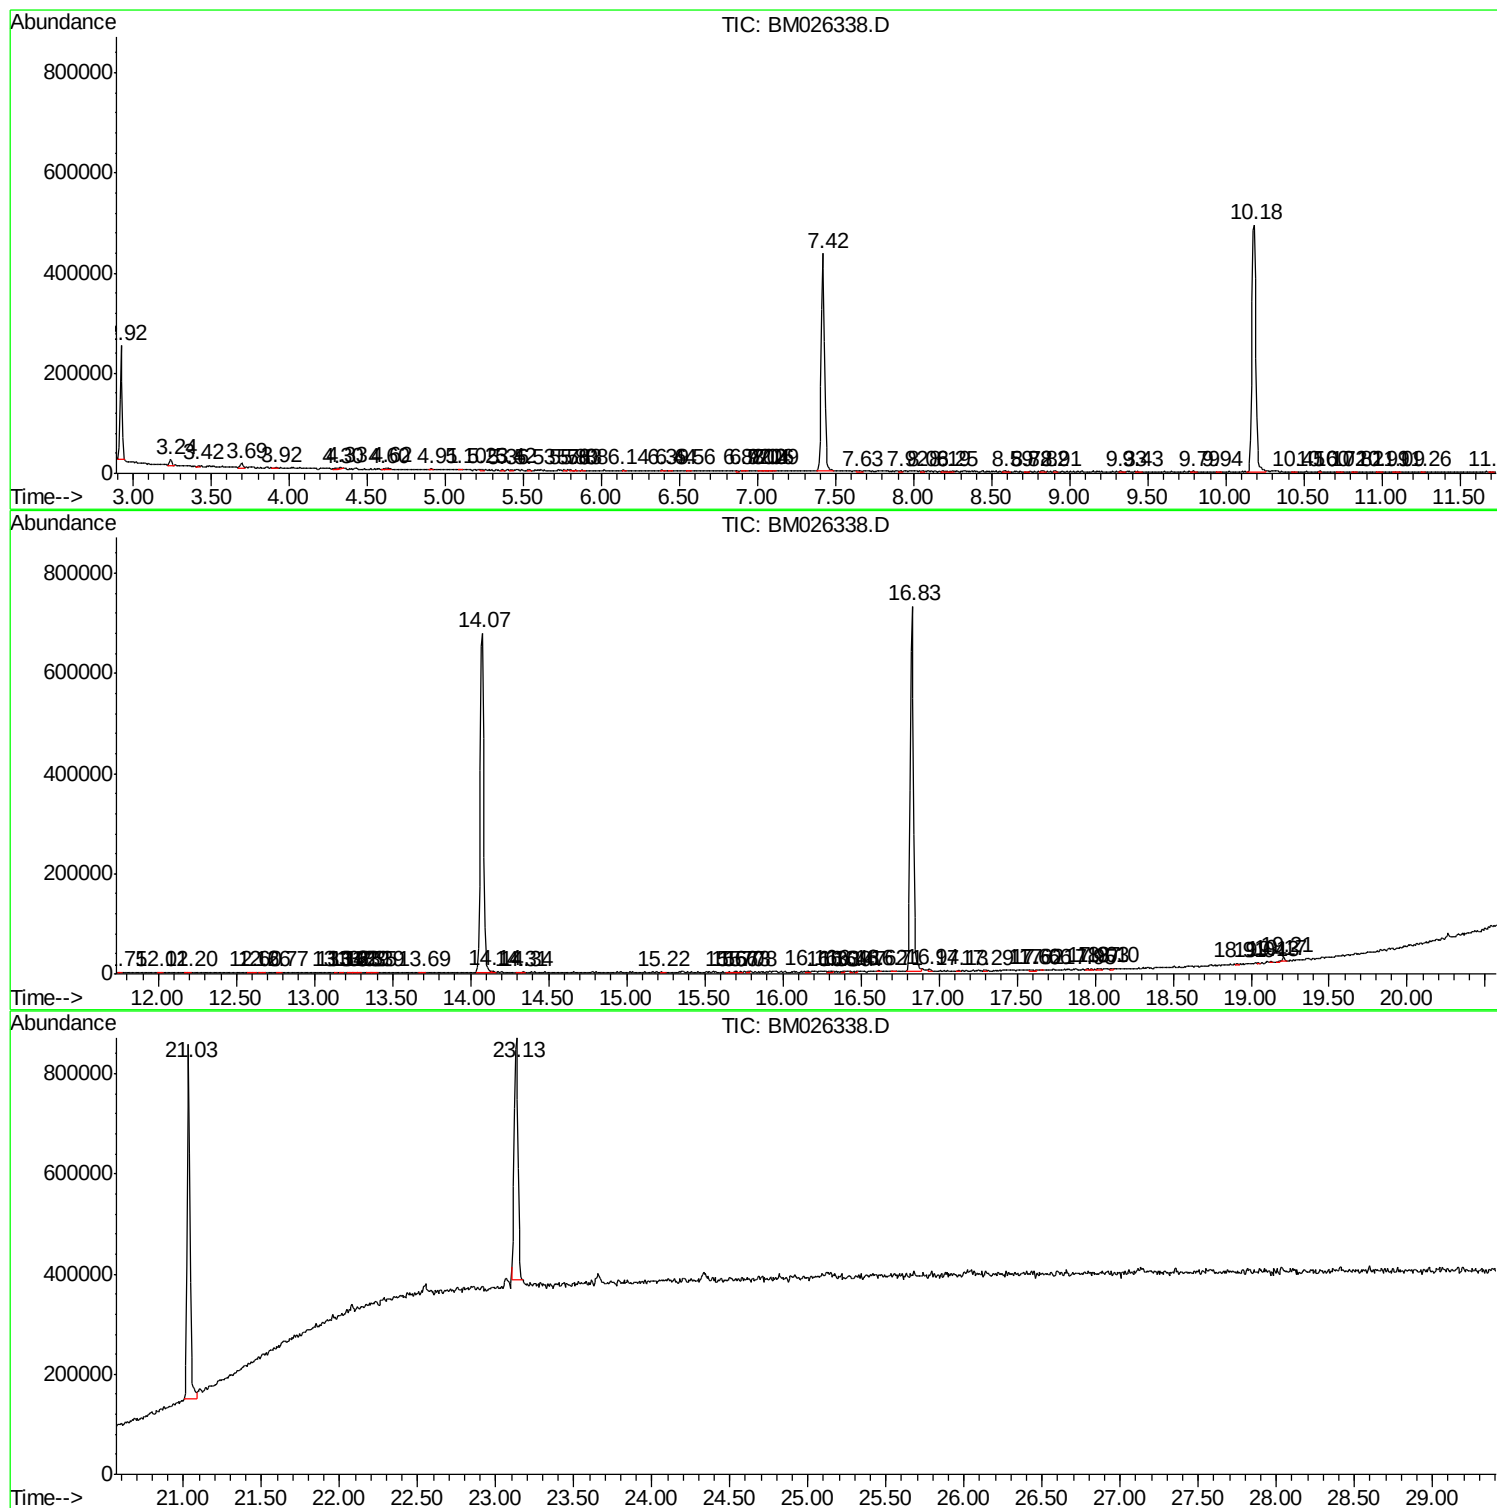

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
Data File : BM026338.D
Acq On : 10 Jun 2020 20:05
Operator : JU/CG
Sample : PB129321BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK21










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.92	6.18 ng/ul	205458	1,4-Dichlorobenzene-d4	7.42

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptane	100	C7H16	000142-82-5	94
2		Heptane	100	C7H16	000142-82-5	90
3		Heptane	100	C7H16	000142-82-5	90
4		Heptane	100	C7H16	000142-82-5	87
5		3-Hexanone, 4-ethyl-	128	C8H16O	006137-12-8	47

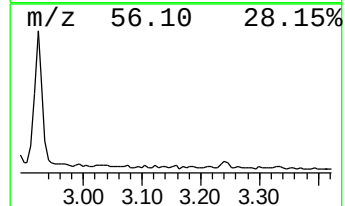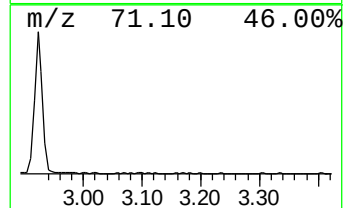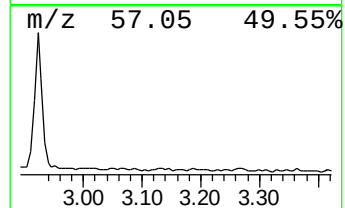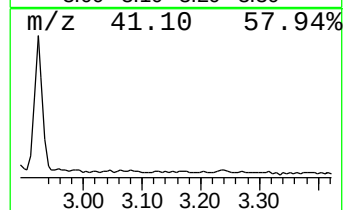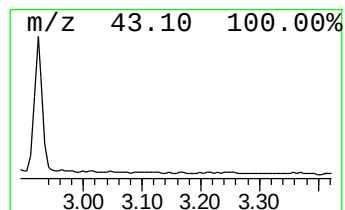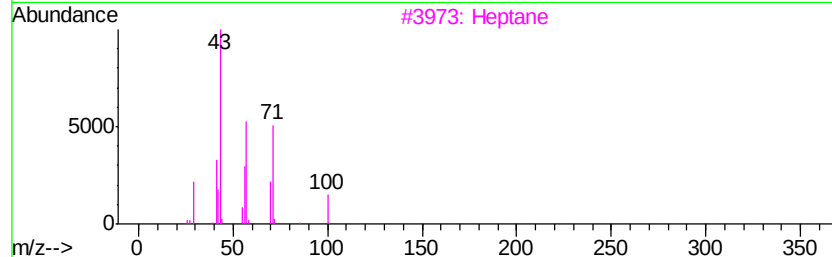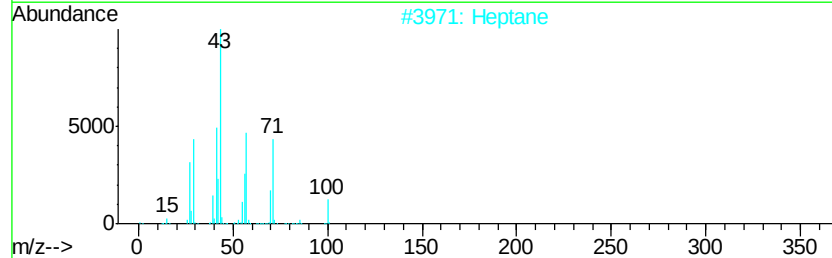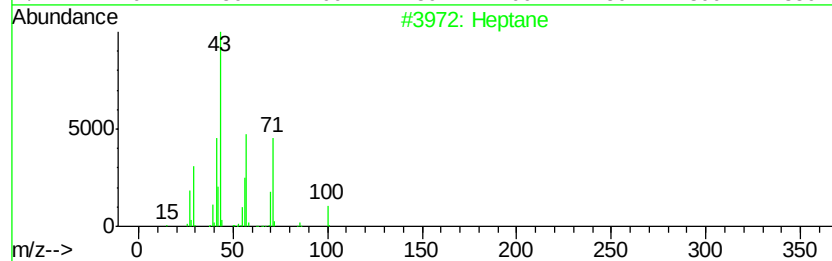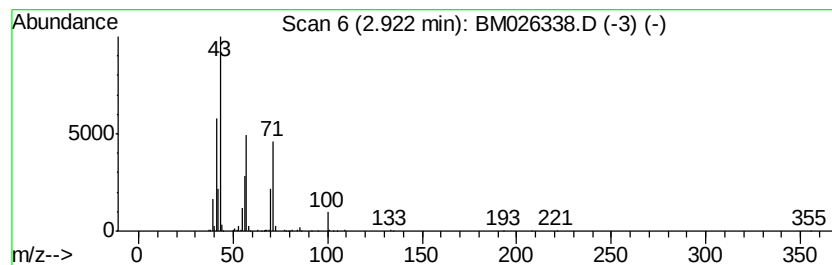

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061020\
Data File : BM026338.D
Acq On : 10 Jun 2020 20:05
Operator : JU/CG
Sample : PB129321BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK21

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	2.92	6.2	ng/ul	205458	1	7.42	665316	20.0