

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026339.D
 Acq On : 10 Jun 2020 20:42
 Operator : JU/CG
 Sample : PB129357BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.922	3	6	10	rVB	227203	210716	23.14%	4.131%
2	3.240	57	60	65	rVB3	11909	15407	1.69%	0.302%
3	3.299	68	70	73	rVB4	2688	2066	0.23%	0.040%
4	3.416	88	90	91	rBV2	1949	1801	0.20%	0.035%
5	3.699	134	138	142	rBV2	8180	9433	1.04%	0.185%
6	3.963	181	183	186	rBV4	1466	1892	0.21%	0.037%
7	4.099	204	206	208	rVB3	1767	1288	0.14%	0.025%
8	4.128	210	211	218	rVB5	2157	3476	0.38%	0.068%
9	4.222	224	227	228	rBV3	2087	1877	0.21%	0.037%
10	4.322	242	244	251	rVB7	3325	4185	0.46%	0.082%
11	4.451	264	266	269	rVB4	1851	1219	0.13%	0.024%
12	4.475	269	270	273	rBV2	1935	1670	0.18%	0.033%
13	4.575	285	287	288	rBV2	1814	1387	0.15%	0.027%
14	4.622	291	295	296	rBV5	3464	4006	0.44%	0.079%
15	4.751	315	317	319	rBV3	1855	1352	0.15%	0.027%
16	4.857	333	335	338	rVV4	1407	1319	0.14%	0.026%
17	5.069	369	371	373	rVB2	1852	1339	0.15%	0.026%
18	5.093	373	375	378	rBV4	1667	1611	0.18%	0.032%
19	5.263	402	404	405	rBV2	1677	1181	0.13%	0.023%
20	5.328	414	415	417	rVB2	1798	1247	0.14%	0.024%
21	5.357	417	420	421	rBV3	1311	1432	0.16%	0.028%
22	5.528	446	449	451	rBV3	1151	1234	0.14%	0.024%
23	5.581	456	458	462	rVV3	1625	2334	0.26%	0.046%
24	5.622	464	465	469	rVV3	1359	1626	0.18%	0.032%
25	5.657	469	471	472	rVV2	2195	1584	0.17%	0.031%
26	5.693	475	477	480	rVB3	1616	1522	0.17%	0.030%
27	5.916	512	515	517	rBV4	1254	1334	0.15%	0.026%
28	6.063	537	540	541	rVB3	1985	1552	0.17%	0.030%
29	6.257	571	573	575	rBV3	1656	1203	0.13%	0.024%
30	6.610	631	633	635	rVB3	1722	1479	0.16%	0.029%
31	6.634	635	637	641	rBV4	1507	2347	0.26%	0.046%
32	6.969	691	694	697	rVB4	1495	1855	0.20%	0.036%
33	7.004	697	700	703	rBV4	1524	2397	0.26%	0.047%
34	7.040	703	706	708	rVV3	1356	1950	0.21%	0.038%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026339.D
 Acq On : 10 Jun 2020 20:42
 Operator : JU/CG
 Sample : PB129357BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	7.093	710	715	717	rBV5	1352	1891	0.21%	0.037%
36	7.110	717	718	723	rVV5	1060	1426	0.16%	0.028%
37	7.192	729	732	735	rVB3	1108	1307	0.14%	0.026%
38	7.351	755	759	762	rVB4	1378	1692	0.19%	0.033%
39	7.416	762	770	781	rBV	391402	605910	66.55%	11.877%
40	7.528	786	789	791	rBV4	1559	1788	0.20%	0.035%
41	7.951	857	861	862	rBV	1608	1386	0.15%	0.027%
42	8.016	870	872	875	rBV4	1123	1182	0.13%	0.023%
43	8.057	878	879	882	rVV3	1589	1354	0.15%	0.027%
44	8.334	923	926	929	rBV3	1047	1337	0.15%	0.026%
45	9.316	1090	1093	1096	rVV4	1213	1715	0.19%	0.034%
46	9.869	1184	1187	1190	rVB5	1127	1184	0.13%	0.023%
47	9.963	1201	1203	1208	rVB5	1164	1554	0.17%	0.030%
48	10.022	1208	1213	1216	rBV4	1122	1833	0.20%	0.036%
49	10.181	1233	1240	1255	rBV	451329	771760	84.77%	15.128%
50	10.275	1255	1256	1260	rVB3	2115	1379	0.15%	0.027%
51	10.592	1305	1310	1312	rBV5	827	1231	0.14%	0.024%
52	11.098	1391	1396	1399	rBV5	969	1790	0.20%	0.035%
53	11.269	1422	1425	1427	rVB3	1141	1254	0.14%	0.025%
54	11.410	1446	1449	1452	rVB2	1374	1252	0.14%	0.025%
55	11.916	1533	1535	1539	rVB3	1163	1270	0.14%	0.025%
56	12.004	1547	1550	1553	rBV2	1620	1715	0.19%	0.034%
57	12.339	1603	1607	1610	rBV4	1359	1731	0.19%	0.034%
58	12.669	1659	1663	1665	rBV3	1420	1249	0.14%	0.024%
59	12.810	1684	1687	1689	rVB4	1162	1476	0.16%	0.029%
60	13.286	1764	1768	1769	rBV2	1018	1306	0.14%	0.026%
61	13.310	1769	1772	1774	rVV2	1617	1302	0.14%	0.026%
62	13.386	1780	1785	1786	rBV3	930	1486	0.16%	0.029%
63	13.669	1829	1833	1838	rBV5	974	1847	0.20%	0.036%
64	13.745	1841	1846	1848	rBV3	683	1283	0.14%	0.025%
65	14.074	1895	1902	1913	rBV	577207	881069	96.77%	17.271%
66	14.180	1918	1920	1922	rVV2	1688	1375	0.15%	0.027%
67	14.304	1938	1941	1942	rBV3	1193	1333	0.15%	0.026%
68	14.357	1948	1950	1953	rVB3	1762	1209	0.13%	0.024%
69	14.533	1975	1980	1982	rBV3	690	1213	0.13%	0.024%
70	14.651	1997	2000	2003	rBV3	1325	1856	0.20%	0.036%
71	14.851	2032	2034	2038	rBV2	1561	2058	0.23%	0.040%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
 Data File : BM026339.D
 Acq On : 10 Jun 2020 20:42
 Operator : JU/CG
 Sample : PB129357BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

72	15.768	2186	2190	2191	rVV4	1116	1247	0.14%	0.024%
73	15.833	2196	2201	2204	rVB6	1427	1850	0.20%	0.036%
74	16.039	2233	2236	2241	rBV6	1224	1555	0.17%	0.030%
75	16.621	2329	2335	2337	rBV4	2742	3959	0.43%	0.078%
76	16.674	2340	2344	2346	rBV5	1463	1810	0.20%	0.035%
77	16.827	2363	2370	2384	rVV	622578	910439	100.00%	17.847%
78	16.939	2388	2389	2393	rVB3	2321	1968	0.22%	0.039%
79	17.280	2443	2447	2448	rBV3	1328	1664	0.18%	0.033%
80	17.292	2448	2449	2452	rVB2	2053	1738	0.19%	0.034%
81	17.327	2452	2455	2458	rBV4	1342	2039	0.22%	0.040%
82	17.351	2458	2459	2462	rBV3	1579	1294	0.14%	0.025%
83	17.386	2462	2465	2467	rBV4	1728	1993	0.22%	0.039%
84	17.415	2467	2470	2472	rBV3	1271	1237	0.14%	0.024%
85	17.621	2502	2505	2508	rBV4	1796	2641	0.29%	0.052%
86	17.680	2513	2515	2517	rVB2	2054	1655	0.18%	0.032%
87	17.704	2517	2519	2520	rBV	1700	1294	0.14%	0.025%
88	17.762	2526	2529	2530	rBV3	2364	2128	0.23%	0.042%
89	17.968	2562	2564	2566	rBV3	1635	1665	0.18%	0.033%
90	18.027	2573	2574	2576	rVB2	2201	1497	0.16%	0.029%
91	18.051	2576	2578	2579	rBV	1615	1205	0.13%	0.024%
92	18.168	2596	2598	2601	rBV4	1892	1503	0.17%	0.029%
93	18.192	2601	2602	2605	rBV2	1923	1540	0.17%	0.030%
94	18.239	2608	2610	2611	rBV2	1624	1435	0.16%	0.028%
95	18.480	2649	2651	2652	rBV2	1518	1226	0.13%	0.024%
96	18.545	2660	2662	2664	rVB3	2519	1551	0.17%	0.030%
97	18.980	2734	2736	2737	rVB2	2518	1235	0.14%	0.024%
98	19.015	2740	2742	2746	rBV4	3360	4245	0.47%	0.083%
99	21.033	3080	3085	3093	rBV	612372	813221	89.32%	15.941%
100	23.127	3437	3441	3448	rVB	443632	729229	80.10%	14.295%


Sum of corrected areas: 5101387

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
Data File : BM026339.D
Acq On : 10 Jun 2020 20:42
Operator : JU/CG
Sample : PB129357BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

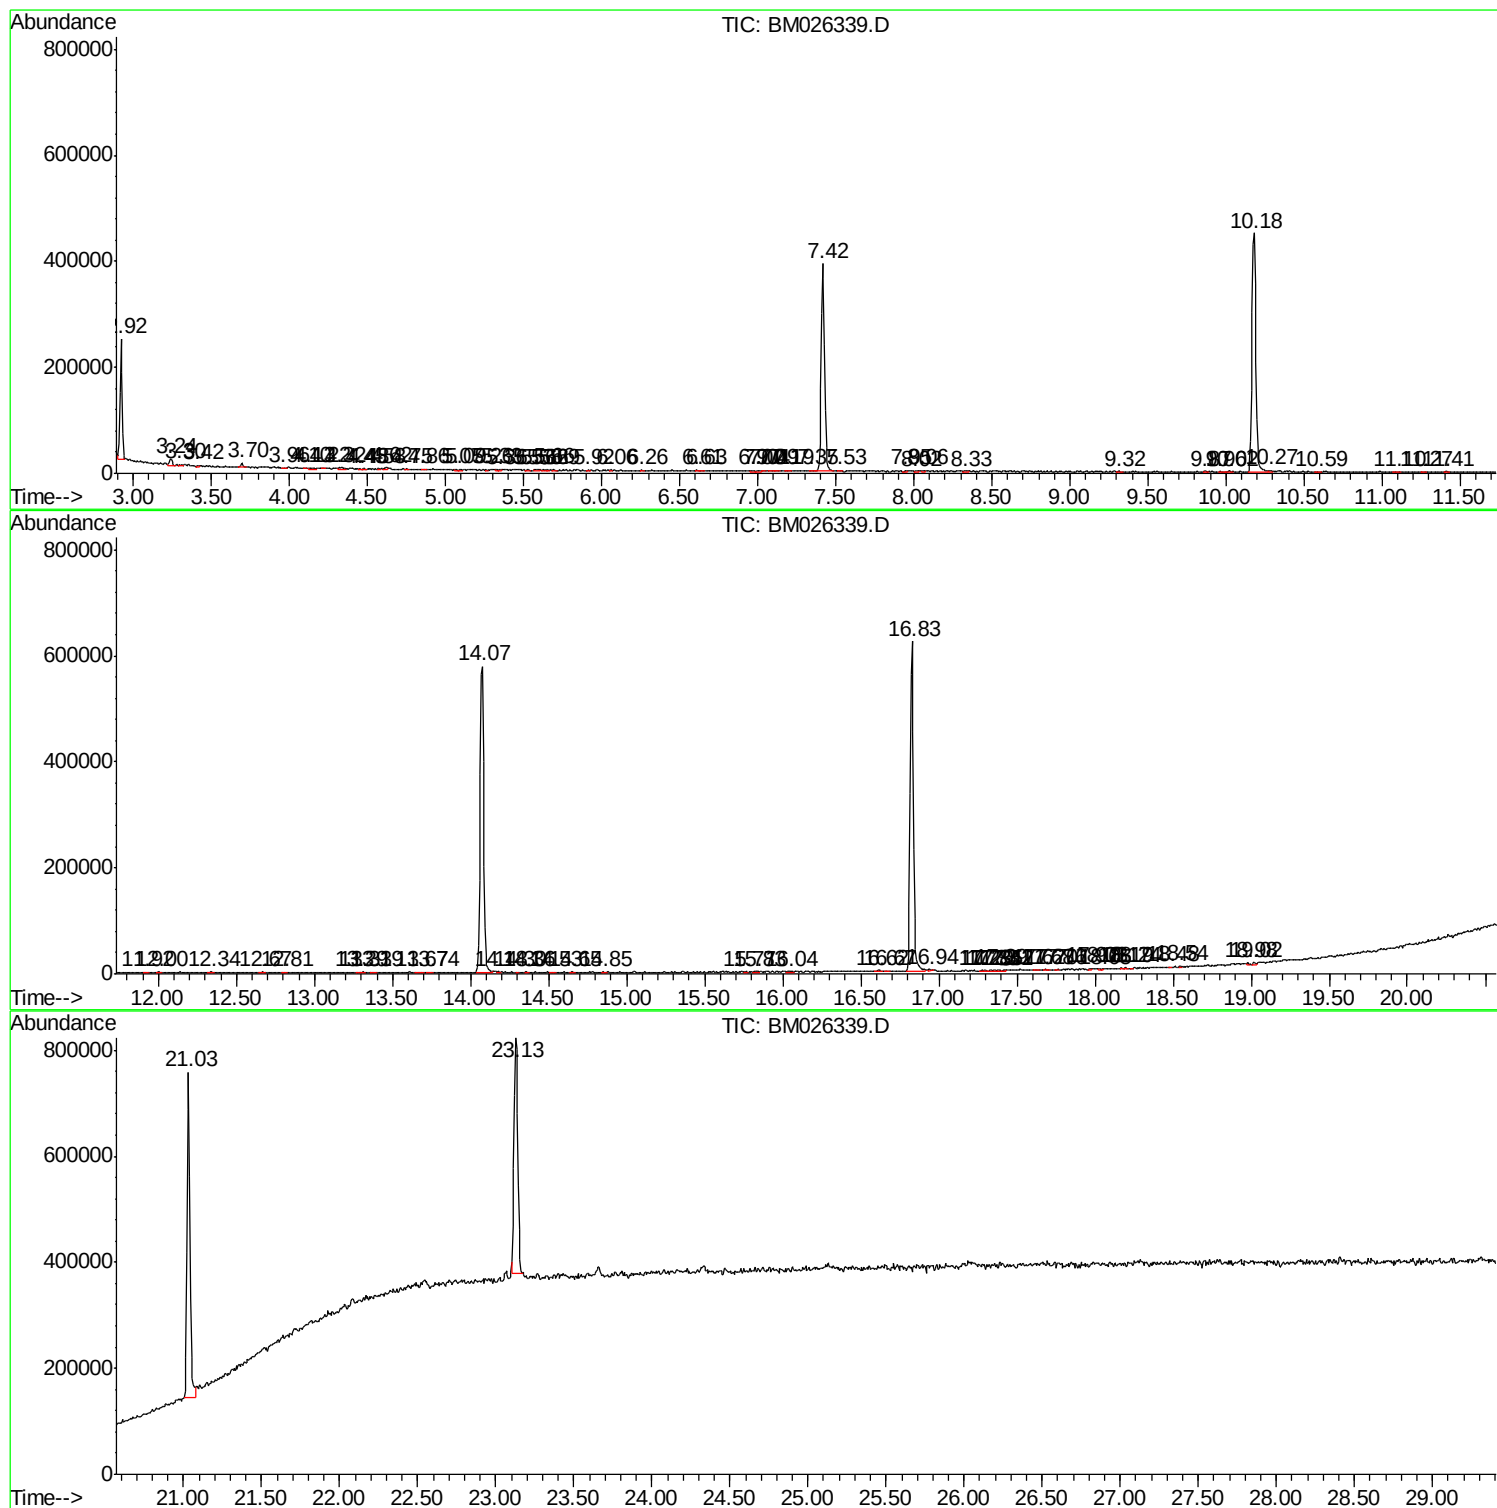

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061020\
Data File : BM026339.D
Acq On : 10 Jun 2020 20:42
Operator : JU/CG
Sample : PB129357BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.92	6.96 ng/ul	210716	1,4-Dichlorobenzene-d4	7.42

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptane	100	C7H16	000142-82-5	95
2		Heptane	100	C7H16	000142-82-5	91
3		Heptane	100	C7H16	000142-82-5	91
4		Heptane	100	C7H16	000142-82-5	72
5		Hexane, 3-methyl-	100	C7H16	000589-34-4	50

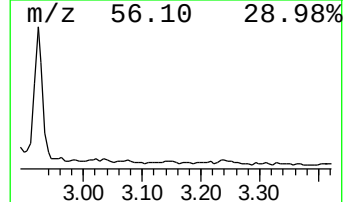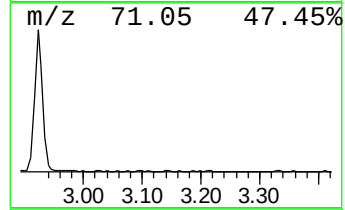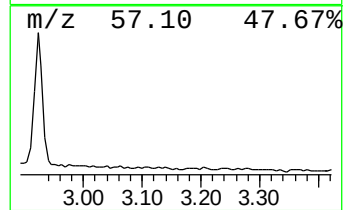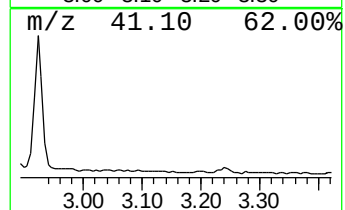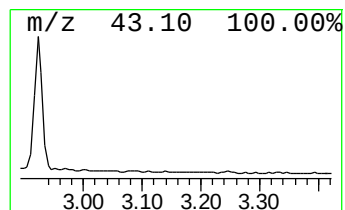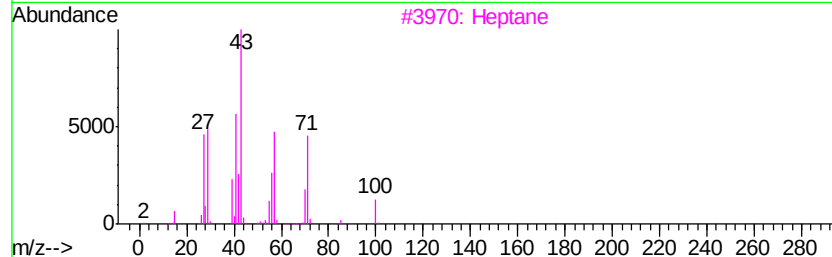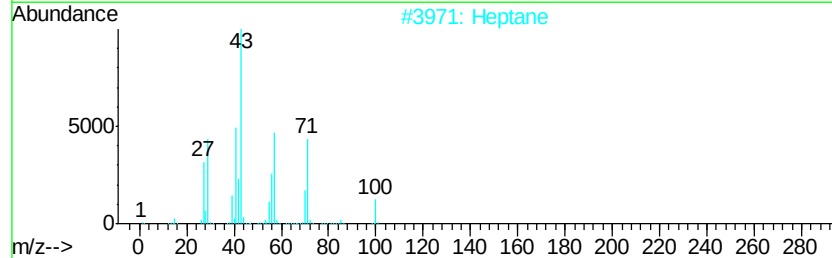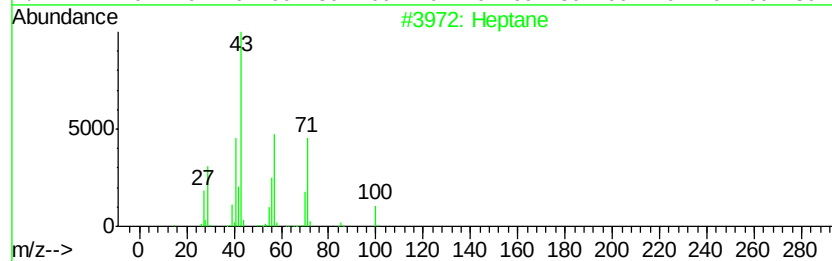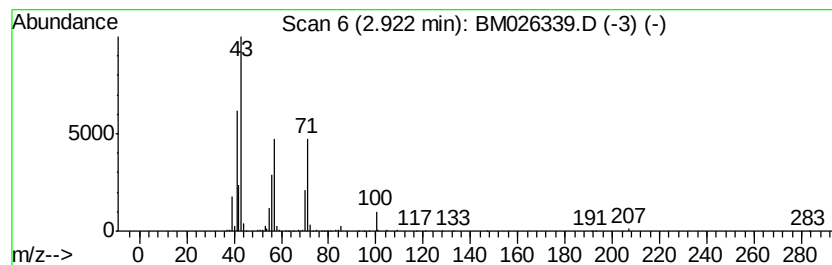

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061020\
Data File : BM026339.D
Acq On : 10 Jun 2020 20:42
Operator : JU/CG
Sample : PB129357BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	2.92	7.0	ng/ul	210716	1	7.42	605910	20.0