
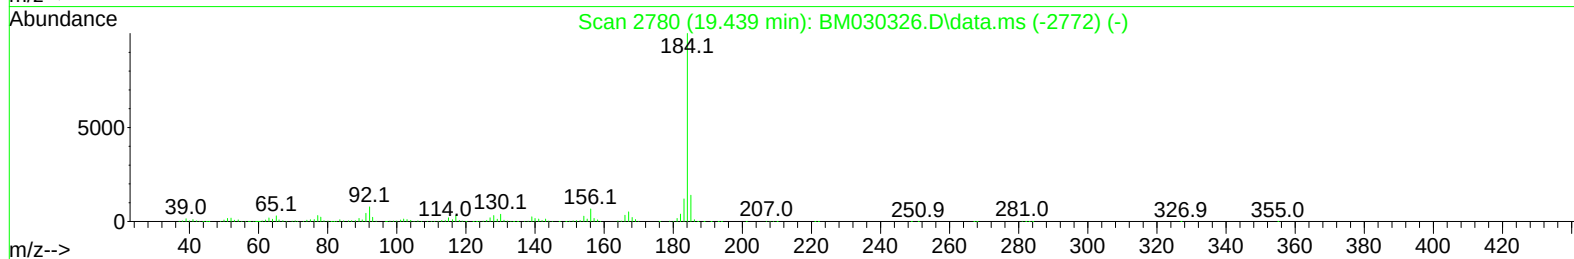
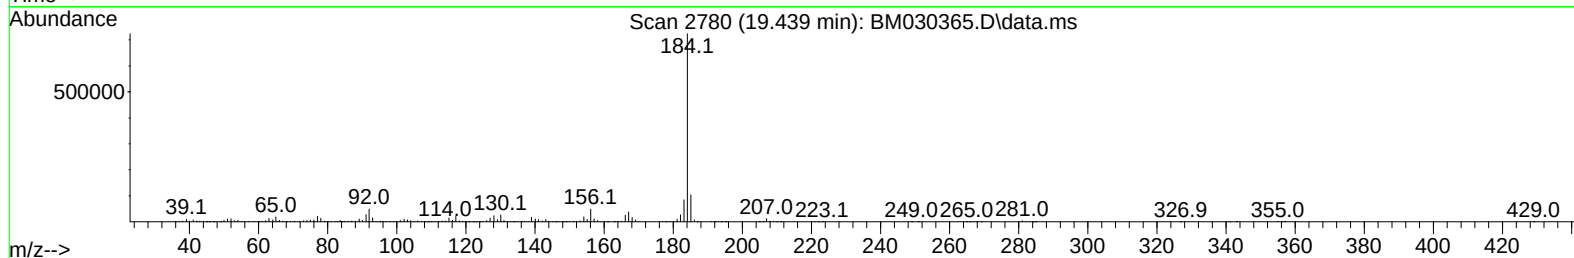


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061021\
Data File : BM030365.D
Acq On : 10 Jun 2021 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 10:33:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 08 20:51:08 2021
Response via : Initial Calibration

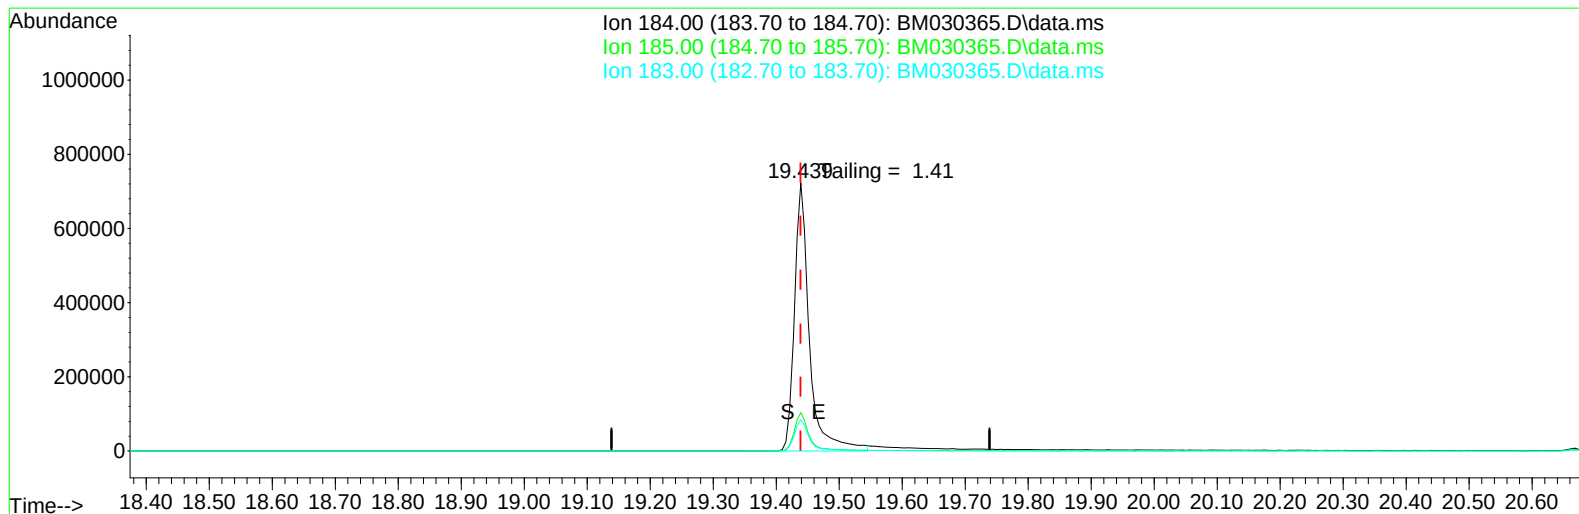

TIC: BM030365.D\data.ms

(77) Benzidine




19.439min (+ 0.000) 1295701.43 ng

response 1260904

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.35
183.00	12.30	11.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061021\
Data File : BM030365.D
Acq On : 10 Jun 2021 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 10:33:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 08 20:51:08 2021
Response via : Initial Calibration

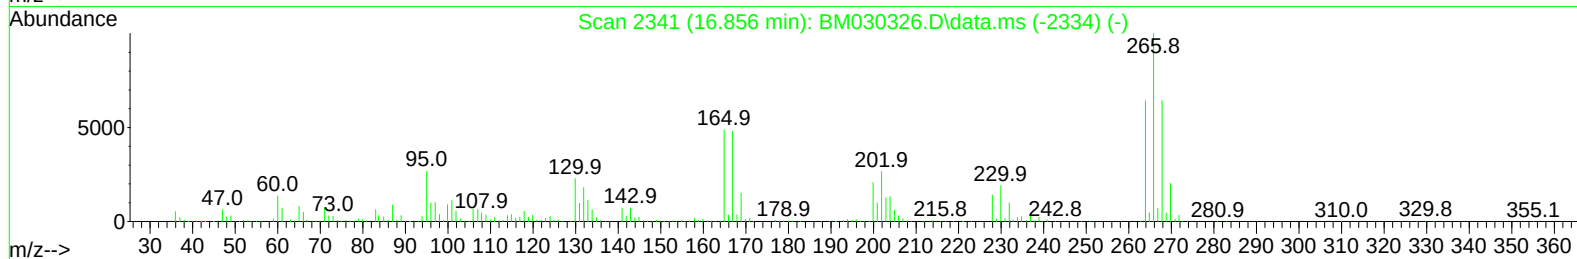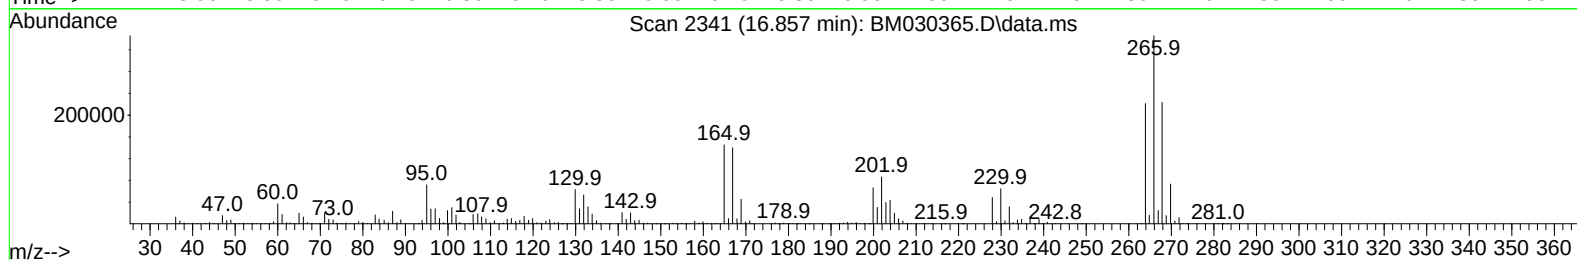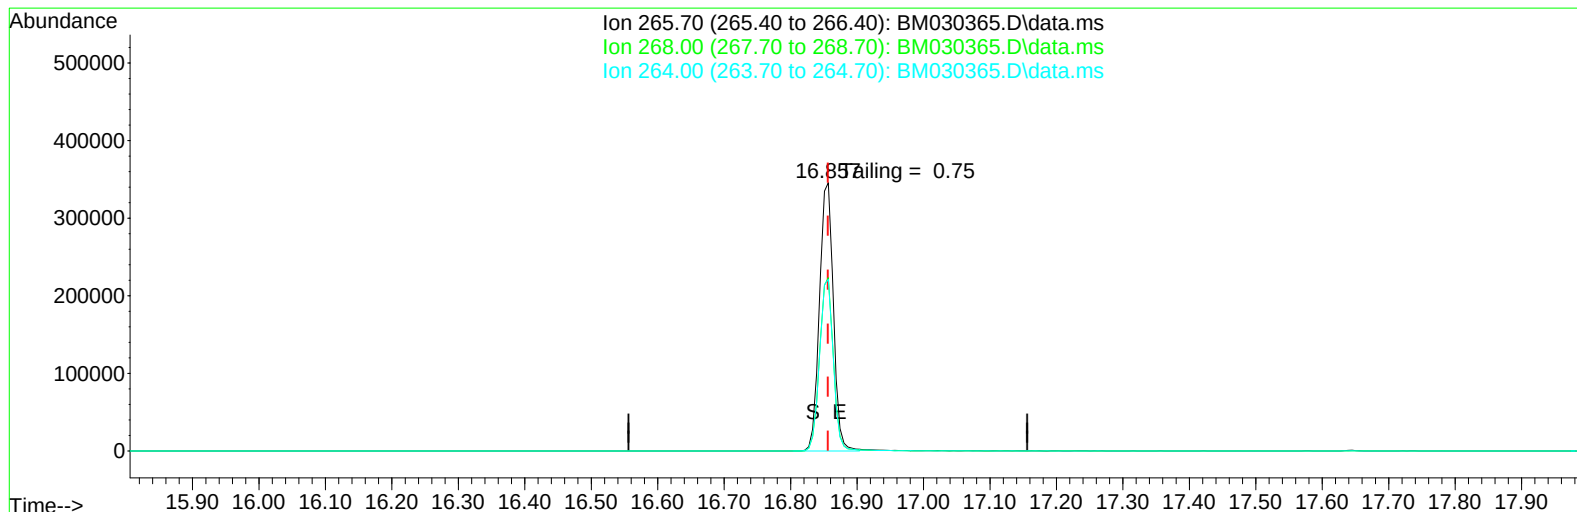

TIC: BM030365.D\data.ms

(70) Pentachlorophenol (C)

16.857min (+ 0.001) 850138.18 ng

response 506267

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.60
264.00	64.90	63.92
0.00	0.00	0.00